


Data Path : Z:\HPCHEM1\BNA G\DATA\BG061417\
 Data File : BG027415.D
 Acq On : 14 Jun 2017 13:33
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 14 19:09:08 2017

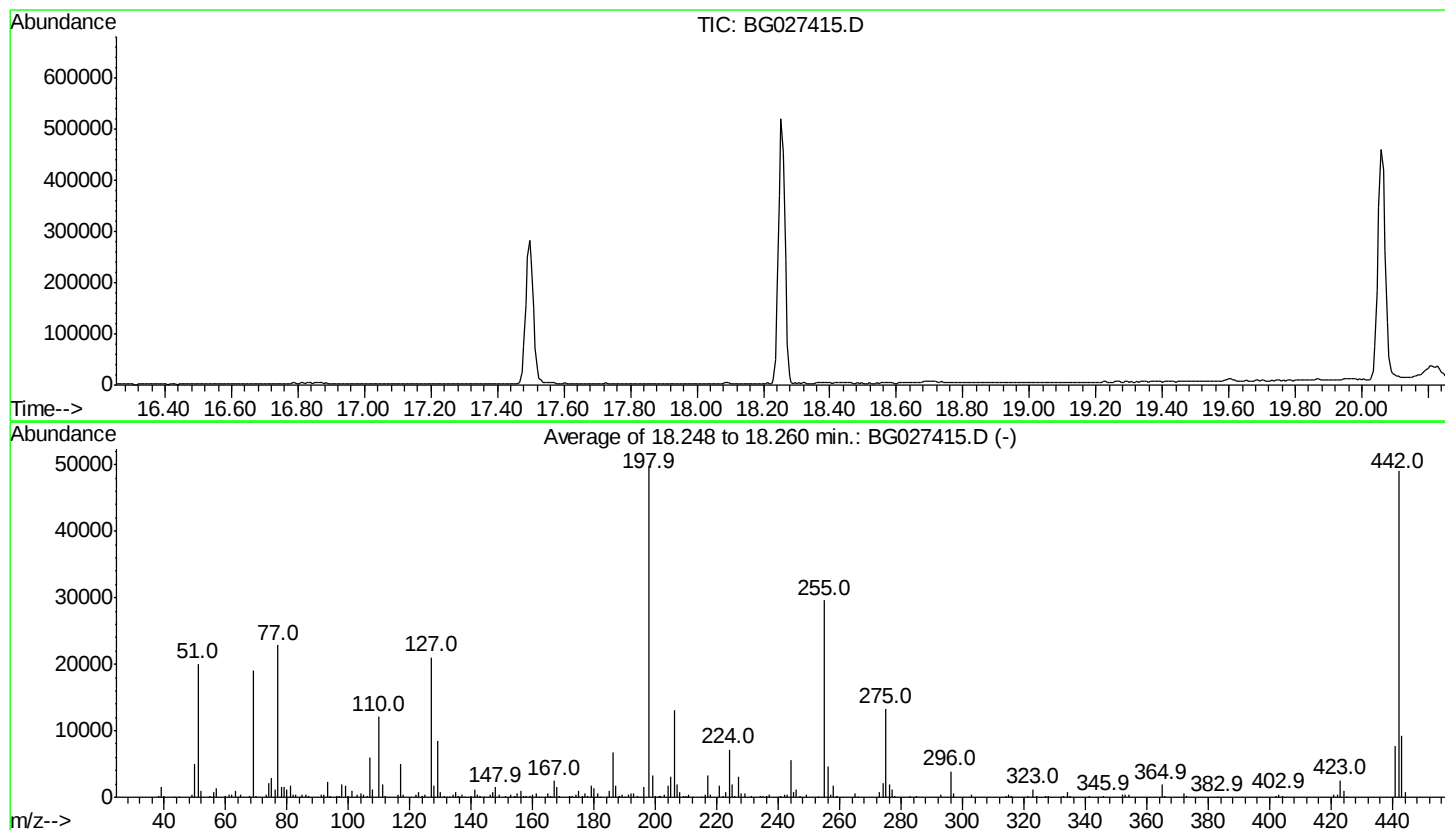

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	20125	PASS
68	69	0.00	2	0.7	138	PASS
69	198	0.00	100	38.4	19130	PASS
70	69	0.00	2	0.6	111	PASS
127	198	10	80	42.2	21056	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49874	PASS
199	198	5	9	6.7	3332	PASS
275	198	10	60	26.7	13301	PASS
365	198	1	100	3.9	1924	PASS
441	442	0.01	24	15.8	7756	PASS
442	198	50	100	98.5	49109	PASS
443	442	15	24	18.8	9222	PASS