


Data Path : Z:\HPCHEM1\BNA G\DATA\BG061417\
 Data File : BG027433.D
 Acq On : 15 Jun 2017 2:06
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 14 19:09:08 2017

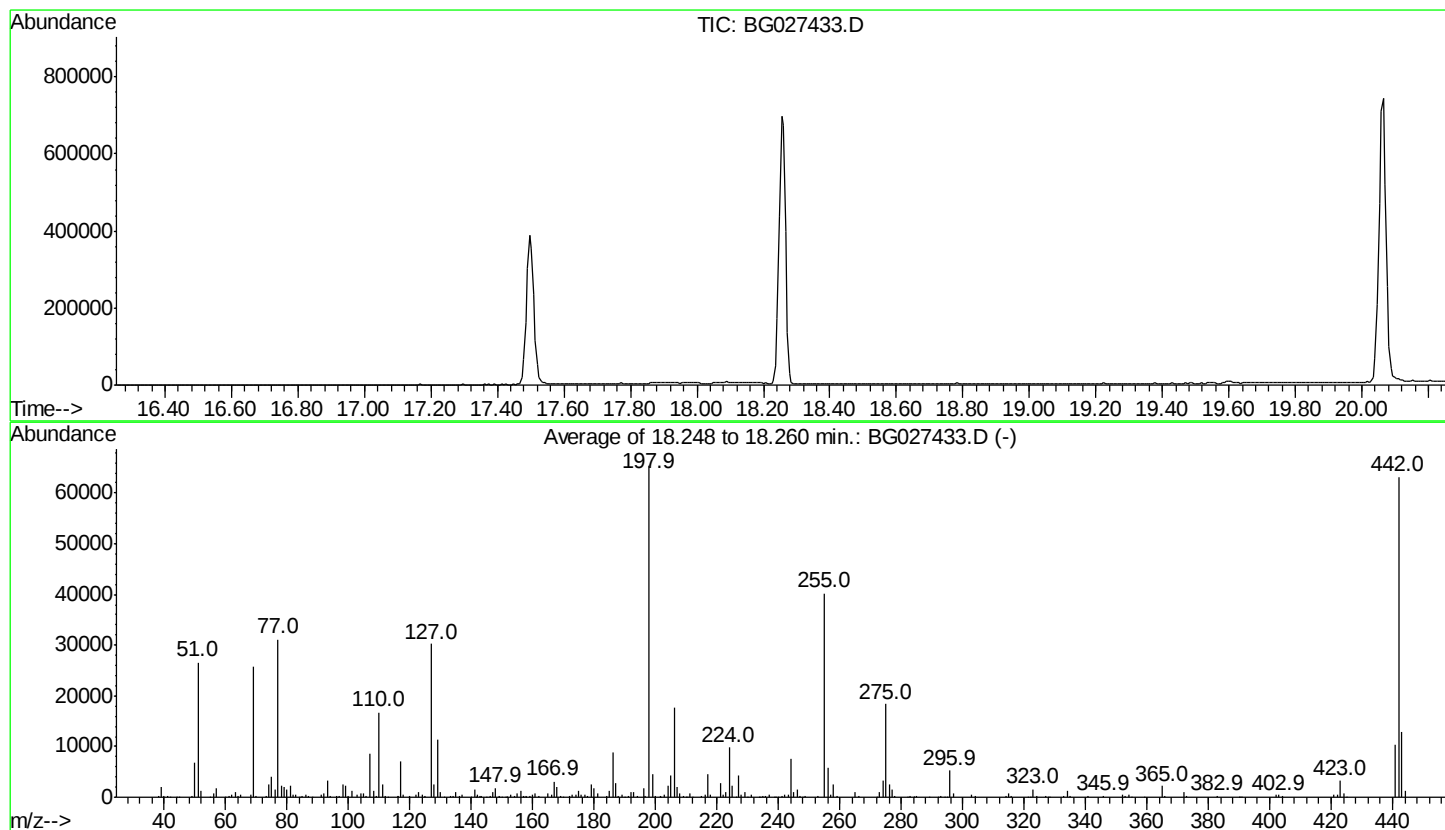

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	26621	PASS
68	69	0.00	2	1.5	399	PASS
69	198	0.00	100	39.5	25848	PASS
70	69	0.00	2	0.7	180	PASS
127	198	10	80	46.3	30258	PASS
197	198	0.00	2	0.3	172	PASS
198	198	100	100	100.0	65408	PASS
199	198	5	9	7.0	4576	PASS
275	198	10	60	28.0	18324	PASS
365	198	1	100	3.4	2232	PASS
441	442	0.01	24	16.4	10356	PASS
442	198	50	100	96.6	63210	PASS
443	442	15	24	20.6	13008	PASS