
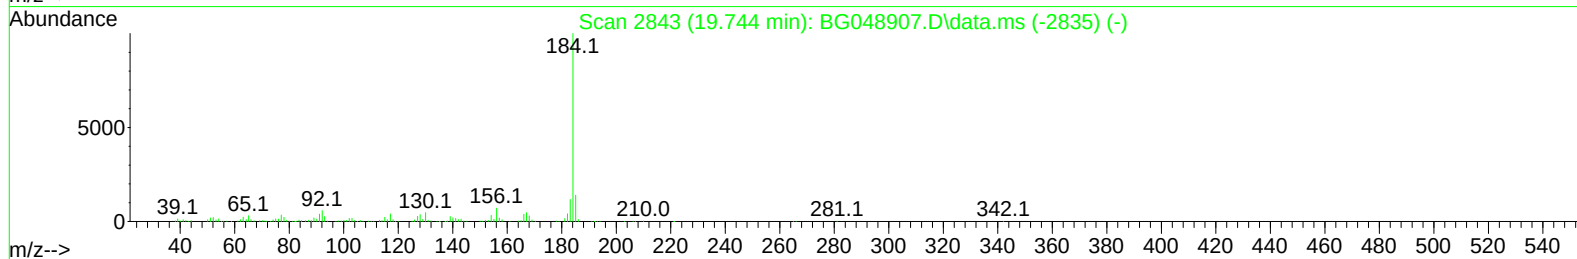
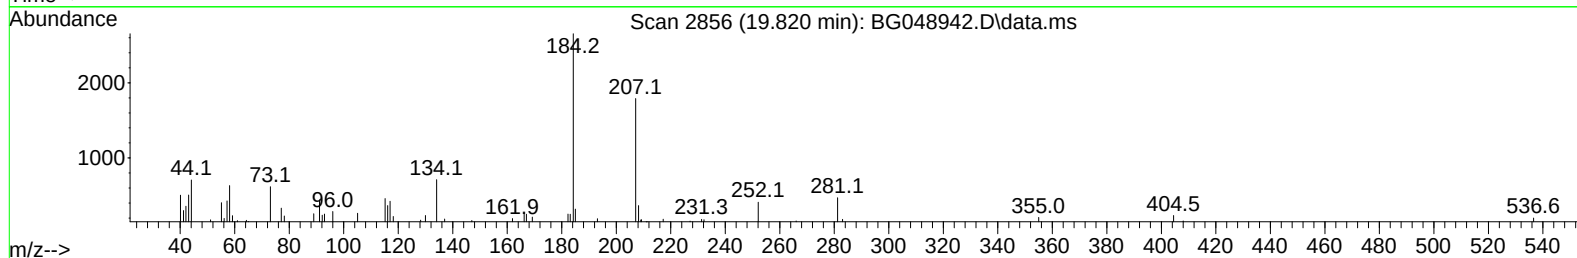


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061421\
Data File : BG048942.D
Acq On : 14 Jun 2021 9:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 14 10:50:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

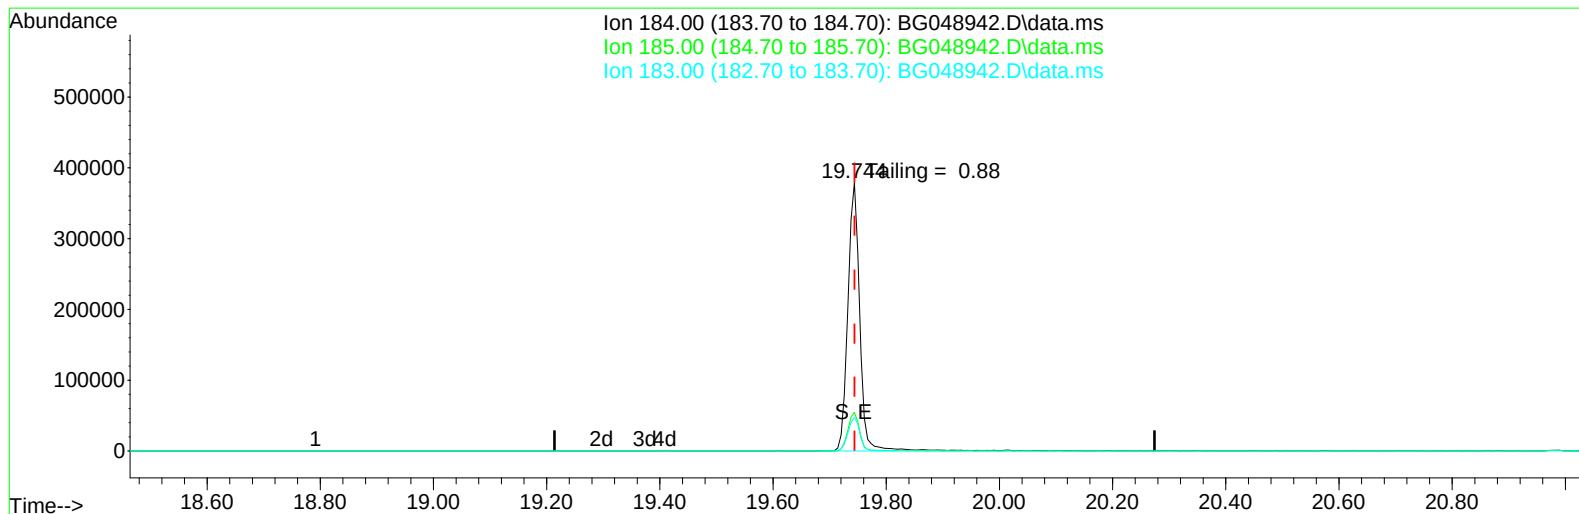

TIC: BG048942.D\data.ms

(77) Benzidine




19.744min (-0.000) 7917.46 ng m

response 548988

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.39
183.00	11.70	12.57
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061421\  
Data File : BG048942.D  
Acq On    : 14 Jun 2021    9:55  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jun 14 10:50:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

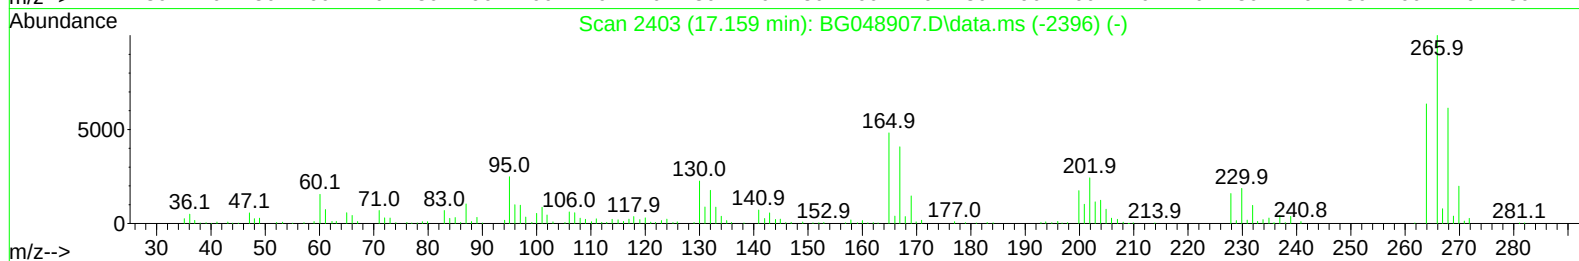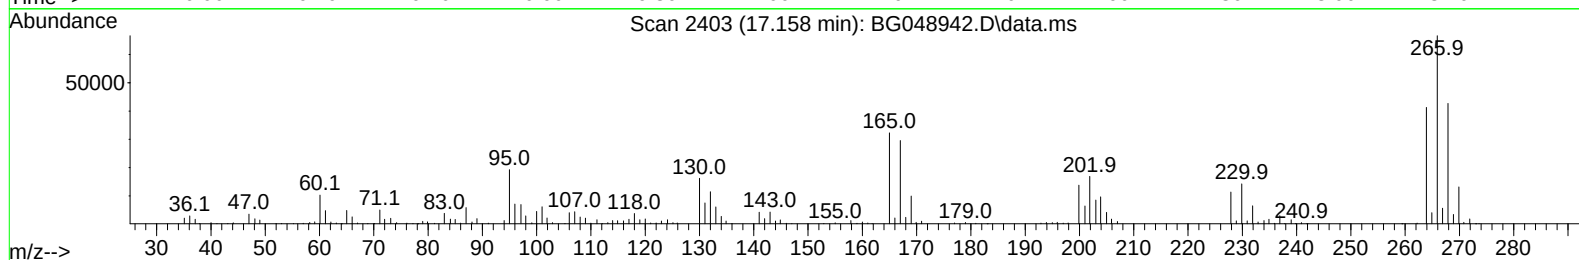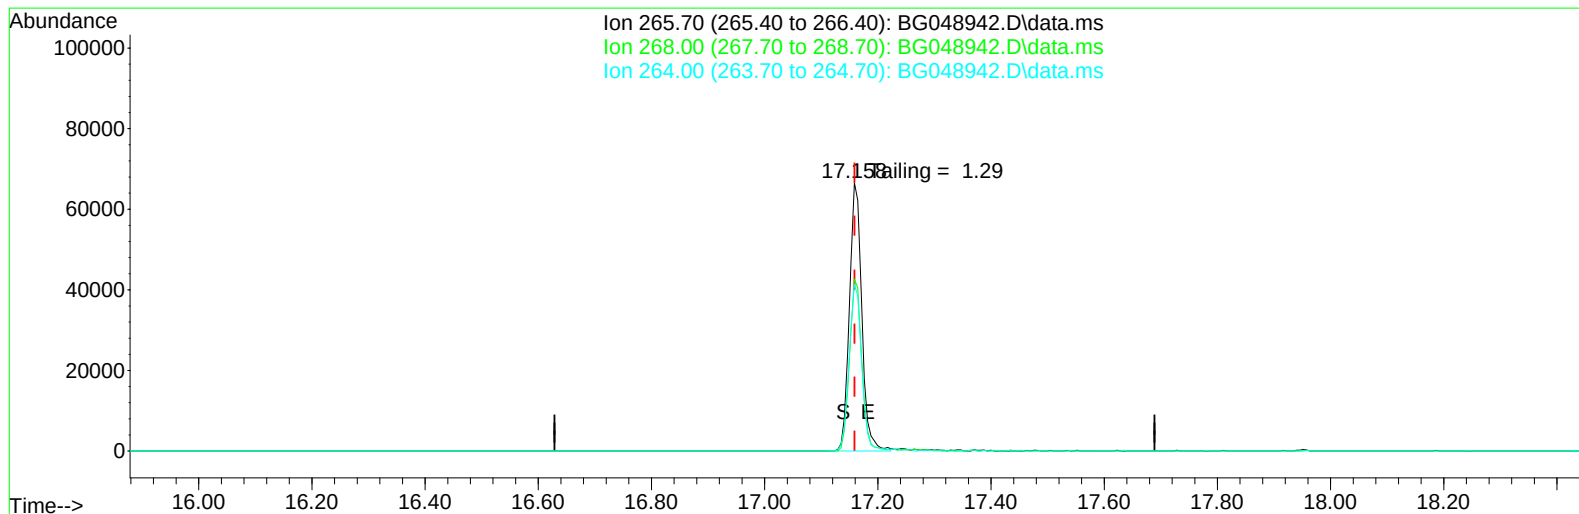

TIC: BG048942.D\data.ms

(70) Pentachlorophenol (C)

17.158min (-0.000) 173355.83 ng

response **97285**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.06
264.00	61.30	61.99
0.00	0.00	0.00