


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061421\
 Data File : BG048942.D
 Acq On : 14 Jun 2021 9:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 16:03:10 2021

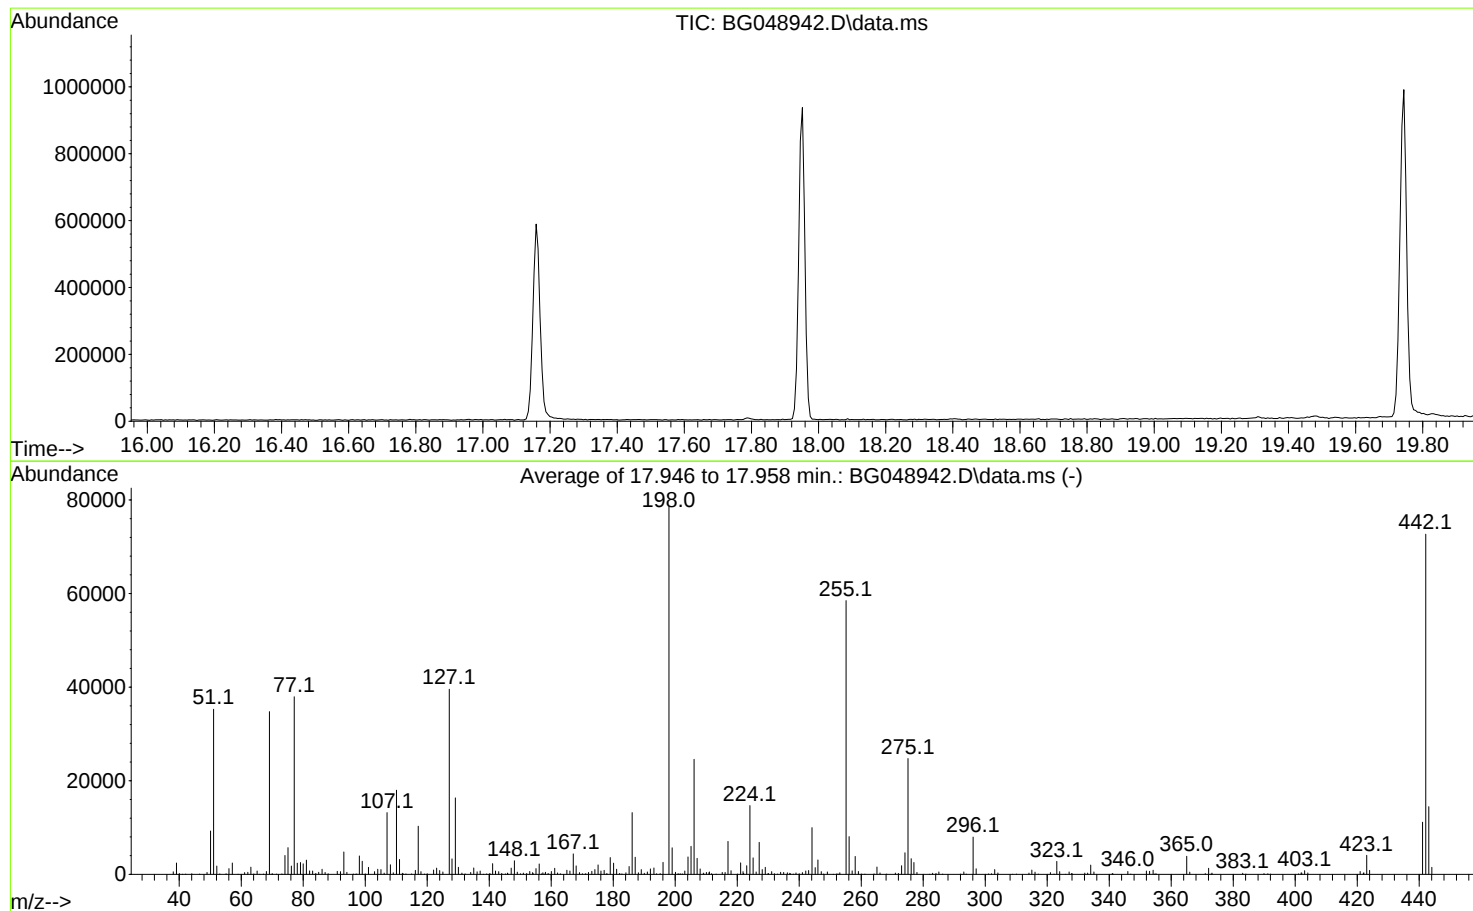

AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2530

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	35299	PASS
68	69	0.00	2	1.7	607	PASS
69	198	0.00	100	44.2	34757	PASS
70	69	0.00	2	0.3	100	PASS
127	198	10	80	50.3	39565	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78597	PASS
199	198	5	9	7.2	5676	PASS
275	198	10	60	31.5	24739	PASS
365	198	1	100	4.9	3882	PASS
441	198	0.01	100	14.2	11163	PASS
442	198	50	100	92.5	72685	PASS
443	442	15	24	19.9	14467	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/14/2021	BNA_G	<u>BG048942.D</u>
Compound Name	Response	Retention Time
DDT	264398	20.98
DDD	17049	20.53
DDE	1530	20.03
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18579	282977	6.57

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061421\
Data File : BG048942.D
Acq On : 14 Jun 2021 9:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 14 10:50:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

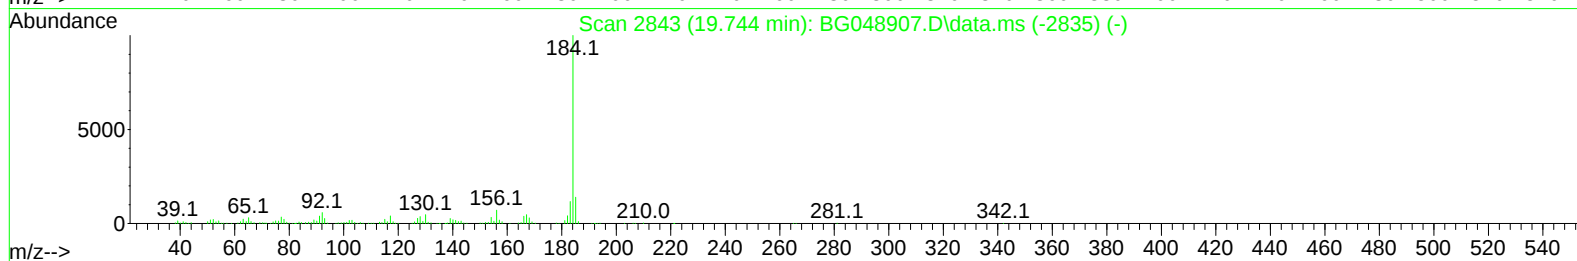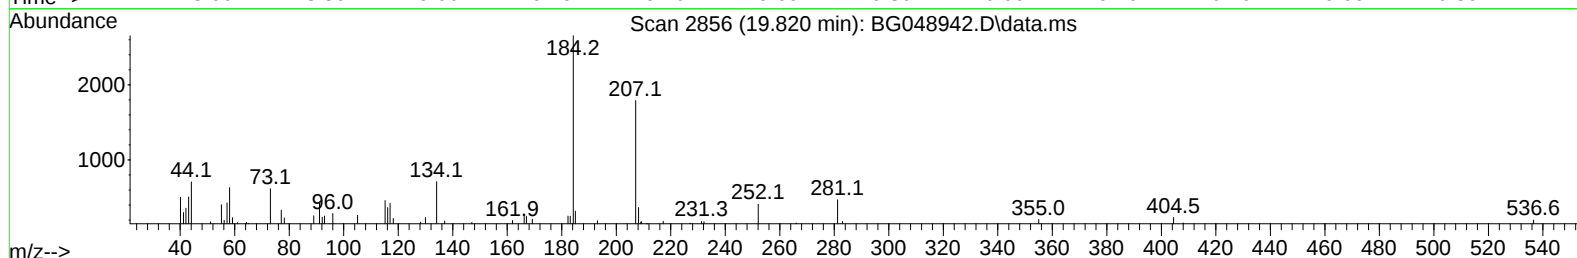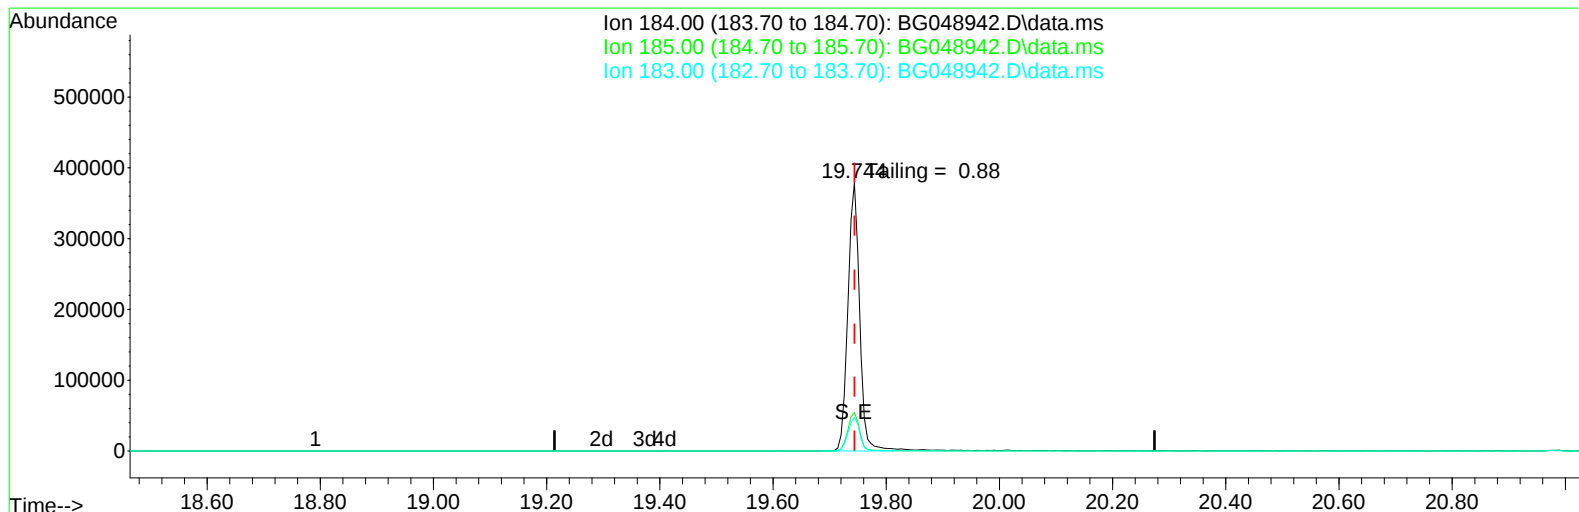

TIC: BG048942.D\data.ms

(77) Benzidine

19.744min (-0.000) 7917.46 ng m




response 548988

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.39
183.00	11.70	12.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061421\
 Data File : BG048942.D
 Acq On : 14 Jun 2021 9:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 14 10:50:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 16:03:10 2021
 Response via : Initial Calibration

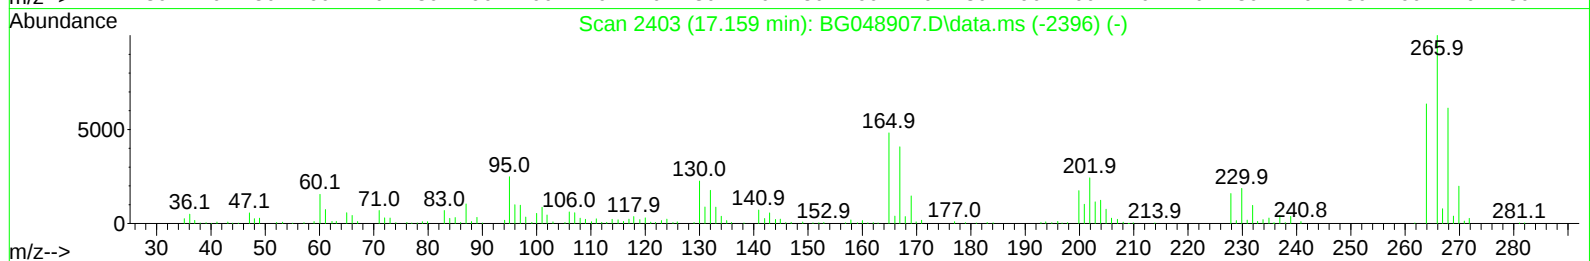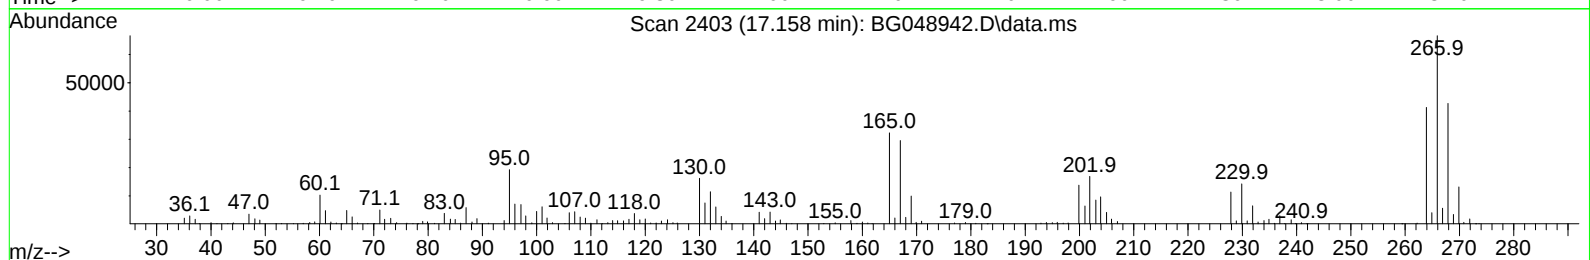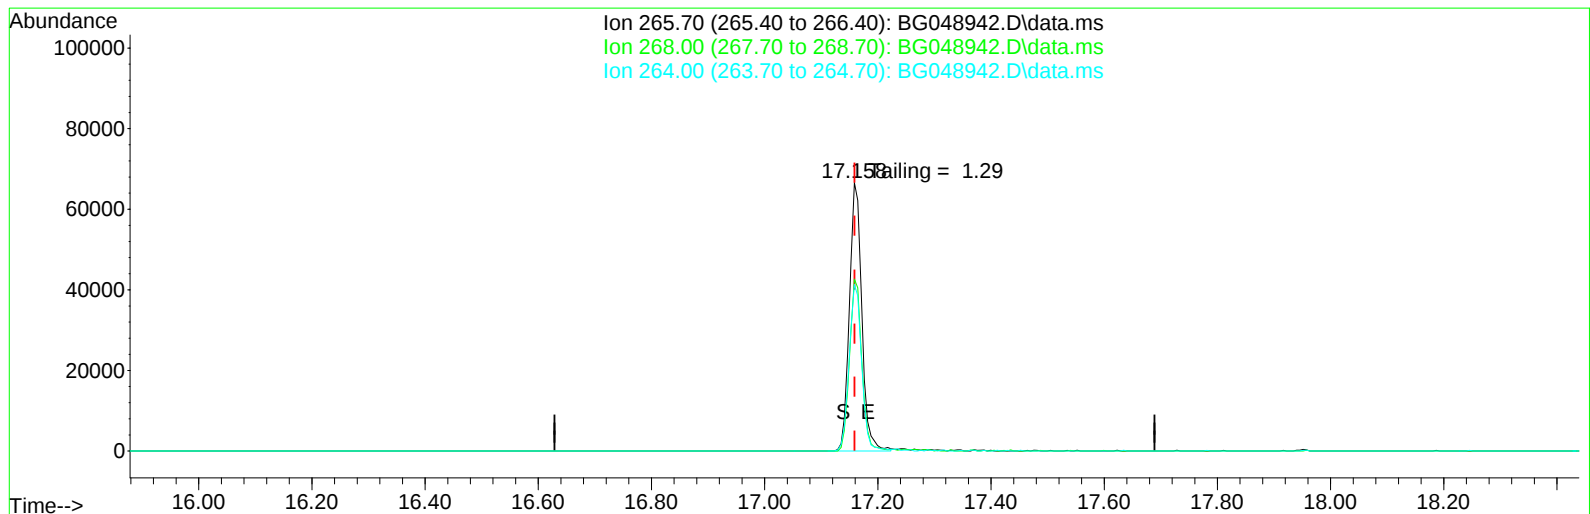

TIC: BG048942.D\data.ms

(70) Pentachlorophenol (C)

17.158min (-0.000) 173355.83 ng

response 97285

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.06
264.00	61.30	61.99
0.00	0.00	0.00