
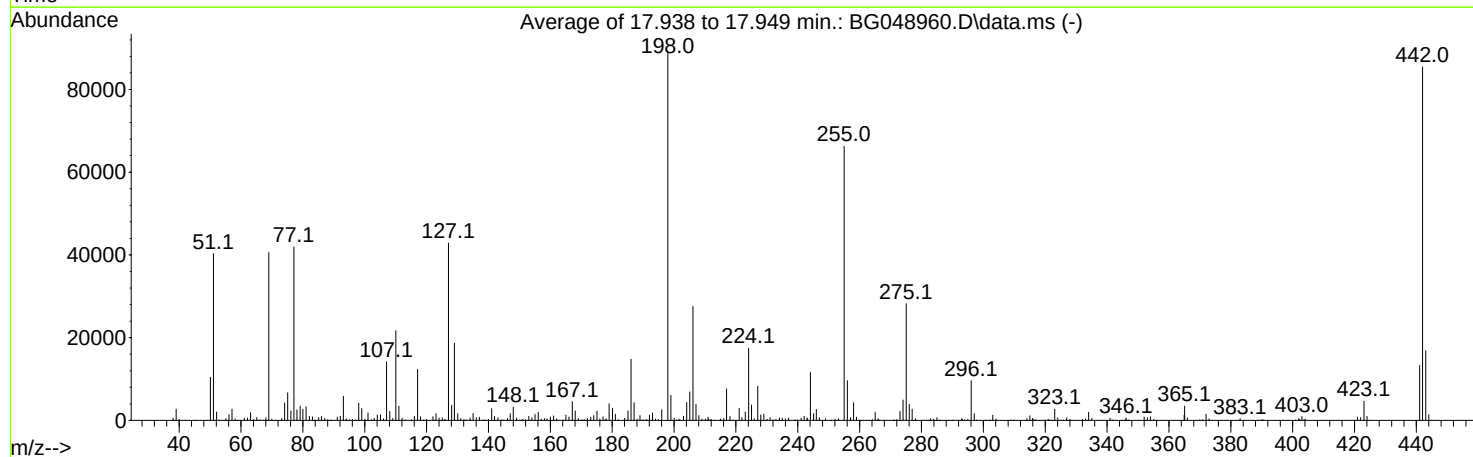


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061421\
 Data File : BG048960.D
 Acq On : 14 Jun 2021 23:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 11 16:03:10 2021

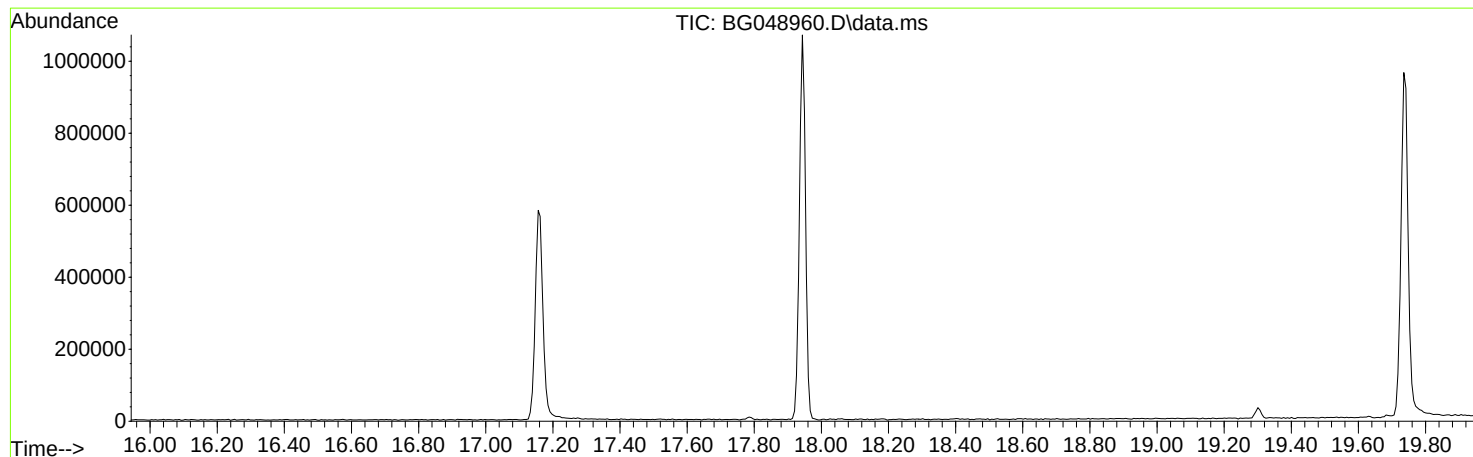

AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	40296	PASS
68	69	0.00	2	1.5	624	PASS
69	198	0.00	100	45.6	40595	PASS
70	69	0.00	2	0.8	309	PASS
127	198	10	80	48.2	42869	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88931	PASS
199	198	5	9	6.8	6090	PASS
275	198	10	60	31.7	28213	PASS
365	198	1	100	3.9	3460	PASS
441	198	0.01	100	14.9	13279	PASS
442	198	50	100	96.1	85429	PASS
443	442	15	24	19.7	16864	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/14/2021	BNA_G	<u>BG048960.D</u>
Compound Name	Response	Retention Time
DDT	169826	20.975
DDD	107193	20.529
DDE	1366	20.023
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
108559	278385	39.00

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061421\
 Data File : BG048960.D
 Acq On : 14 Jun 2021 23:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 15 02:07:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 16:03:10 2021
 Response via : Initial Calibration

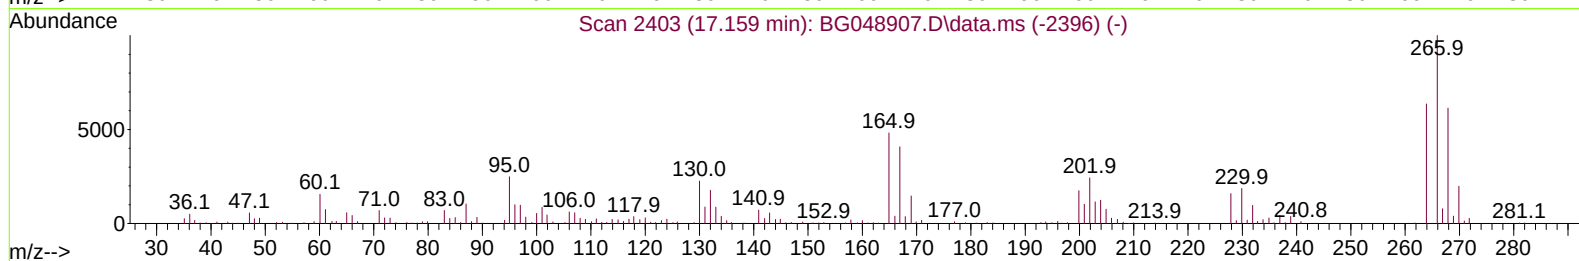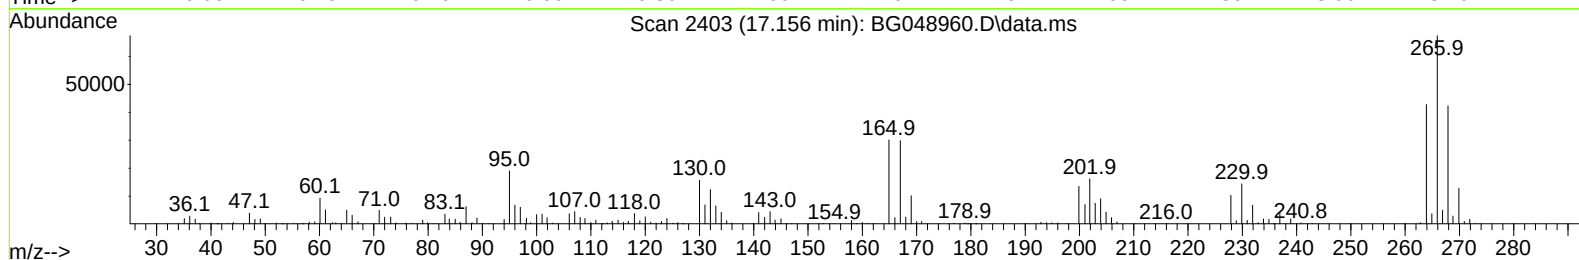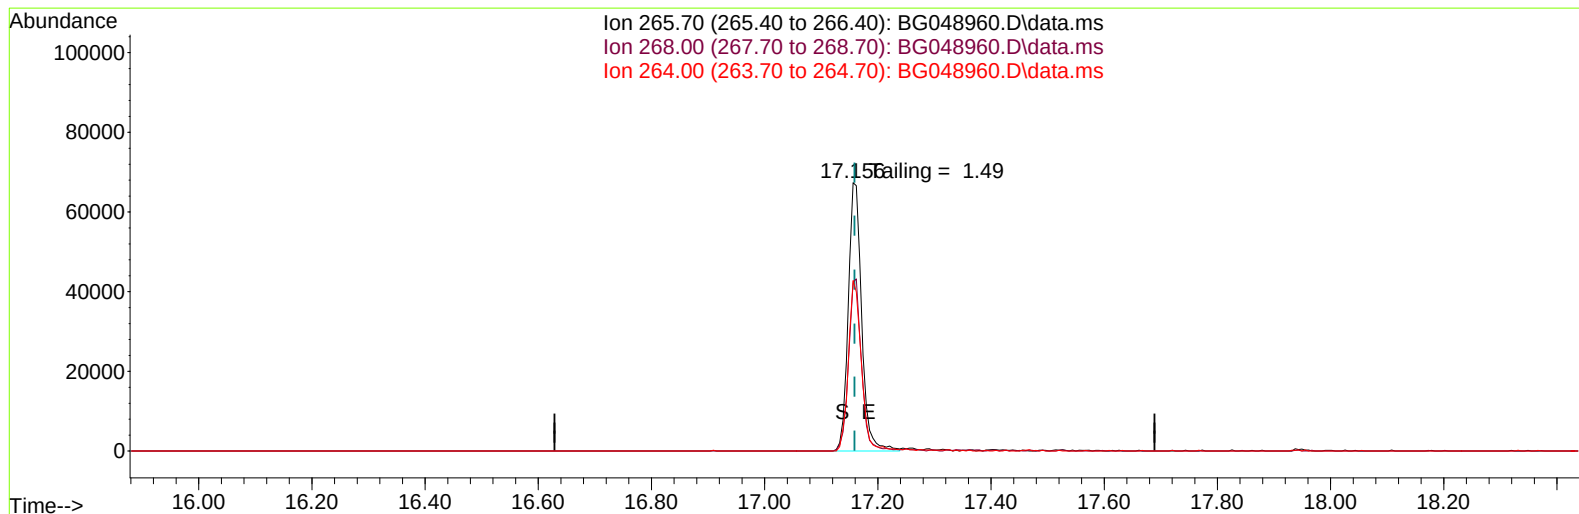

TIC: BG048960.D\data.ms

(70) Pentachlorophenol (C)

17.156min (-0.003) 26036.21 ng




response 111172

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.80
264.00	61.30	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061421\
Data File : BG048960.D
Acq On : 14 Jun 2021 23:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 15 02:07:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

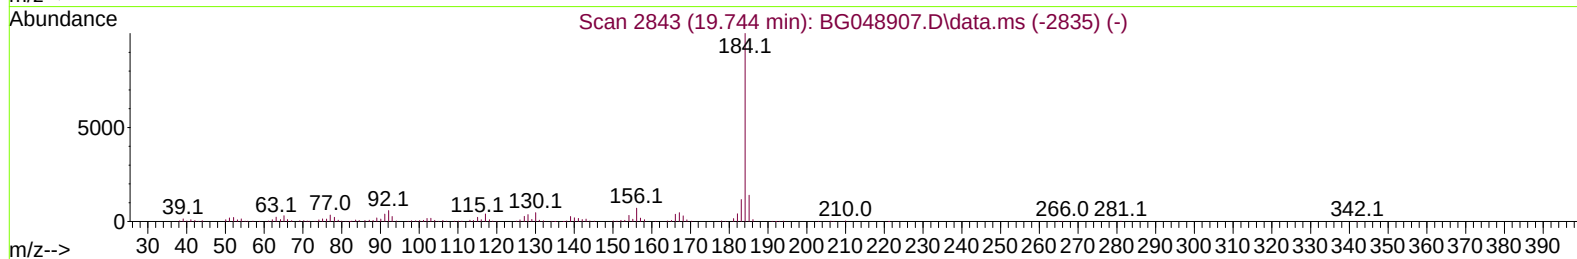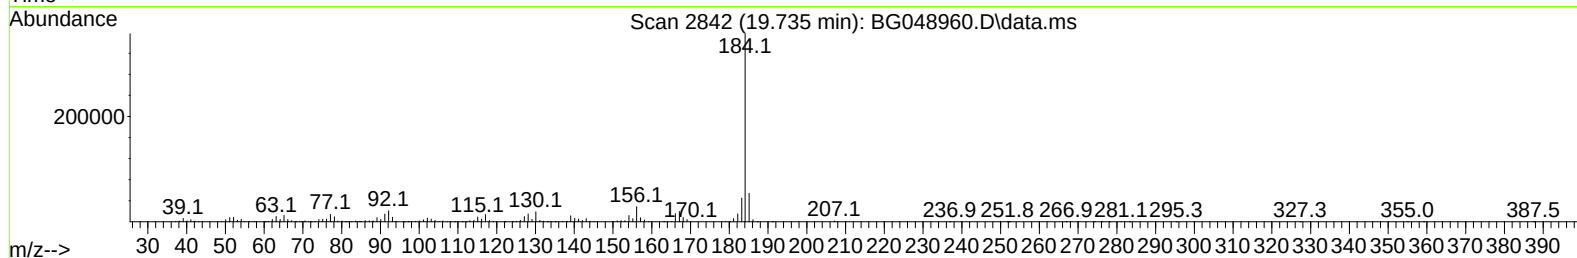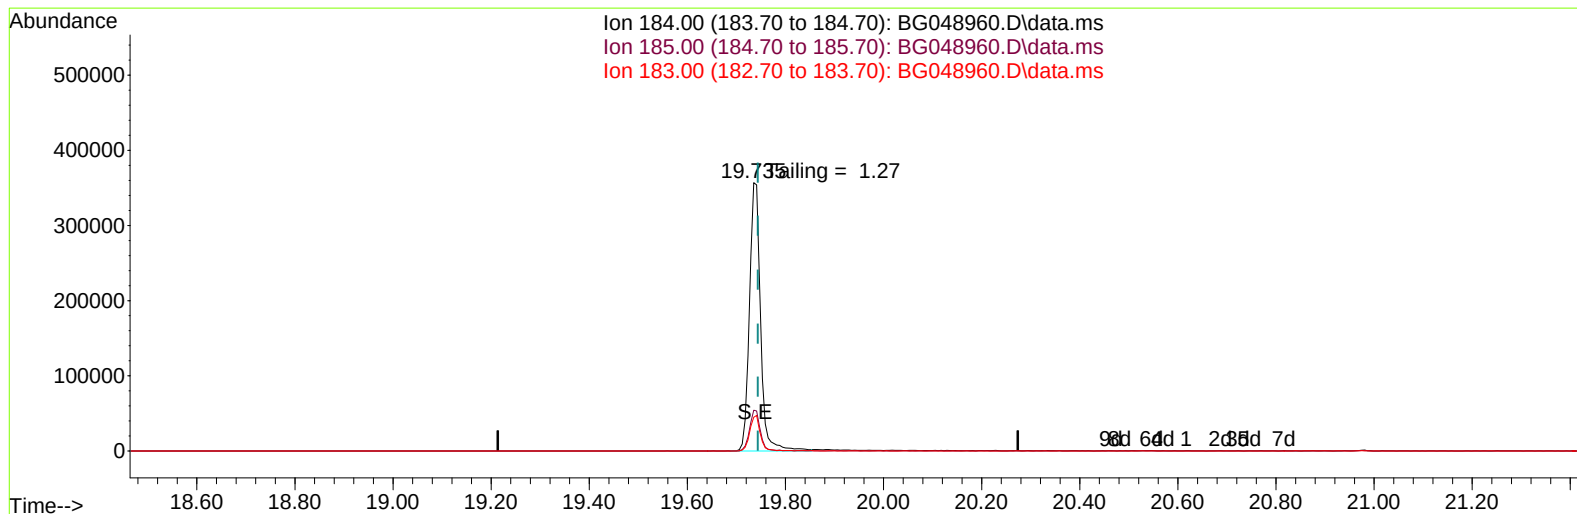

TIC: BG048960.D\data.ms

(77) Benzidine

19.735min (-0.008) 521886.33 ng m

response 588749

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.23
183.00	11.70	12.62
0.00	0.00	0.00