
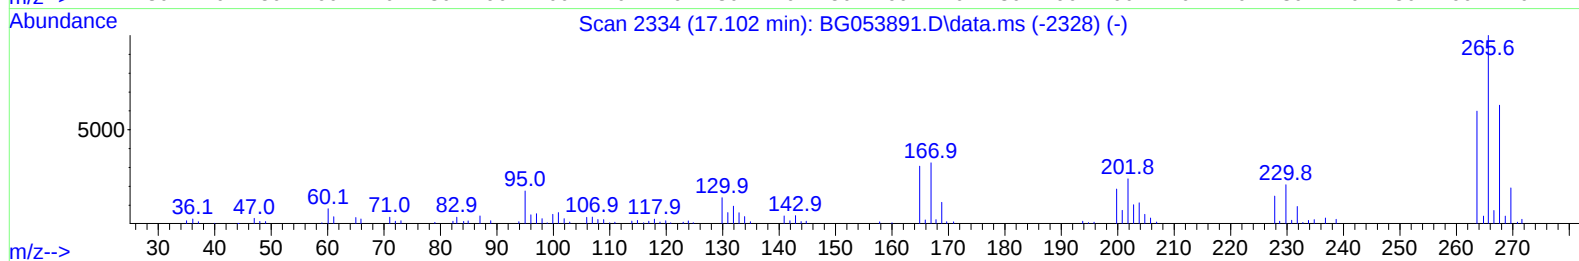
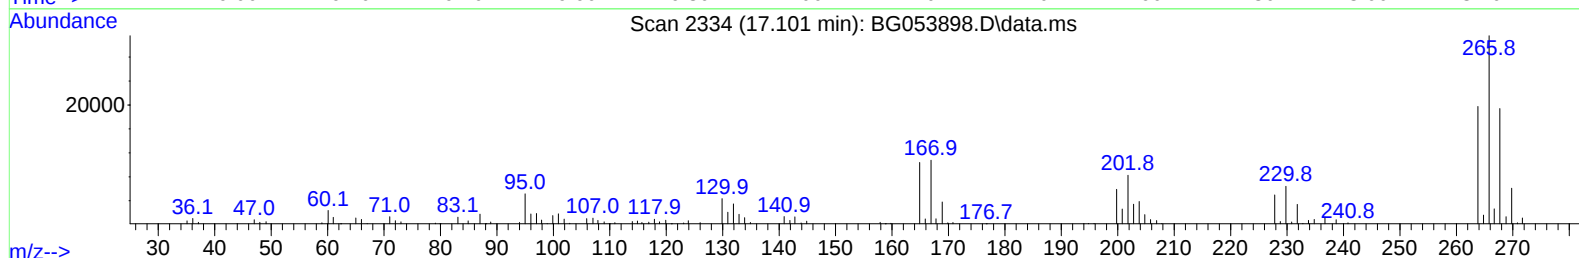


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061422\
Data File : BG053898.D
Acq On : 14 Jun 2022 11:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 02:57:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

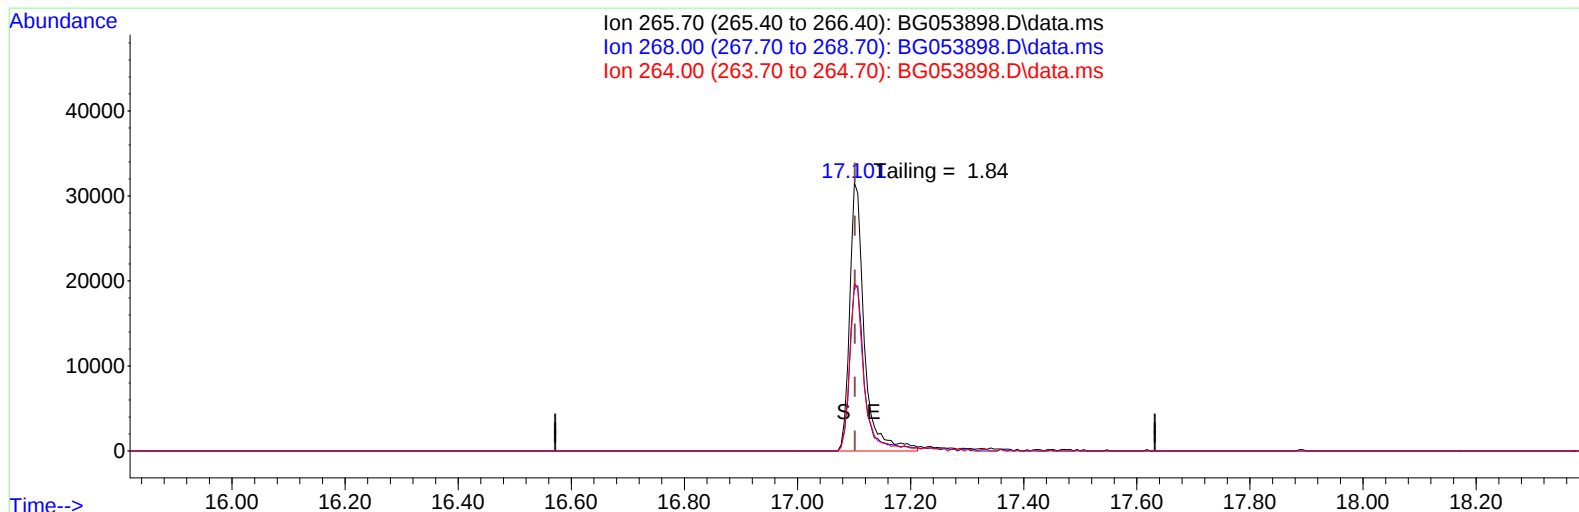

TIC: BG053898.D\data.ms

(70) Pentachlorophenol (C)




17.101min (-0.001) 32786.81 ng

response 55267

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.45
264.00	66.20	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061422\
Data File : BG053898.D
Acq On : 14 Jun 2022 11:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 02:57:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

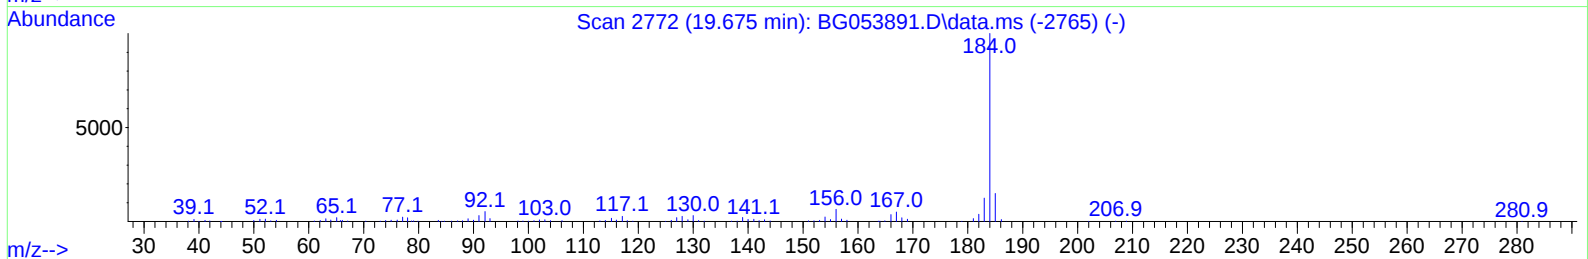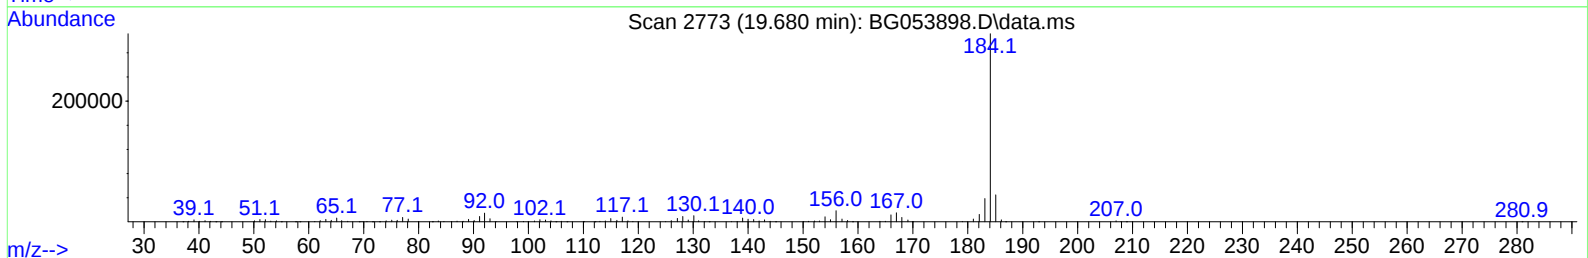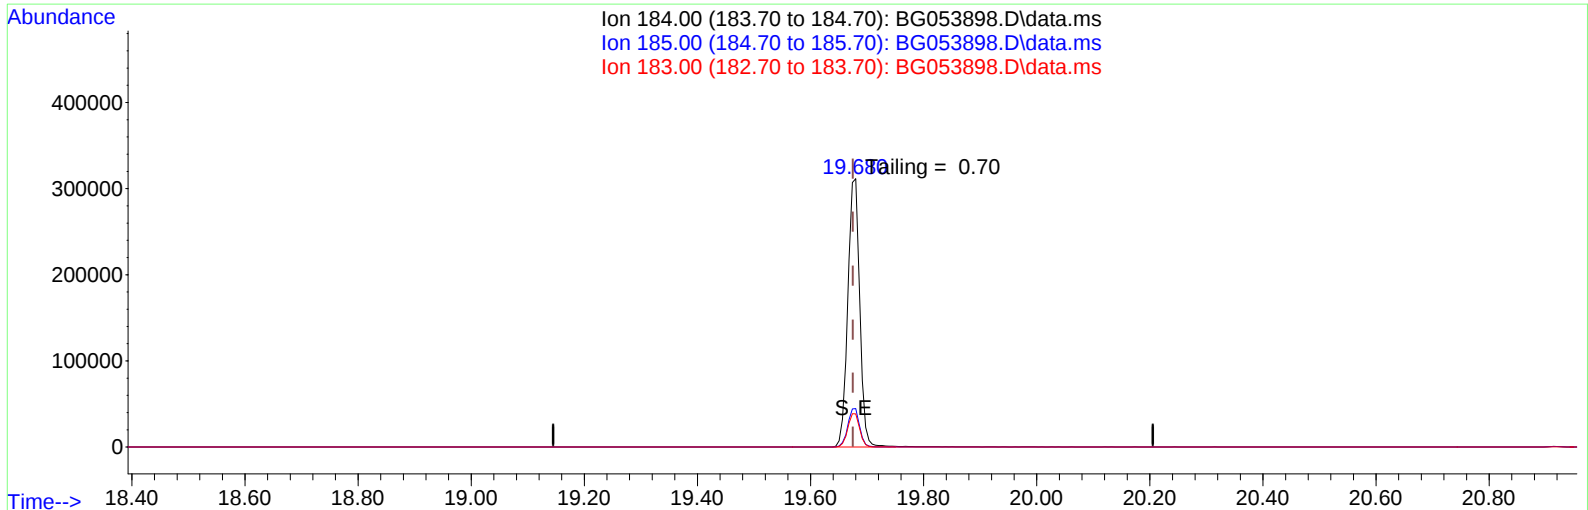

TIC: BG053898.D\data.ms

(77) Benzidine

19.680min (+ 0.005) 0.00 ng

response 459006

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.33
183.00	11.10	12.37
0.00	0.00	0.00