


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061422\
 Data File : BG053898.D
 Acq On : 14 Jun 2022 11:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 15:49:31 2022

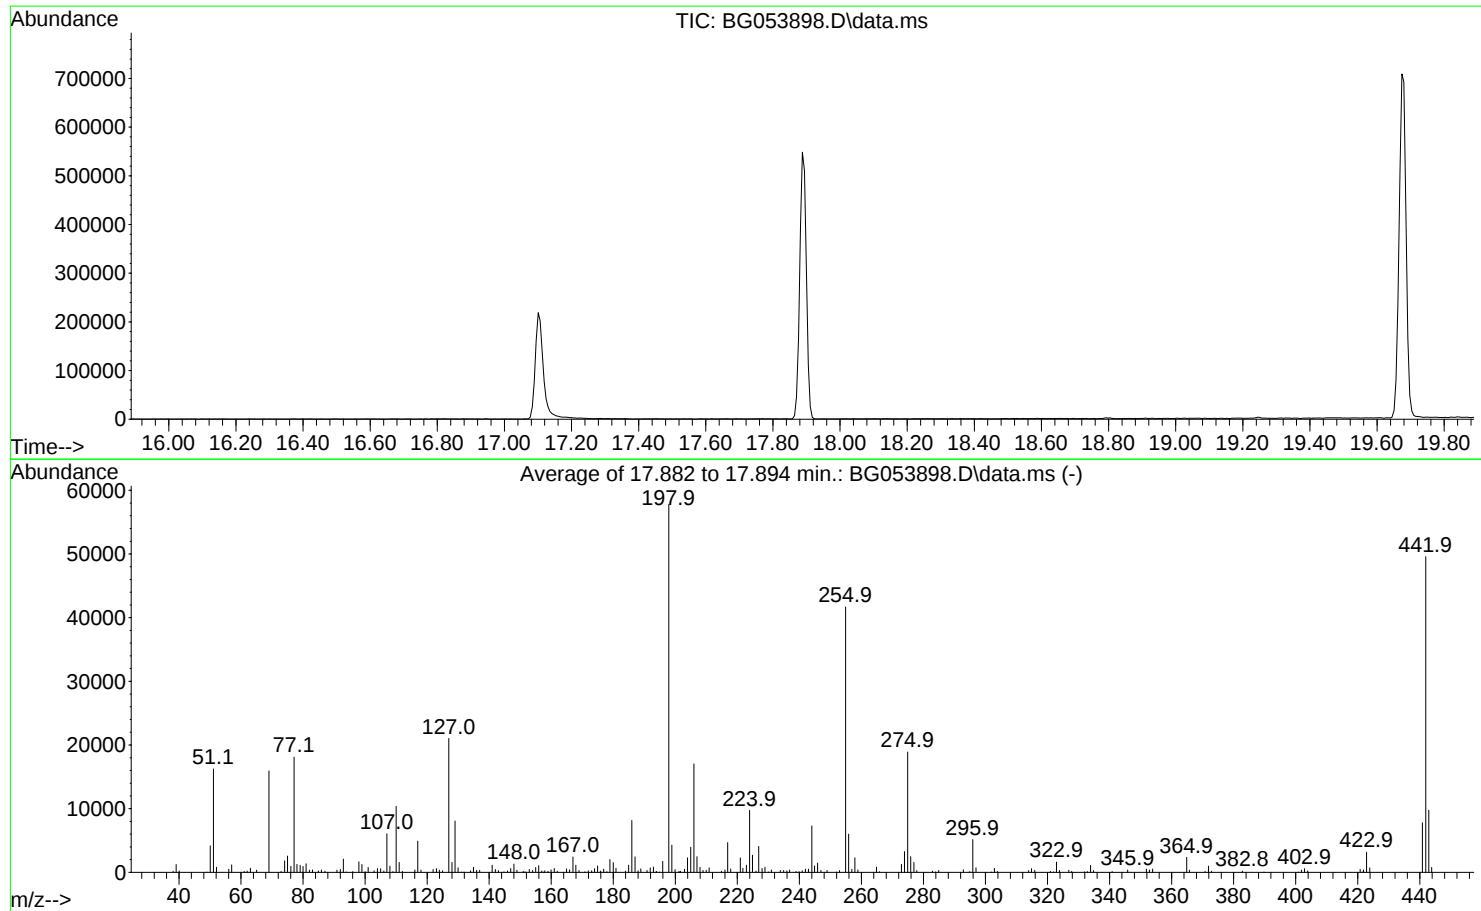




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	16240	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.6	15935	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.4	21021	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57768	PASS
199	198	5	9	7.4	4267	PASS
275	198	10	60	32.7	18899	PASS
365	198	1	100	4.1	2357	PASS
441	198	0.01	100	13.5	7783	PASS
442	442	50	100	100.0	49581	PASS
443	442	15	24	19.7	9756	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061422\
Data File : BG053898.D
Acq On : 14 Jun 2022 11:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 15 02:57:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

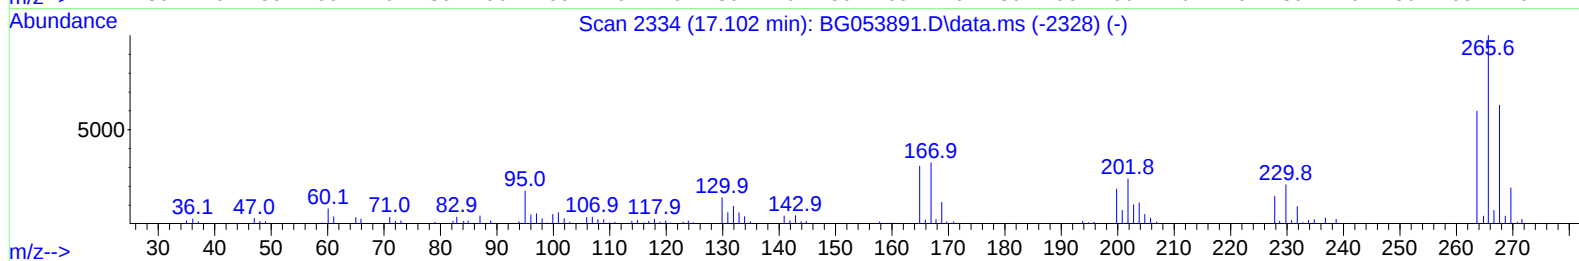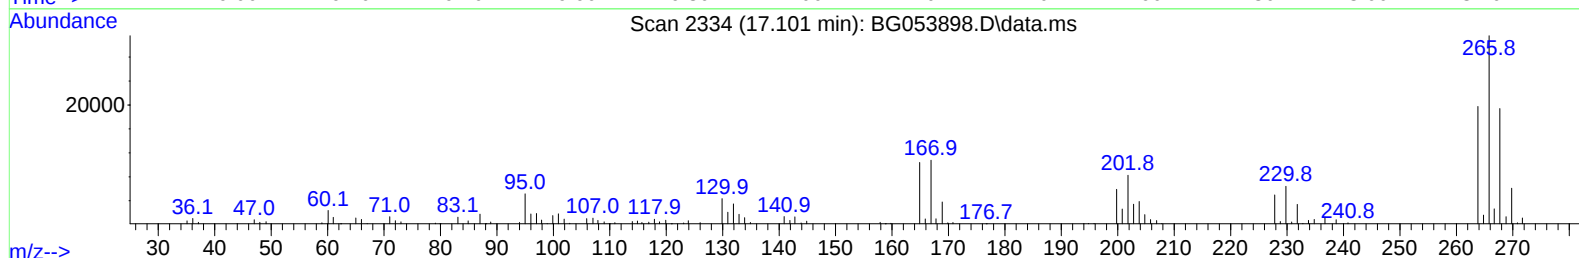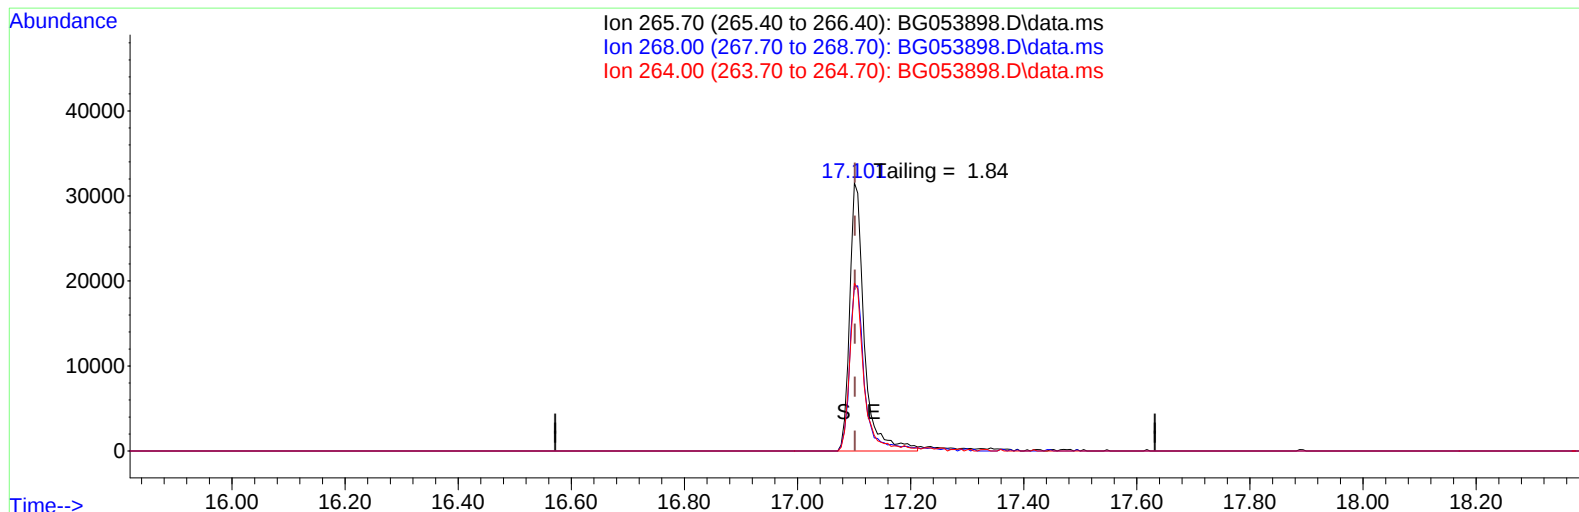

TIC: BG053898.D\data.ms

(70) Pentachlorophenol (C)

17.101min (-0.001) 32786.81 ng




response 55267

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.45
264.00	66.20	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061422\
Data File : BG053898.D
Acq On : 14 Jun 2022 11:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 15 02:57:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

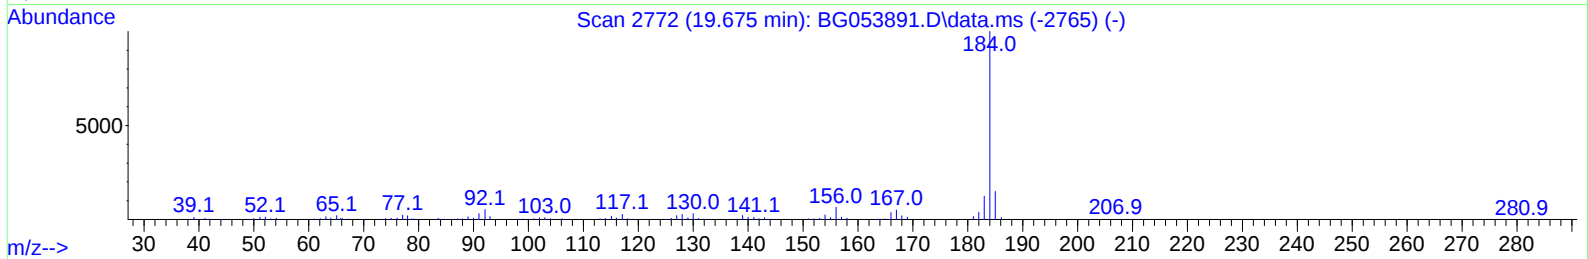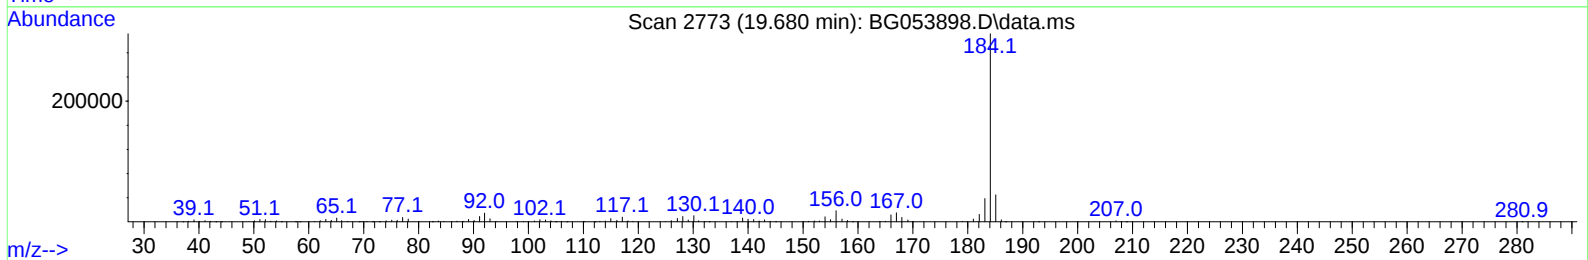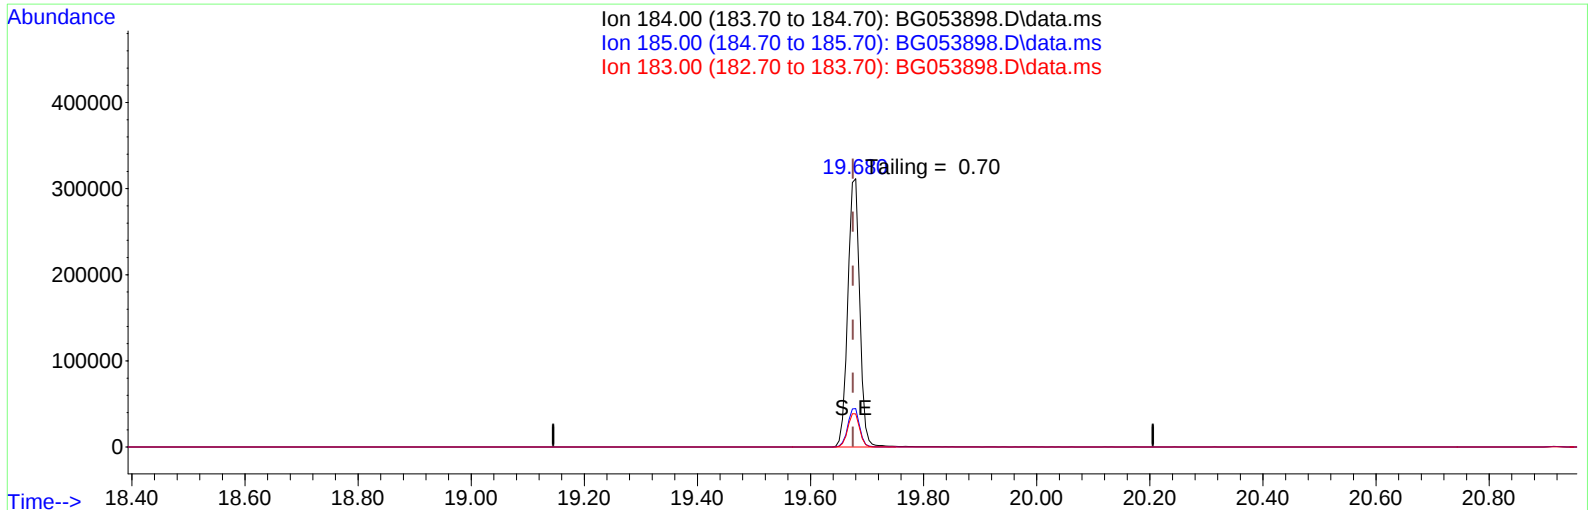

TIC: BG053898.D\data.ms

(77) Benzidine

19.680min (+ 0.005) 0.00 ng

response 459006

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.33
183.00	11.10	12.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/14/2022	BNA_G	<u>BG053898.D</u>
Compound Name	Response	Retention Time
DDT	231178	20.92
DDD	2019	20.467
DDE	0	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2019	233197	0.87

Instrument :
BNA_G
ClientSampleId :
DFTPP