


Data Path : Z:\HPCHEM1\BNA G\Data\BG061515\
Data File : BG017684.D
Acq On : 15 Jun 2015 10:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 07:17:03 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 13 02:22:44 2015
Response via : Initial Calibration

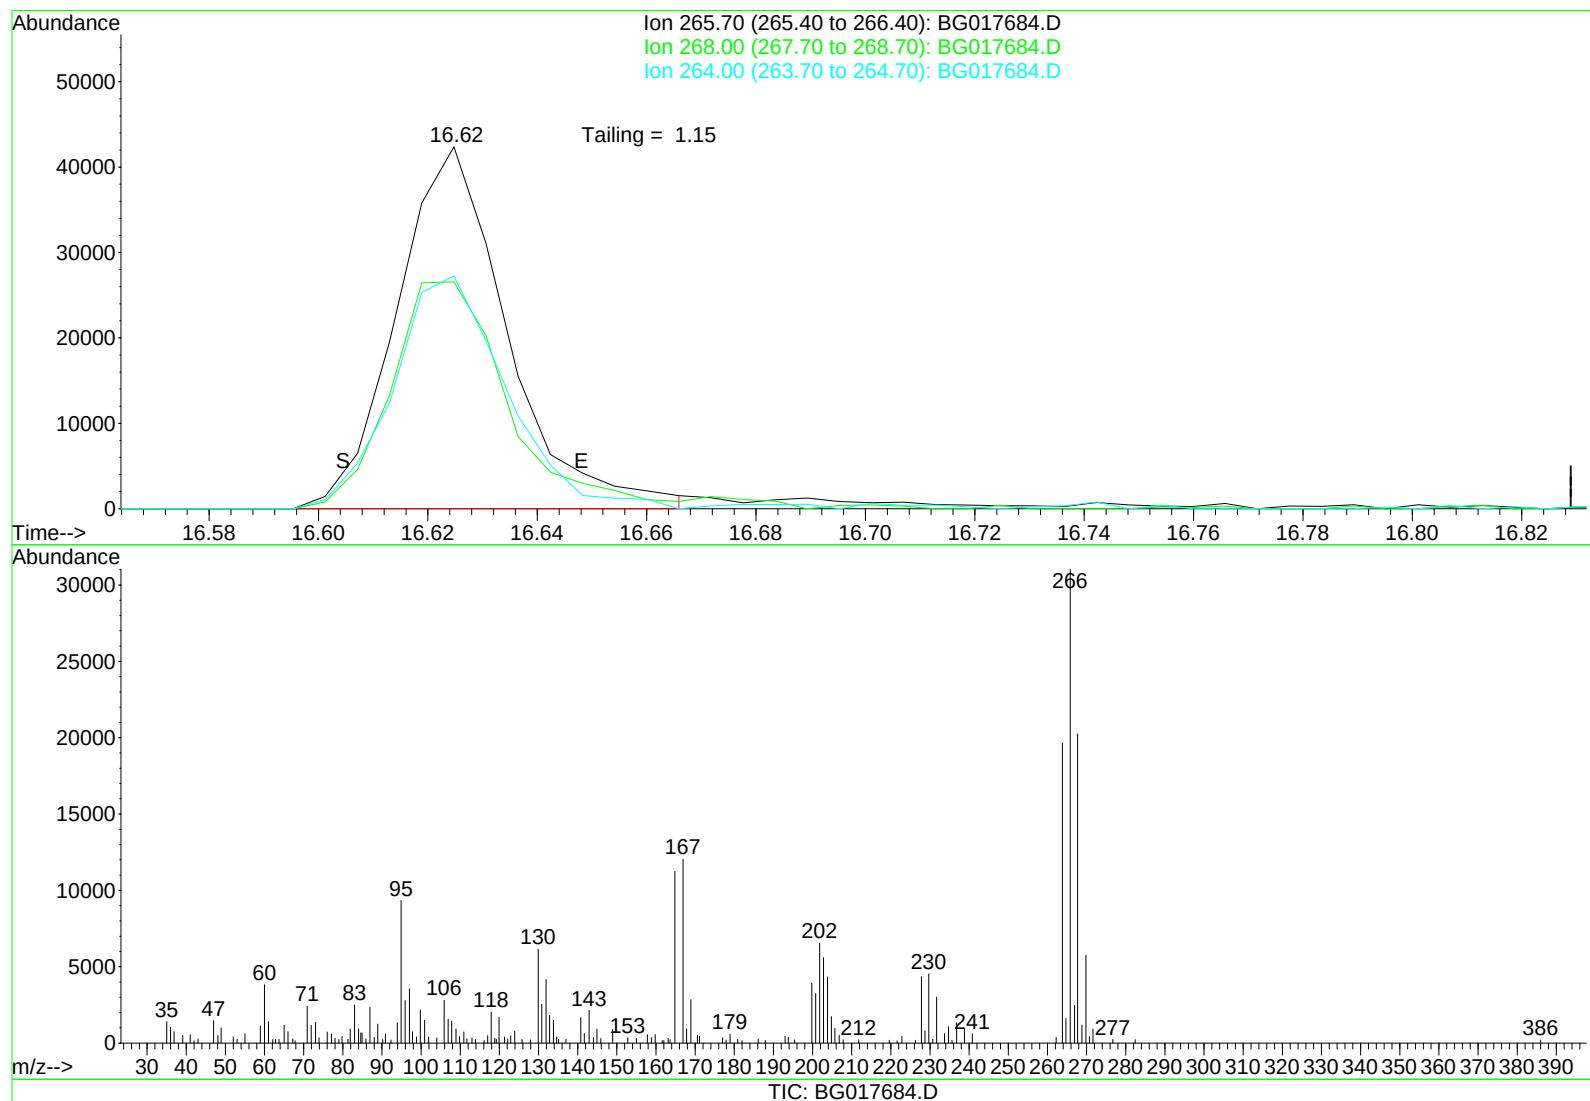

(69) Pentachlorophenol (C)



16.629min (-16.629) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	65.90	0.00#
264.00	65.30	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG061515\
Data File : BG017684.D
Acq On : 15 Jun 2015 10:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 07:17:03 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 13 02:22:44 2015
Response via : Initial Calibration

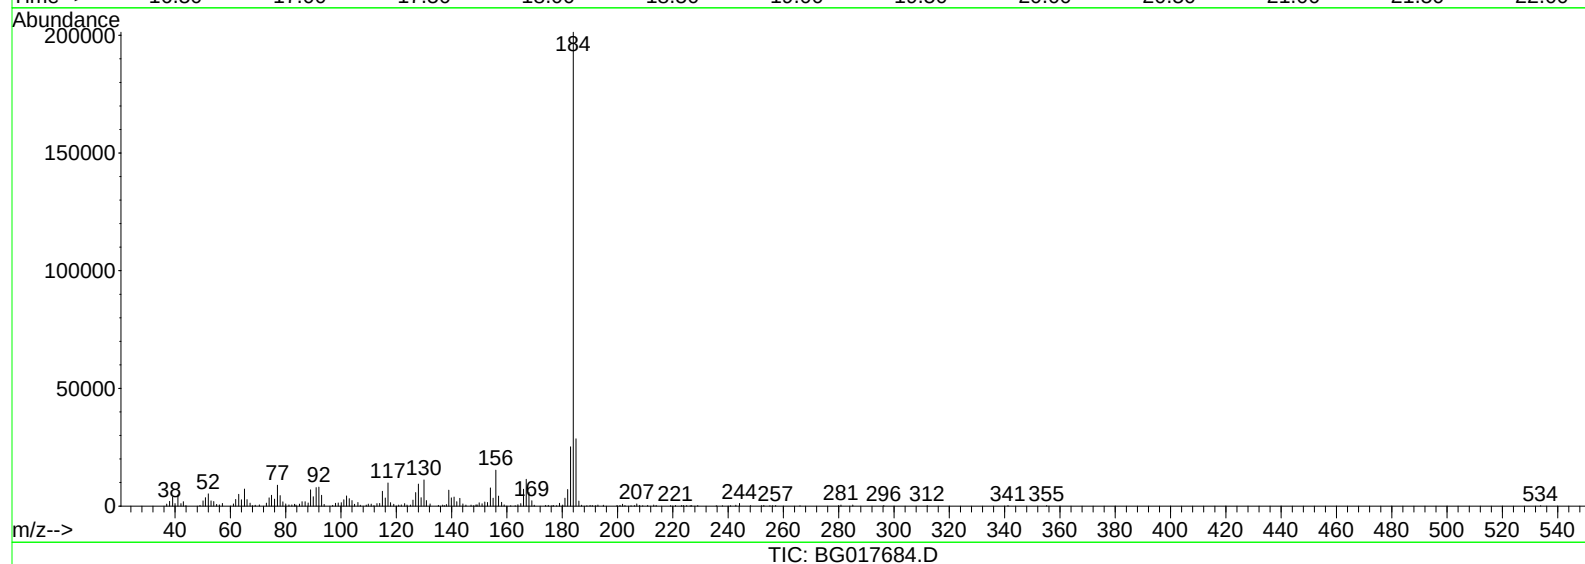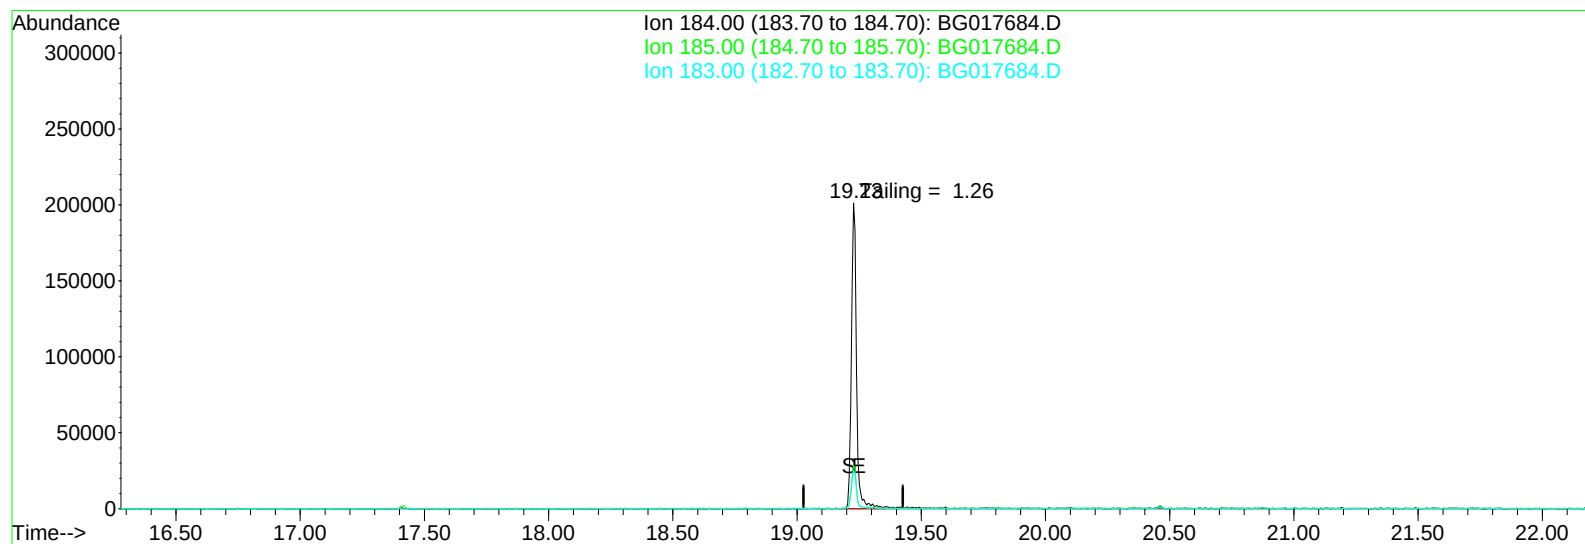

(76) Benzidine

19.226min (-19.226) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.30	0.00#
183.00	14.00	0.00#
0.00	0.00	0.00