


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061515\
Data File : BG017684.D
Acq On : 15 Jun 2015 10:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jun 13 02:22:44 2015

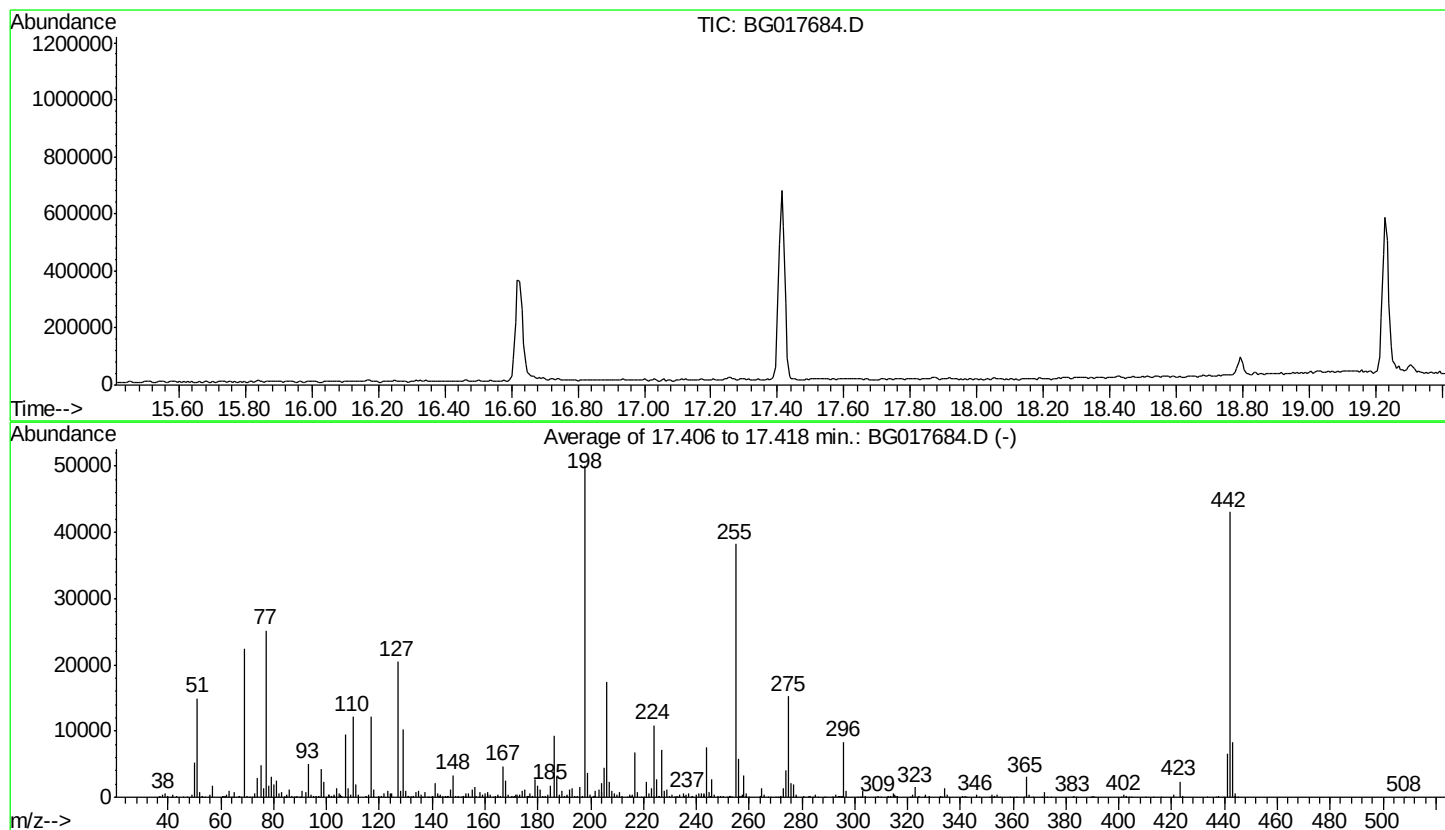

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	14923	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.9	22464	PASS
70	69	0.00	2	0.8	176	PASS
127	198	10	80	40.9	20473	PASS
197	198	0.00	2	0.5	244	PASS
198	198	100	100	100.0	50064	PASS
199	198	5	9	7.4	3693	PASS
275	198	10	60	30.5	15258	PASS
365	198	1	100	6.0	3014	PASS
441	442	0.01	24	15.4	6614	PASS
442	198	50	100	86.0	43072	PASS
443	442	15	24	19.4	8348	PASS