


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061515\
 Data File : BG017701.D
 Acq On : 15 Jun 2015 21:51
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jun 13 02:22:44 2015

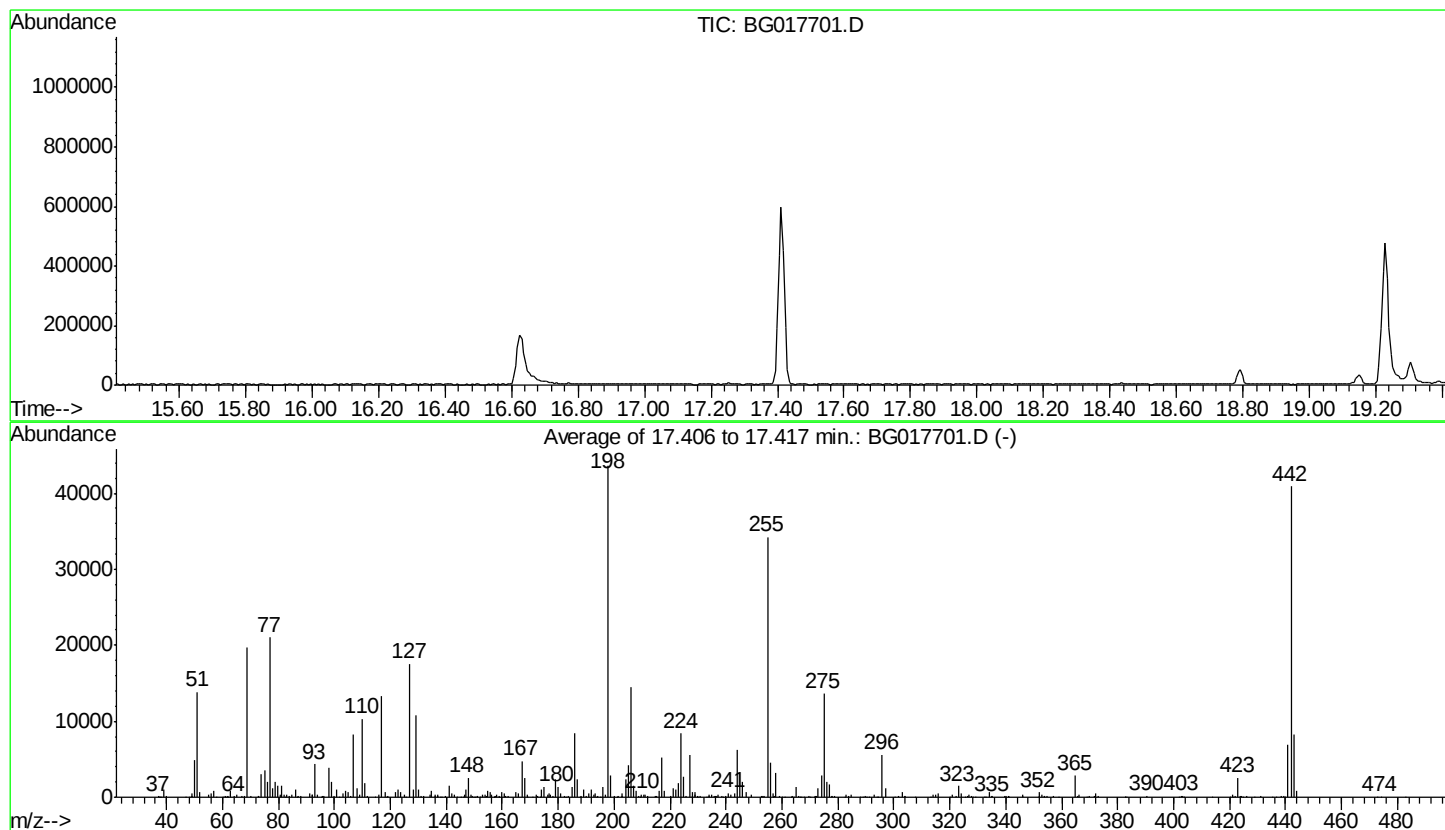

AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	13822	PASS
68	69	0.00	2	0.9	171	PASS
69	198	0.00	100	45.0	19645	PASS
70	69	0.00	2	0.6	110	PASS
127	198	10	80	40.3	17588	PASS
197	198	0.00	2	0.7	290	PASS
198	198	100	100	100.0	43642	PASS
199	198	5	9	6.6	2867	PASS
275	198	10	60	31.1	13590	PASS
365	198	1	100	6.4	2814	PASS
441	442	0.01	24	16.9	6905	PASS
442	198	50	100	93.8	40930	PASS
443	442	15	24	20.2	8265	PASS