
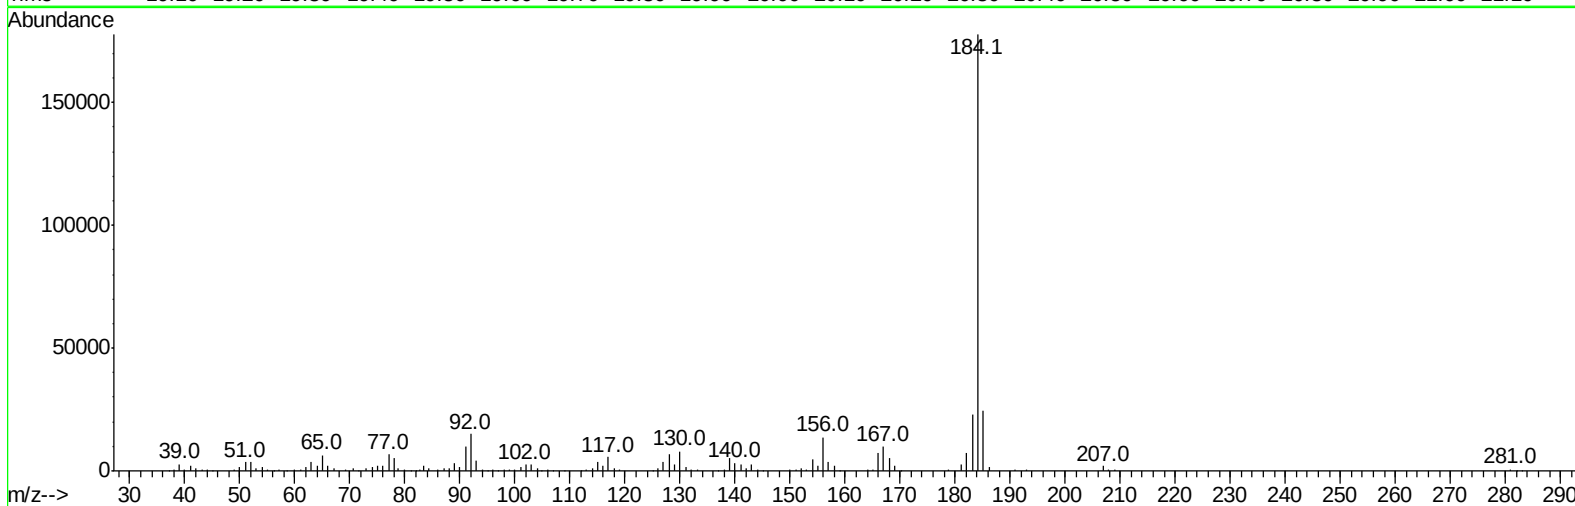


Data Path : Z:\HPCHEM1\BNA G\DATA\BG061517\
Data File : BG027451.D
Acq On : 15 Jun 2017 21:04
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 07:54:14 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG061417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 19:09:08 2017
Response via : Initial Calibration

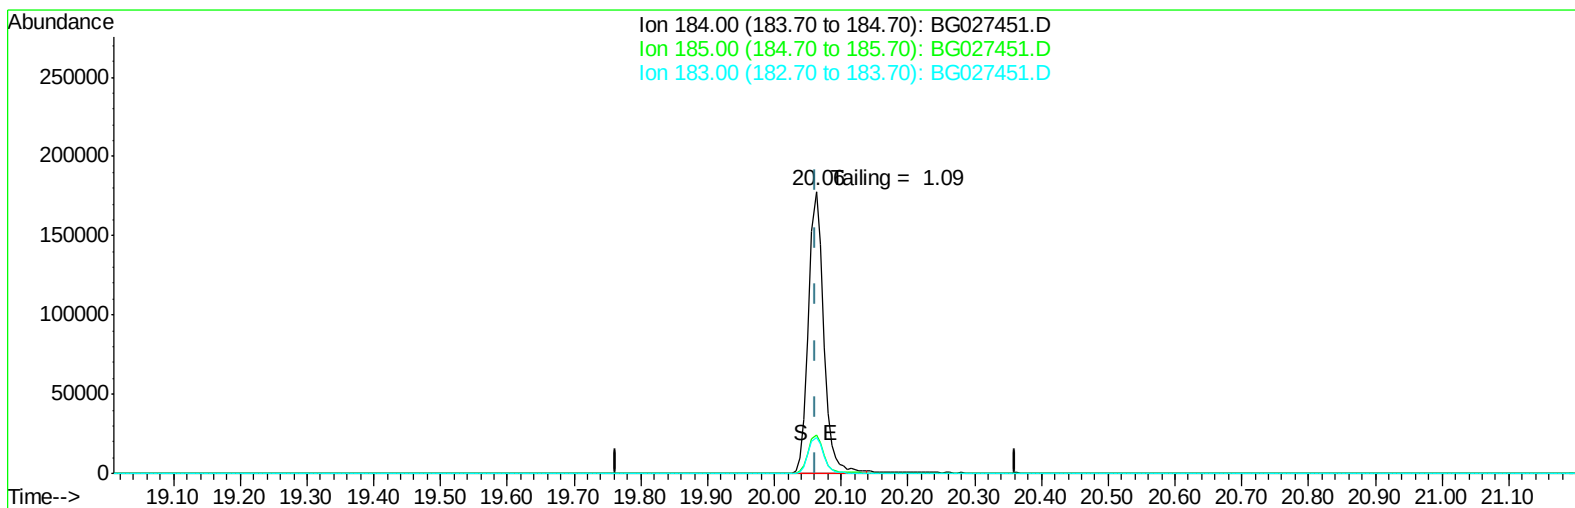

TIC: BG027451.D

(76) Benzidine



20.062min (+0.000) 0.00ng

response 276073

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.87
183.00	13.80	12.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061517\
Data File : BG027451.D
Acq On : 15 Jun 2017 21:04
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 07:54:14 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG061417.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 19:09:08 2017
Response via : Initial Calibration

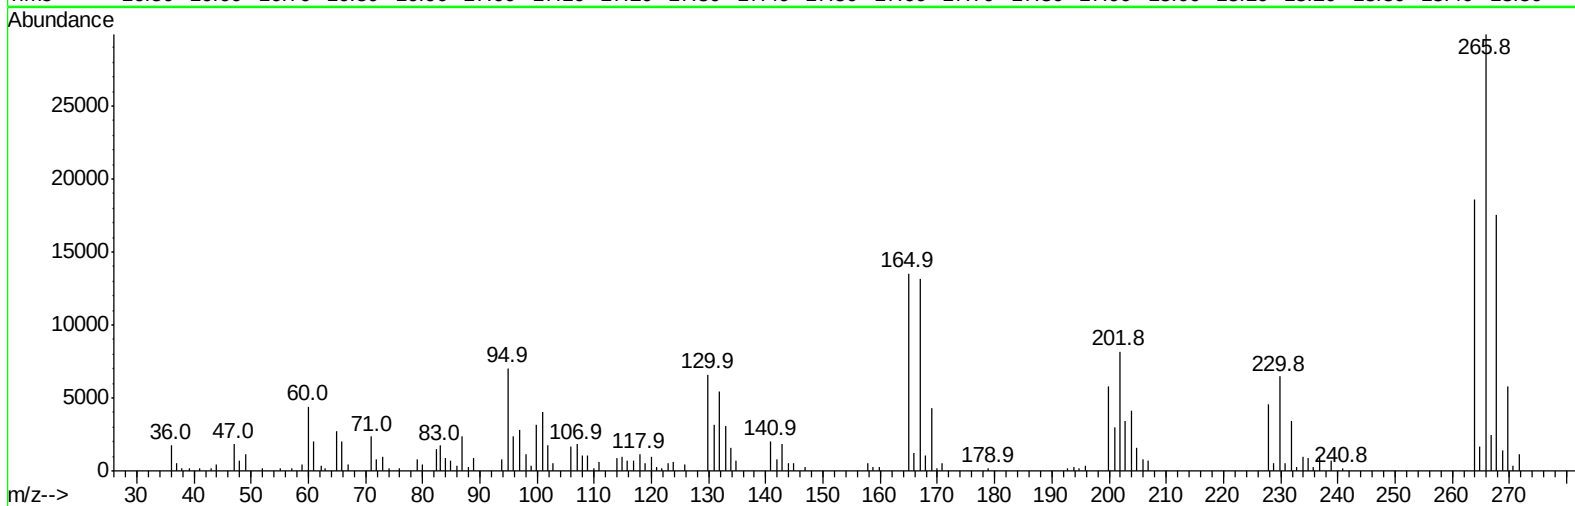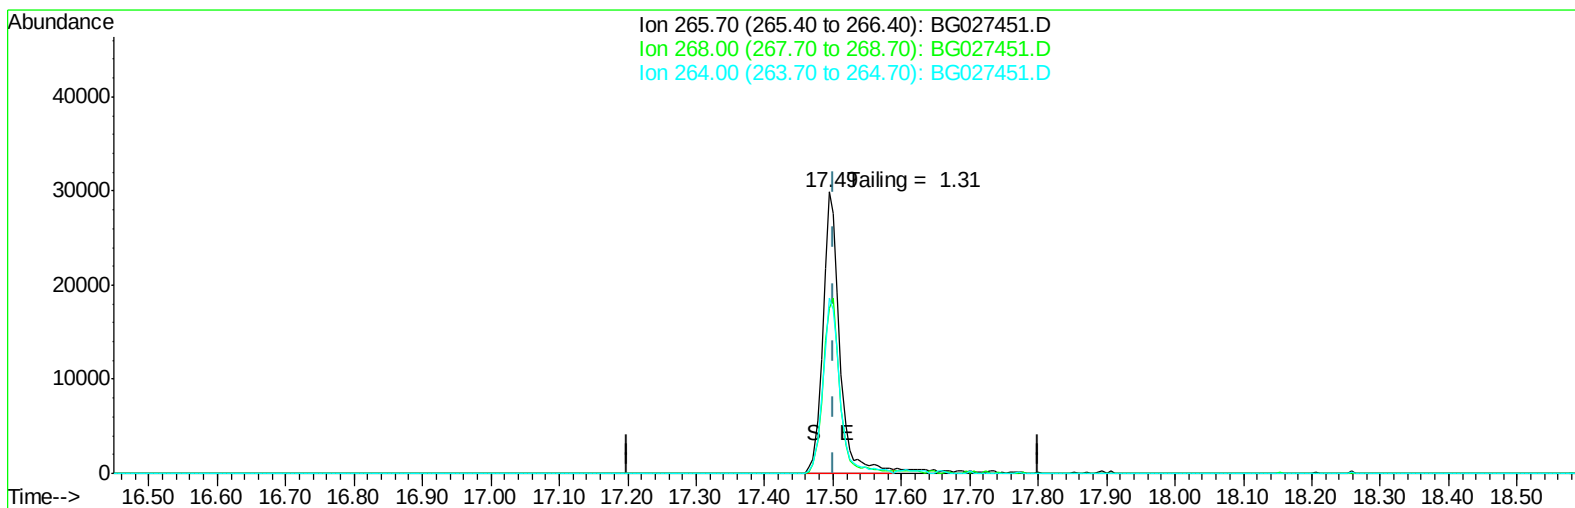

TIC: BG027451.D

(69) Pentachlorophenol (C)

17.495min (-0.006) 0.00ng

response 51420

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	58.76
264.00	62.60	62.29
0.00	0.00	0.00