


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061517\
 Data File : BG027451.D
 Acq On : 15 Jun 2017 21:04
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061417.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 14 19:09:08 2017

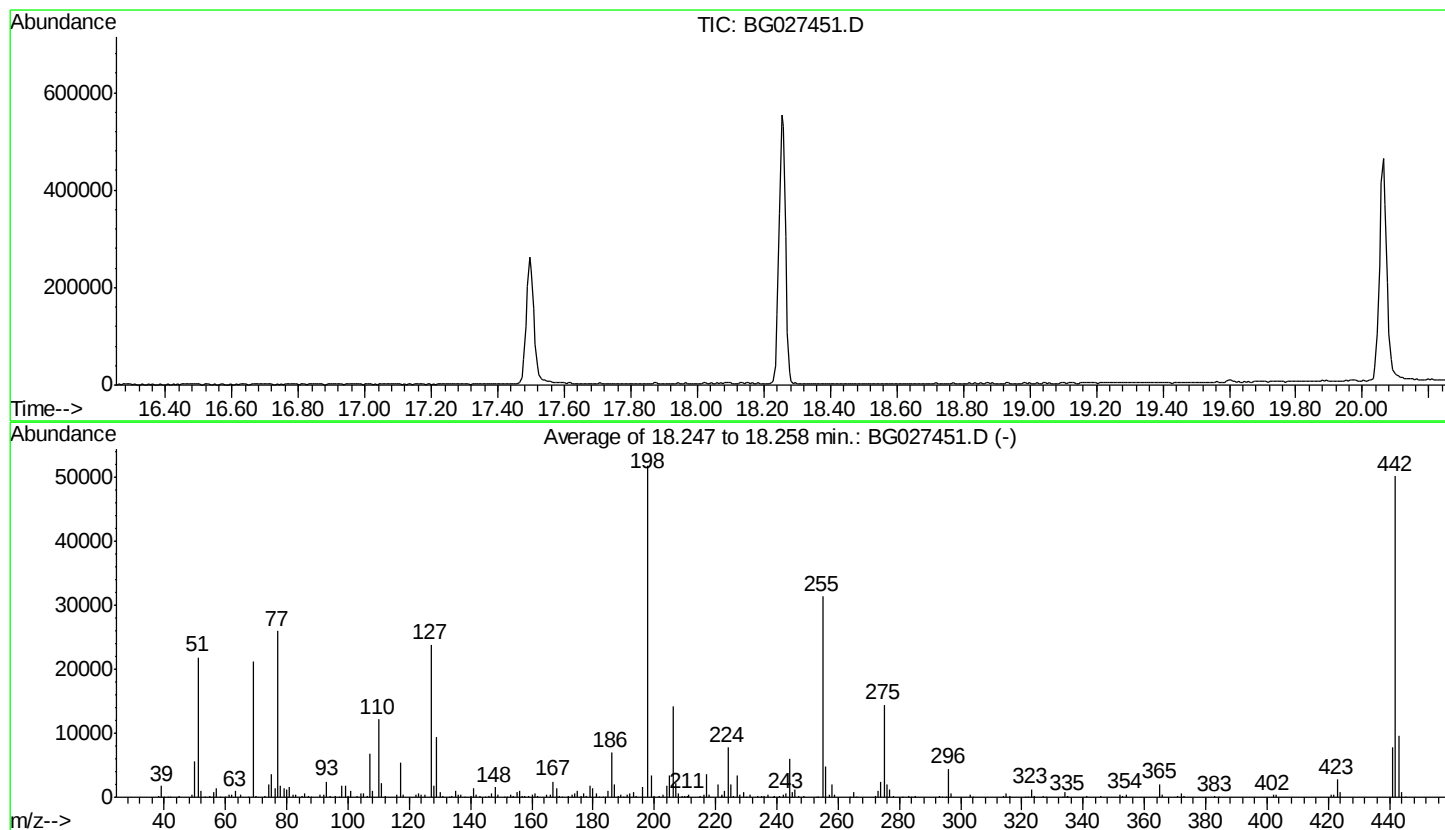

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	21896	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.8	21122	PASS
70	69	0.00	2	0.8	164	PASS
127	198	10	80	46.1	23893	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51816	PASS
199	198	5	9	6.4	3338	PASS
275	198	10	60	27.9	14470	PASS
365	198	1	100	4.1	2099	PASS
441	442	0.01	24	15.6	7801	PASS
442	198	50	100	96.8	50146	PASS
443	442	15	24	19.3	9690	PASS