
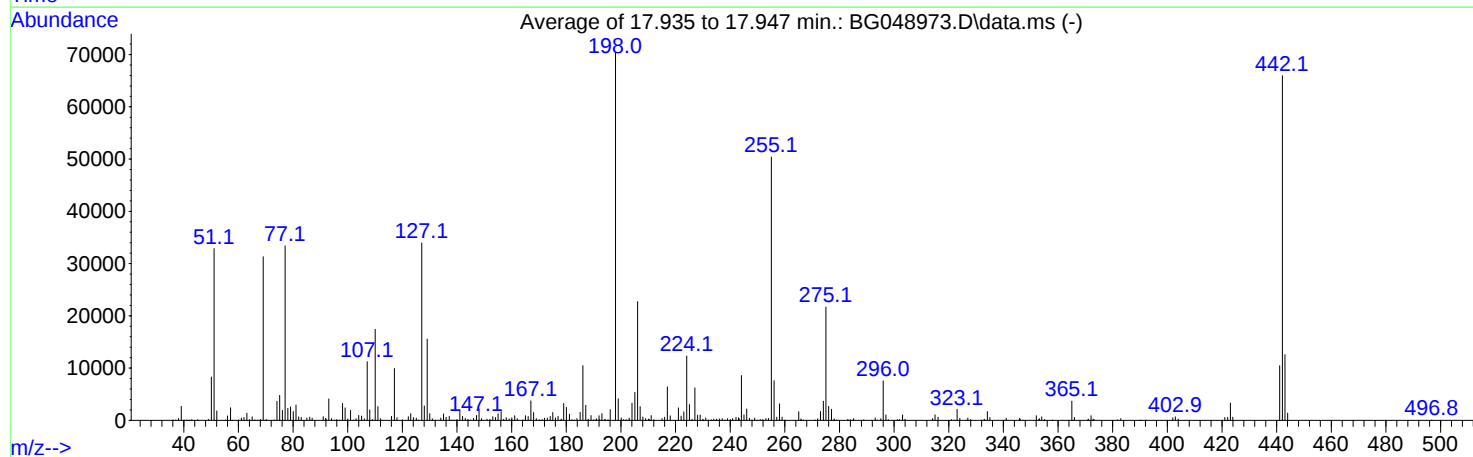


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061521\
 Data File : BG048973.D
 Acq On : 15 Jun 2021 11:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 16 12:04:50 2021

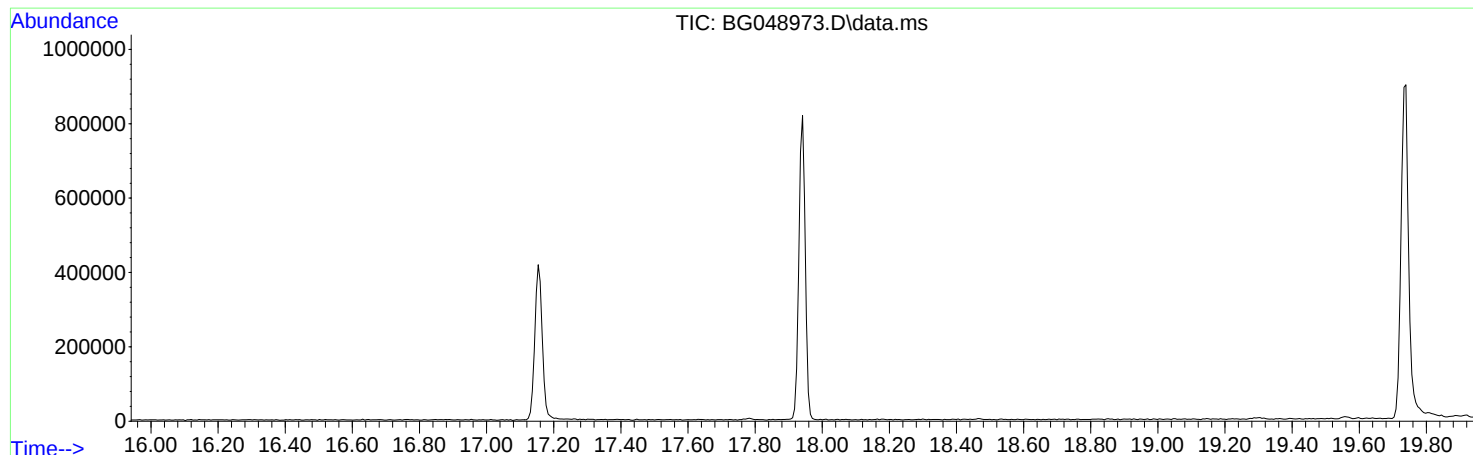




AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	32893	PASS
68	69	0.00	2	0.6	179	PASS
69	198	0.00	100	44.5	31323	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	48.2	33963	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70395	PASS
199	198	5	9	5.9	4121	PASS
275	198	10	60	30.8	21675	PASS
365	198	1	100	5.2	3677	PASS
441	198	0.01	100	14.8	10446	PASS
442	442	100	100	100.0	65944	PASS
443	442	15	24	19.1	12597	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061521\
 Data File : BG048973.D
 Acq On : 15 Jun 2021 11:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 15 13:16:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 11 16:03:10 2021
 Response via : Initial Calibration

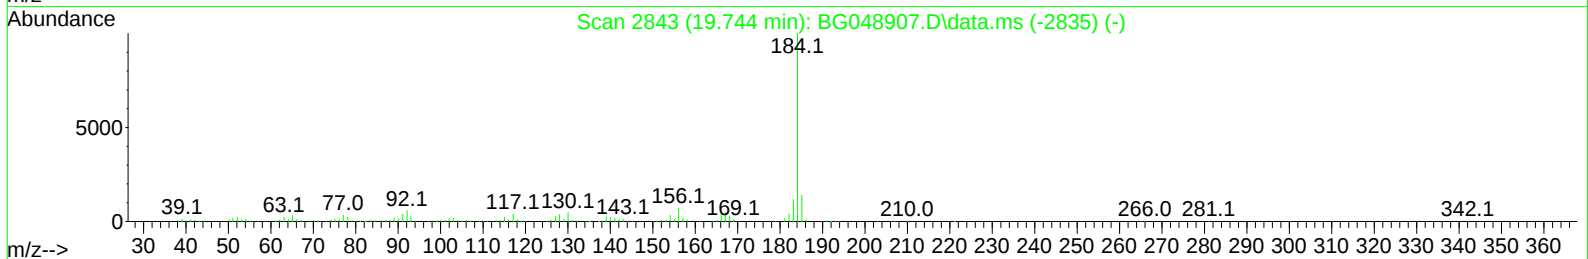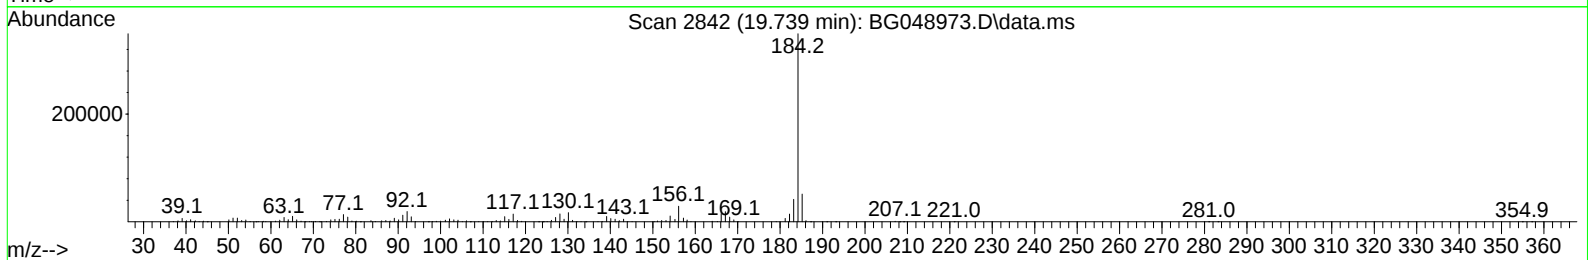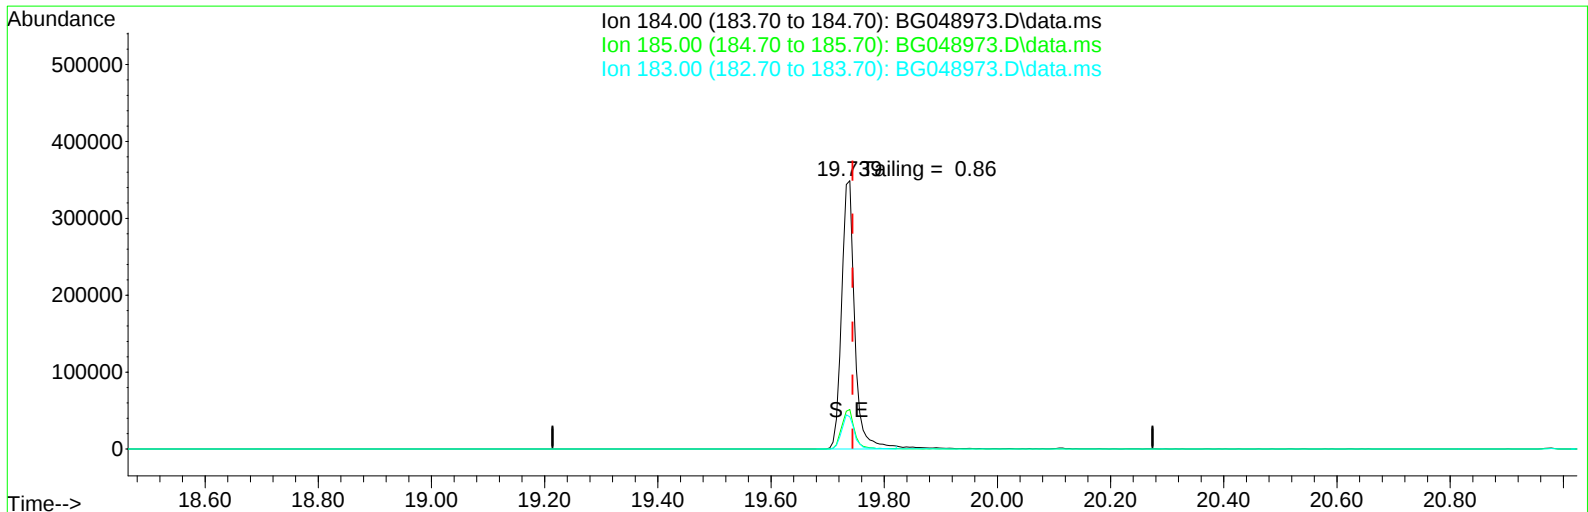

TIC: BG048973.D\data.ms

(77) Benzidine

19.739min (-0.005) 505999.08 ng




response 560633

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.74
183.00	11.70	11.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061521\
Data File : BG048973.D
Acq On : 15 Jun 2021 11:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 15 13:16:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

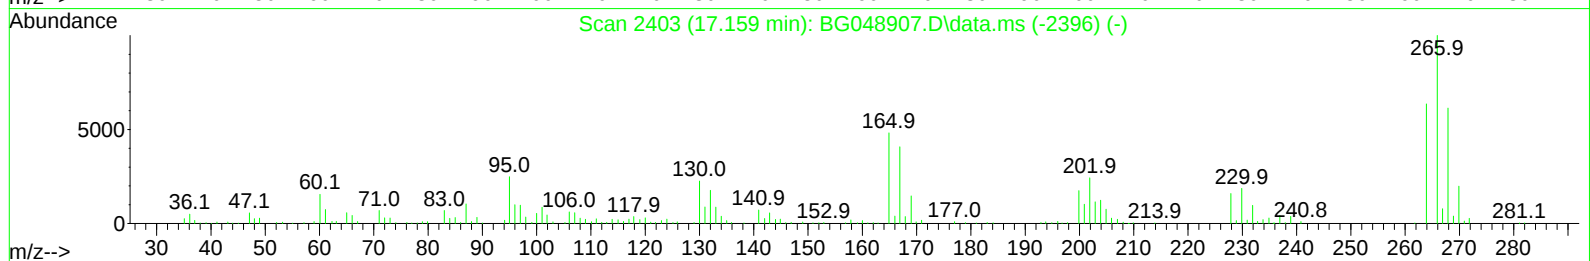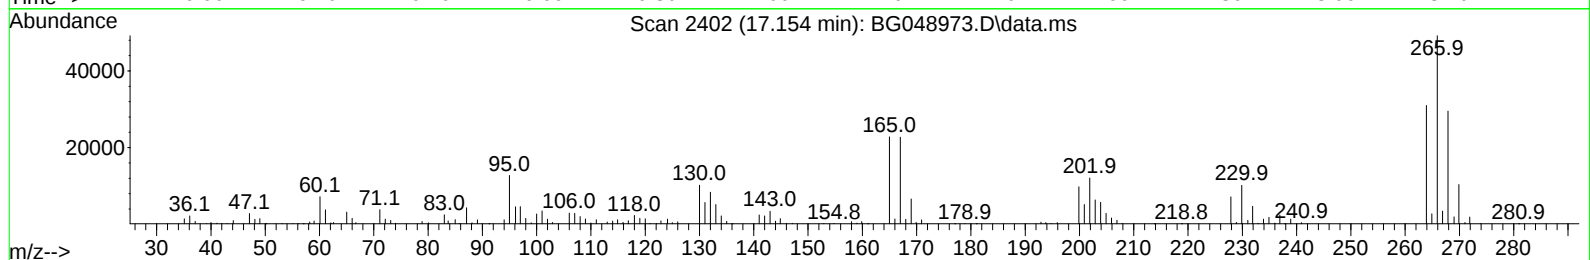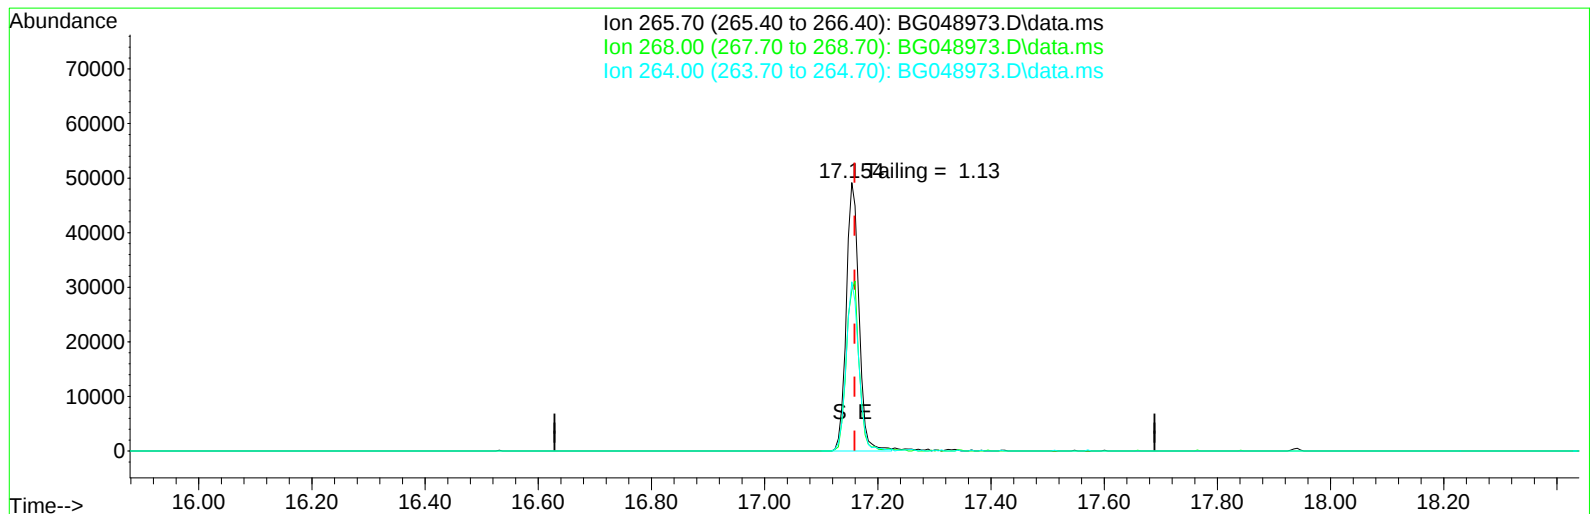

TIC: BG048973.D\data.ms

(70) Pentachlorophenol (C)

17.154min (-0.005) 21649.16 ng

response 76769

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.05
264.00	61.30	63.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/15/2021	BNA_G	BG048973.D
Compound Name	Response	Retention Time
DDT	237537	20.97
DDD	547	20.53
DDE	133	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
680	238217	0.29

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP