
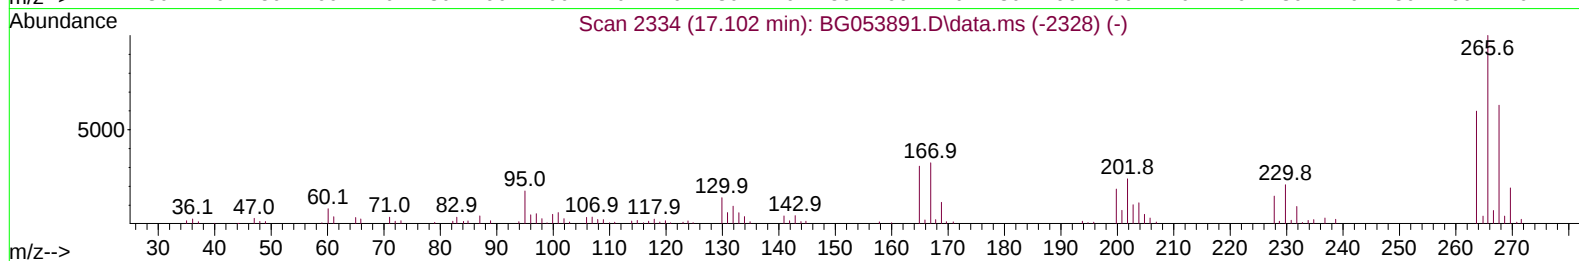
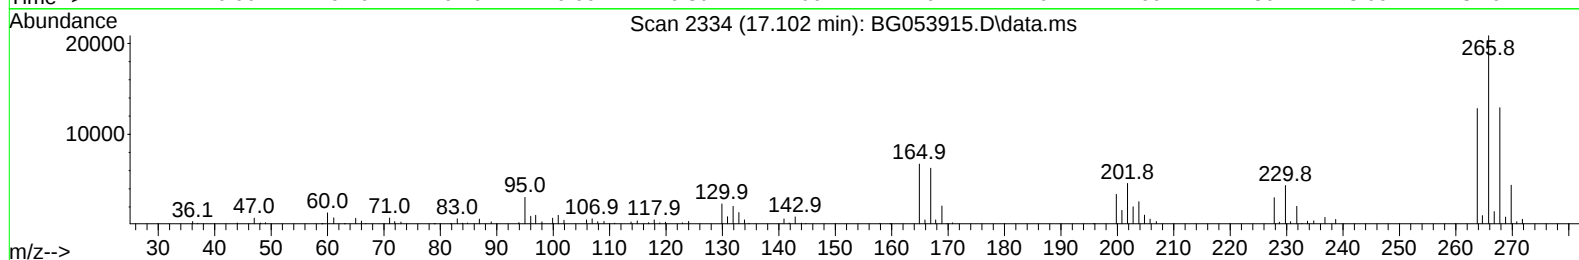


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053915.D
Acq On : 15 Jun 2022 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 17:23:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

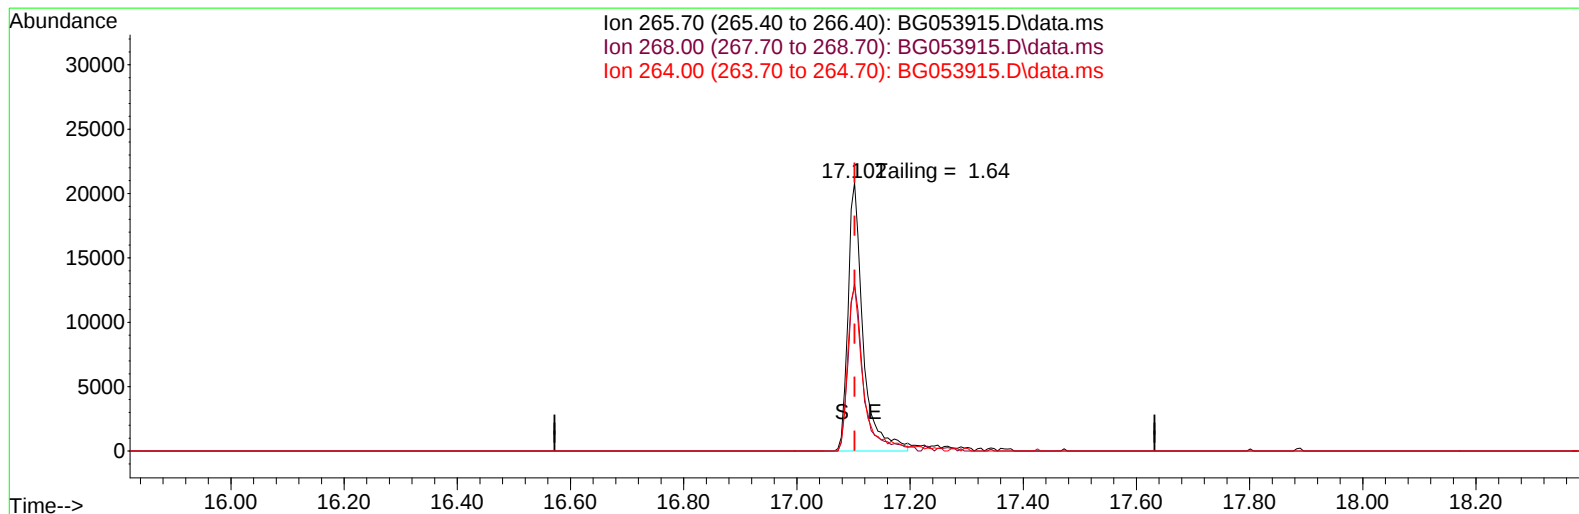

TIC: BG053915.D\data.ms

(70) Pentachlorophenol (C)




17.102min (+ 0.000) 87365.66 ng

response 39426

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.95
264.00	66.20	66.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053915.D
Acq On : 15 Jun 2022 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 17:23:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

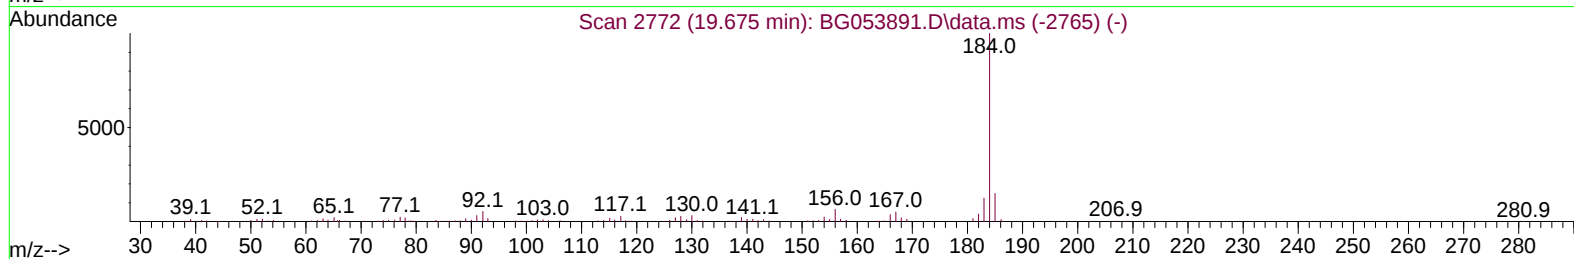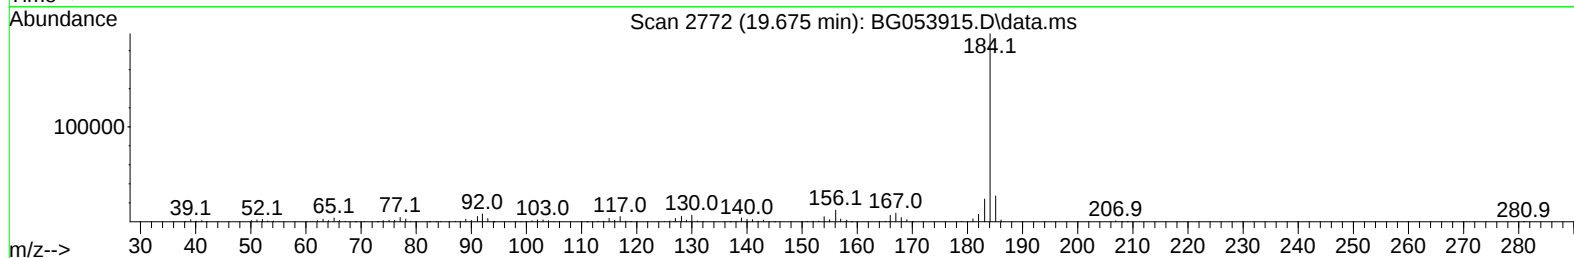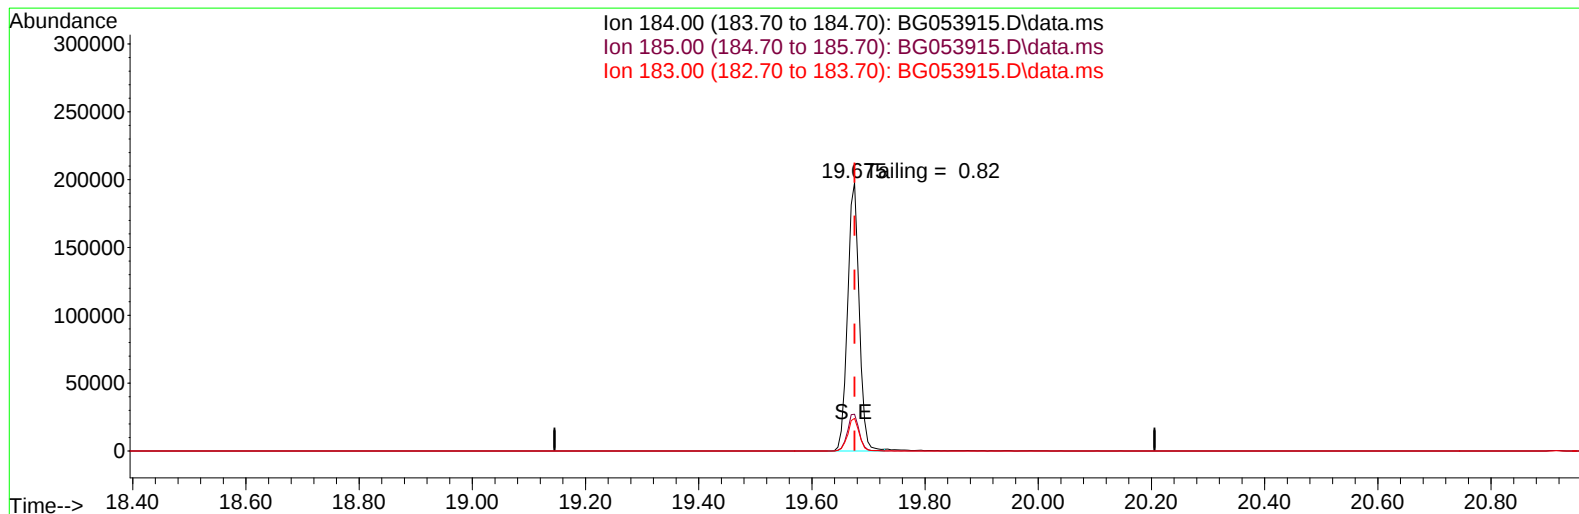

TIC: BG053915.D\data.ms

(77) Benzidine**19.675min (+ 0.000) 0.00 ng****response 283665**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.76
183.00	11.10	12.20
0.00	0.00	0.00