

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
 Data File : BG053926.D
 Acq On : 15 Jun 2022 19:53
 Operator : CG/JU
 Sample : N3354-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-50D

Quant Time: Jun 16 01:26:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 13 15:49:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.083	152	19558	20.000	ng	0.00
21) Naphthalene-d8	10.891	136	78373	20.000	ng	0.00
39) Acenaphthene-d10	14.704	164	59232	20.000	ng	0.00
64) Phenanthrene-d10	17.448	188	159127	20.000	ng	# 0.00
76) Chrysene-d12	21.726	240	194420	20.000	ng	0.00
86) Perylene-d12	24.987	264	202848	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.650	112	76633	74.913	ng	0.00
7) Phenol-d6	7.237	99	63057	45.439	ng	0.00
23) Nitrobenzene-d5	9.240	82	151955	108.957	ng	0.00
42) 2,4,6-Tribromophenol	16.191	330	173228	182.026	ng	0.00
45) 2-Fluorobiphenyl	13.336	172	437200	107.332	ng	0.00
79) Terphenyl-d14	20.057	244	908754	94.142	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053926.D
Acq On : 15 Jun 2022 19:53
Operator : CG/JU
Sample : N3354-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-50D

Quant Time: Jun 16 01:26:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration




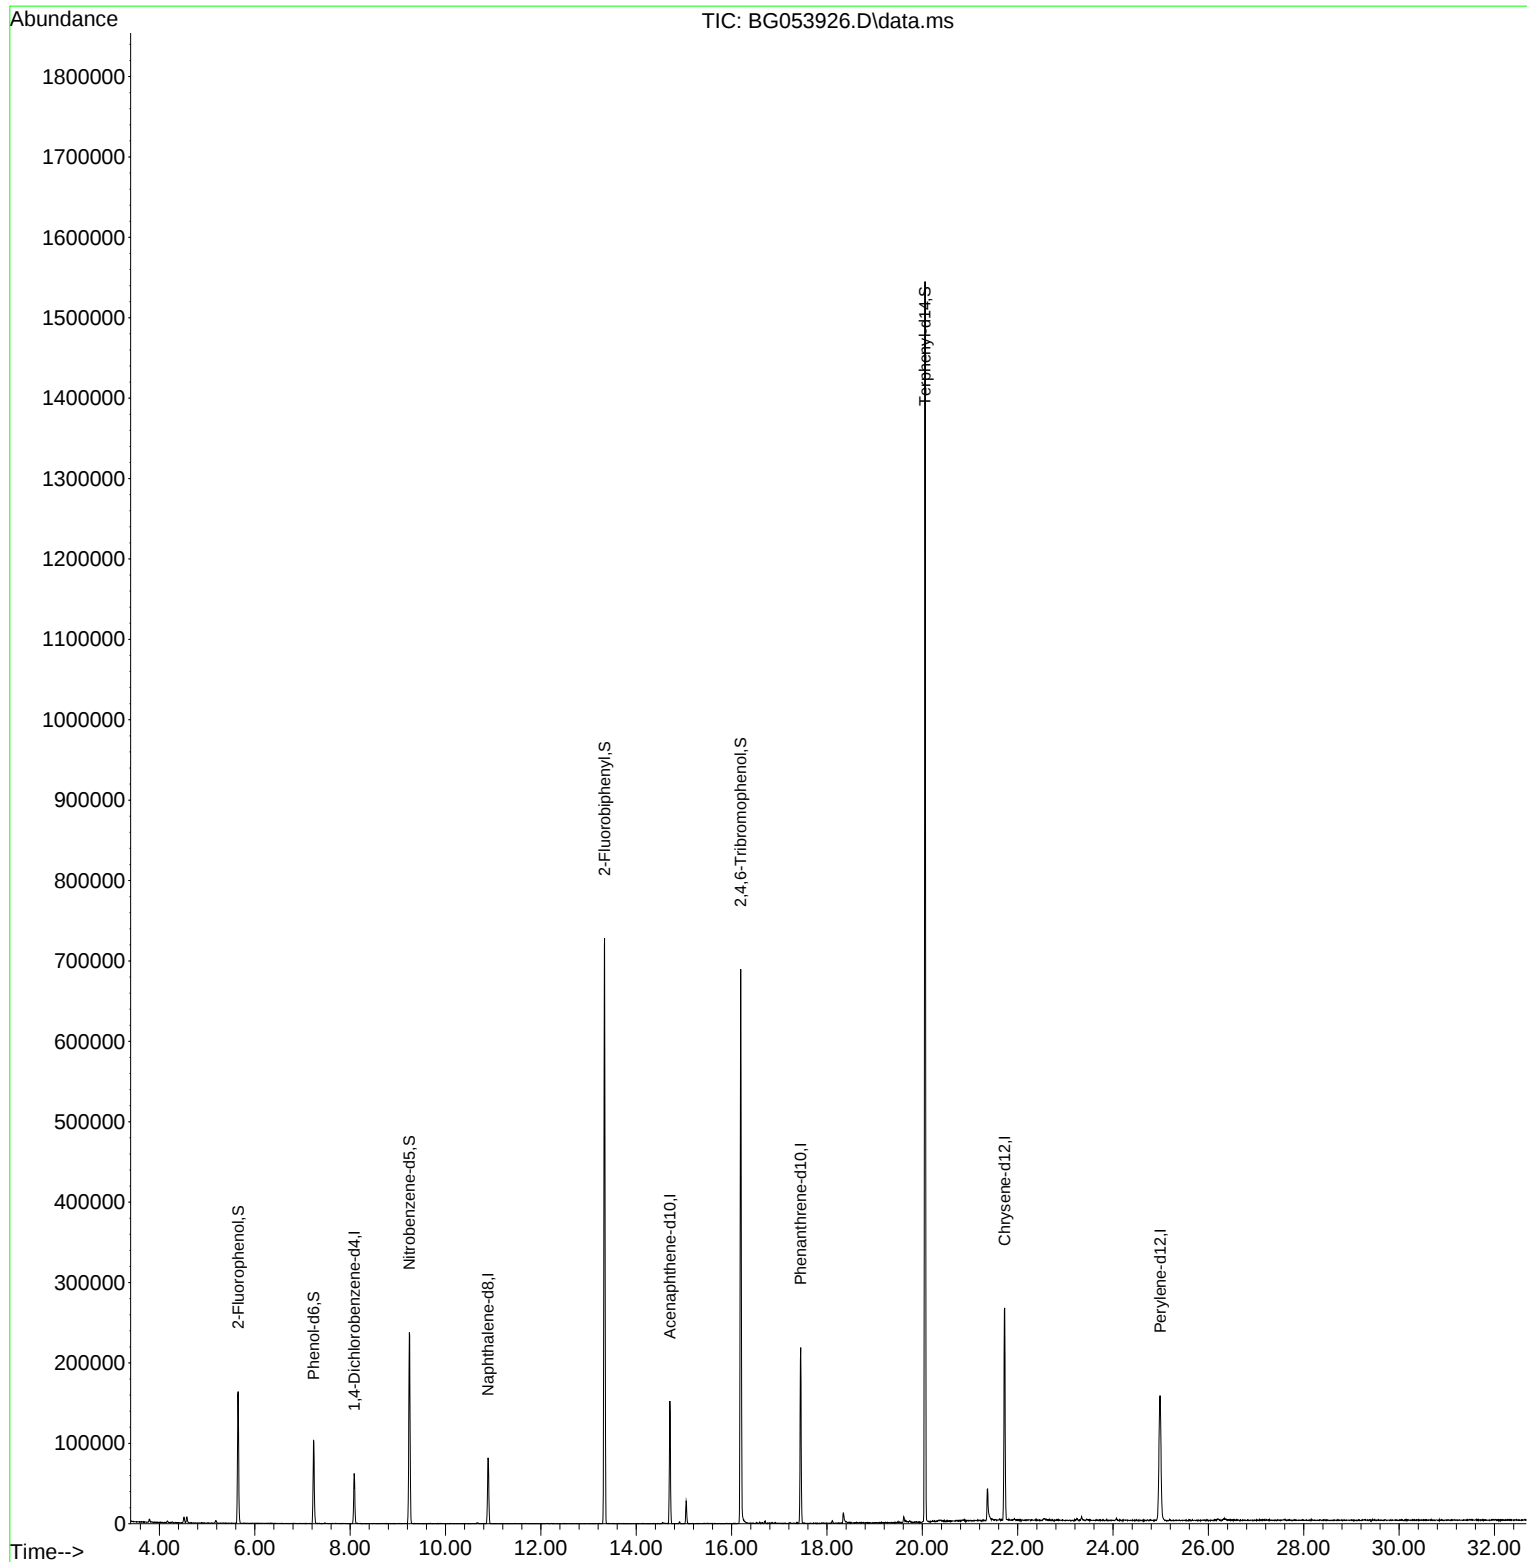


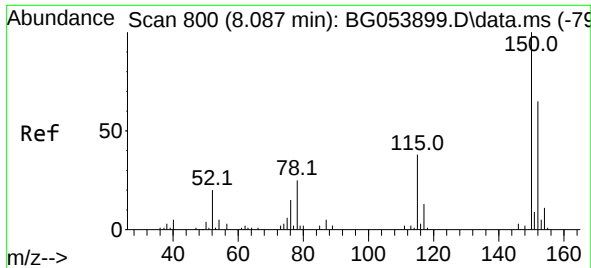

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.083 min Scan# 799
Delta R.T. -0.006 min
Lab File: BG053926.D
Acq: 15 Jun 2022 19:53




Instrument :
BNA_G
ClientSampleId :
MW-50D


Tgt Ion:152 Resp: 19558
Ion Ratio Lower Upper
152 100
150 154.1 131.6 197.4
115 53.6 50.9 76.3

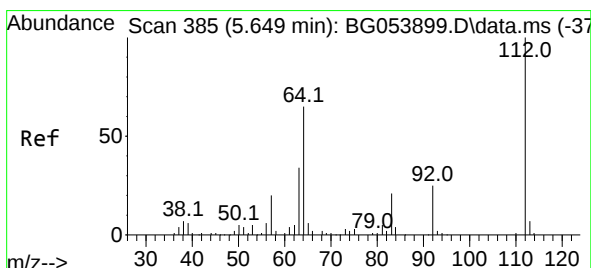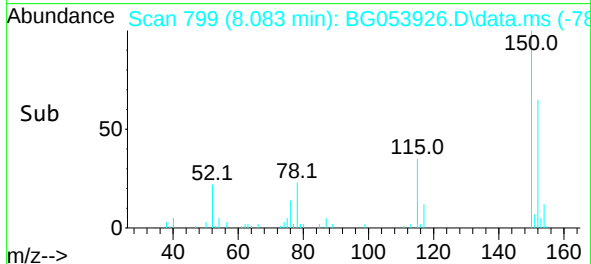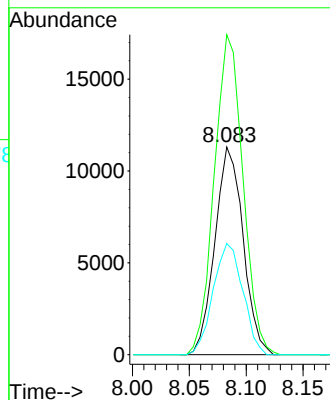

#5
2-Fluorophenol
Concen: 74.913 ng
RT: 5.650 min Scan# 385
Delta R.T. 0.000 min
Lab File: BG053926.D
Acq: 15 Jun 2022 19:53

Tgt Ion:112 Resp: 76633
Ion Ratio Lower Upper
112 100
64 58.8 55.1 82.7
63 34.0 30.4 45.6


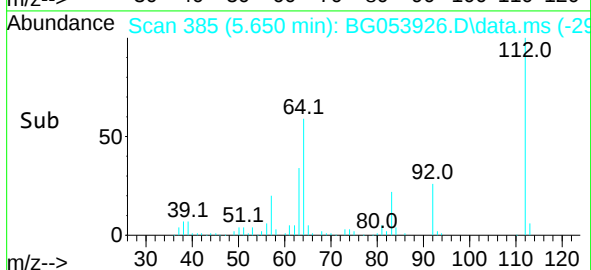
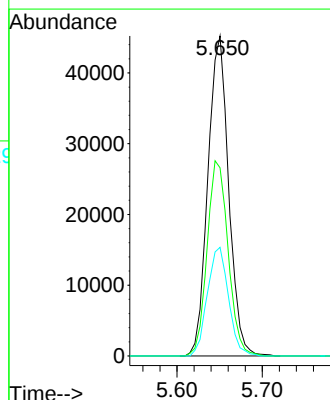
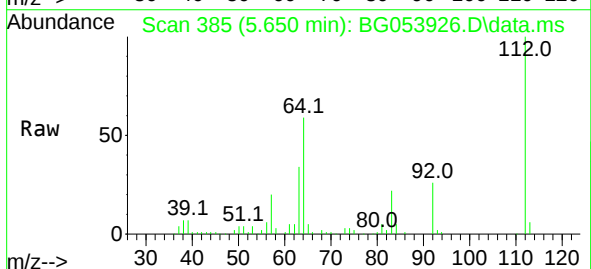


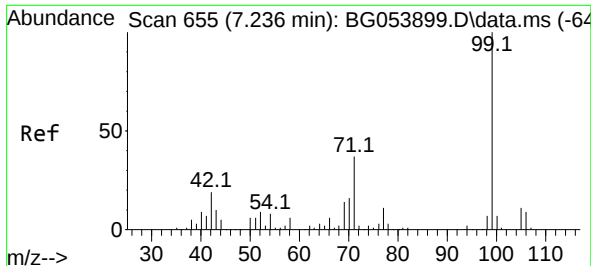

#7
Phenol-d6
Concen: 45.439 ng
RT: 7.237 min Scan# 61
Delta R.T. 0.000 min
Lab File: BG053926.D
Acq: 15 Jun 2022 19:53




Instrument :
BNA_G
ClientSampleId :
MW-50D


Tgt Ion: 99 Resp: 63057
Ion Ratio Lower Upper
99 100
42 18.8 17.0 25.6
71 39.0 33.8 50.8

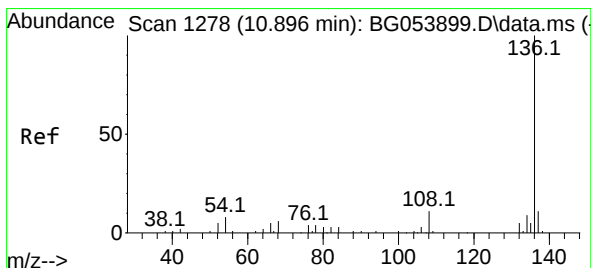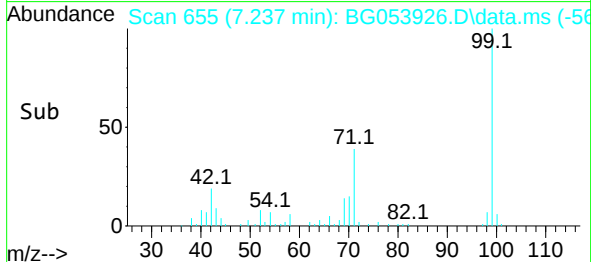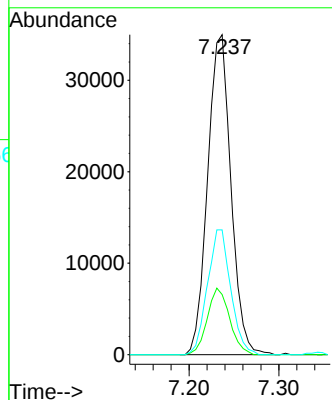

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.891 min Scan# 1277
Delta R.T. -0.006 min
Lab File: BG053926.D
Acq: 15 Jun 2022 19:53

Tgt Ion: 136 Resp: 78373
Ion Ratio Lower Upper
136 100
137 11.5 8.5 12.7
54 7.5 7.4 11.2
68 5.0 4.9 7.3


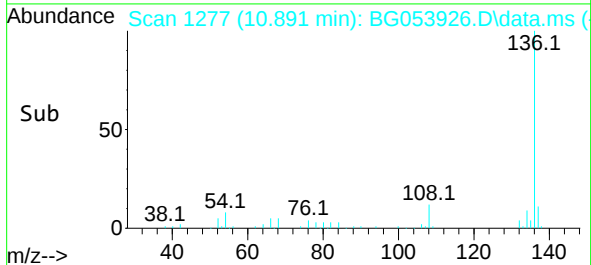
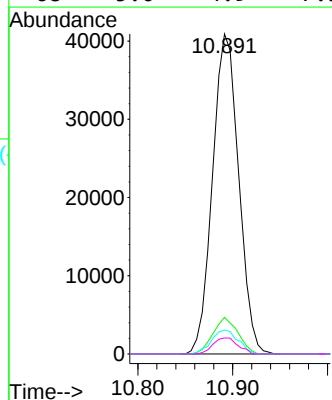
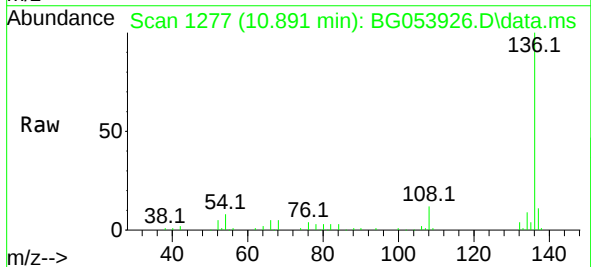


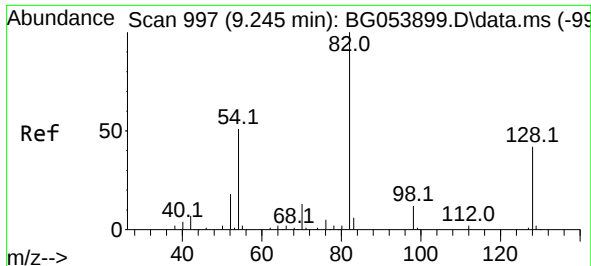

#23
Nitrobenzene-d5
Concen: 108.957 ng
RT: 9.240 min Scan# 997
Delta R.T. -0.006 min
Lab File: BG053926.D
Acq: 15 Jun 2022 19:53




Instrument :
BNA_G
ClientSampleId :
MW-50D


Tgt Ion: 82 Resp: 151955
Ion Ratio Lower Upper
82 100
128 40.4 27.9 41.9
54 53.7 41.2 61.8

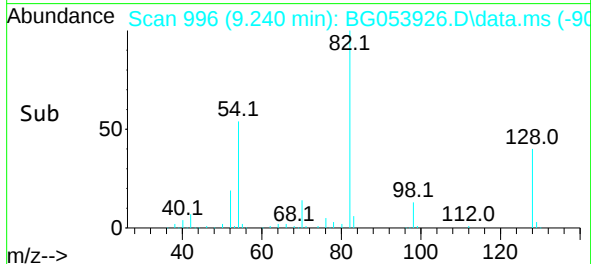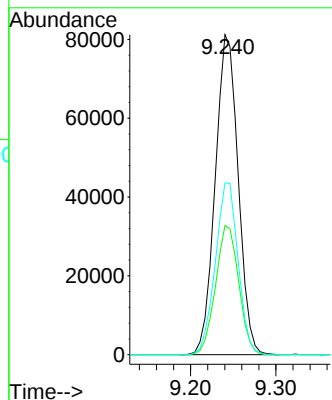

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.704 min Scan# 1926
Delta R.T. -0.006 min
Lab File: BG053926.D
Acq: 15 Jun 2022 19:53

Tgt Ion: 164 Resp: 59232
Ion Ratio Lower Upper
164 100
162 110.0 82.3 123.5
160 45.1 34.2 51.2



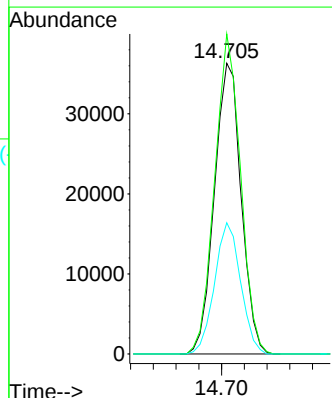
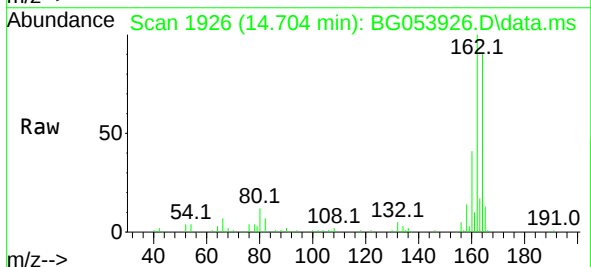


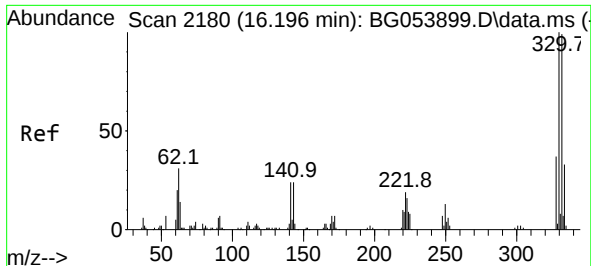

#42
2,4,6-Tribromophenol
Concen: 182.026 ng
RT: 16.191 min Scan# 21
Delta R.T. 0.000 min
Lab File: BG053926.D
Acq: 15 Jun 2022 19:53




Instrument :
BNA_G
ClientSampleId :
MW-50D


Tgt Ion:330 Resp: 173228
Ion Ratio Lower Upper
330 100
332 97.6 76.0 114.0
141 22.9 27.1 40.7#

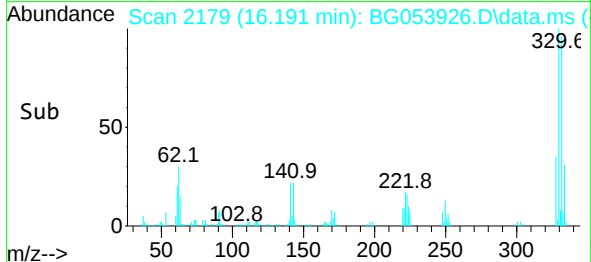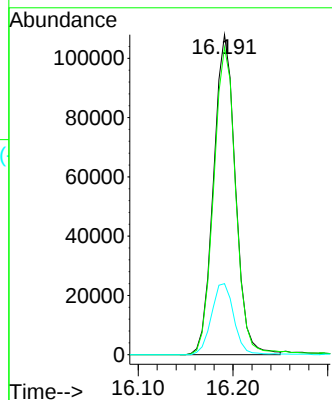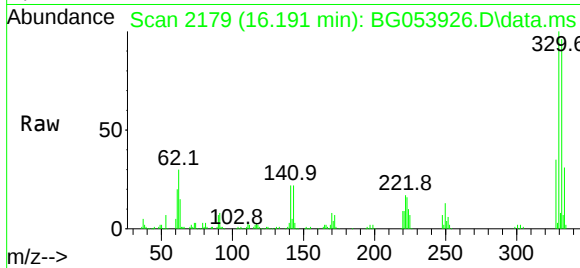

#45
2-Fluorobiphenyl
Concen: 107.332 ng
RT: 13.336 min Scan# 1693
Delta R.T. 0.000 min
Lab File: BG053926.D
Acq: 15 Jun 2022 19:53

Tgt Ion:172 Resp: 437200
Ion Ratio Lower Upper
172 100
171 36.5 28.5 42.7
170 24.5 18.9 28.3


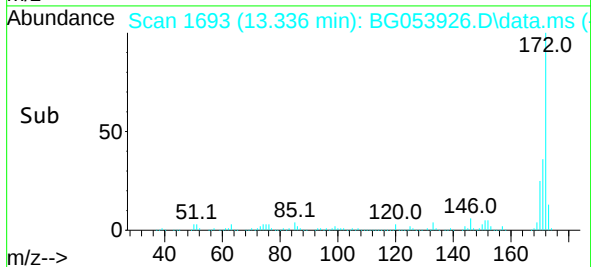
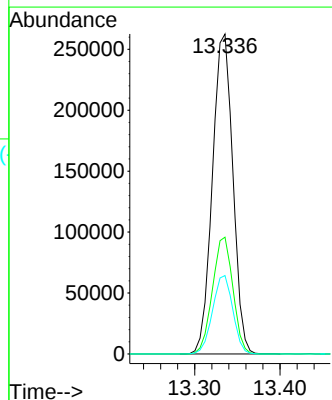
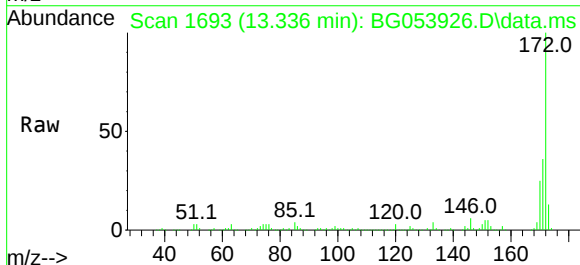


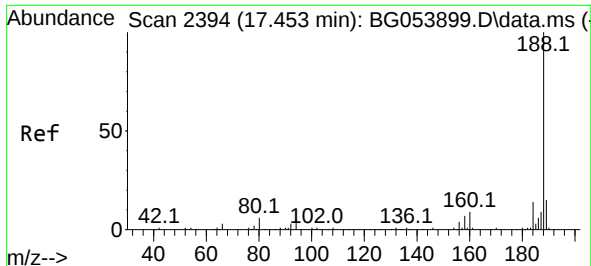

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.448 min Scan# 21
Delta R.T. -0.006 min
Lab File: BG053926.D
Acq: 15 Jun 2022 19:53




Instrument :
BNA_G
ClientSampleId :
MW-50D


Tgt Ion:188 Resp: 159127
Ion Ratio Lower Upper
188 100
94 5.8 5.4 8.0
80 6.0 6.8 10.2#

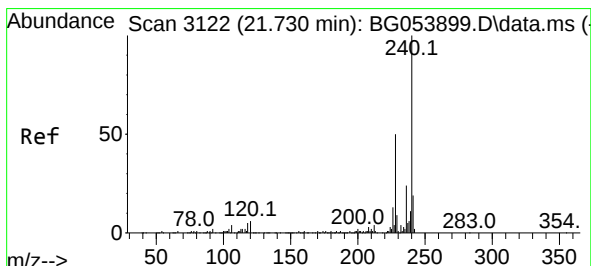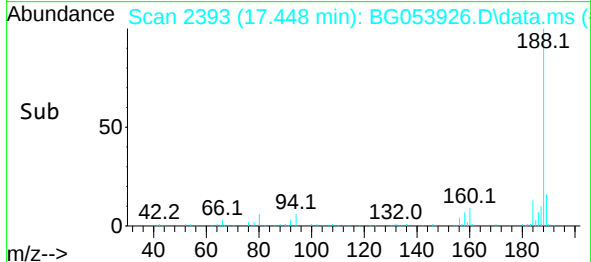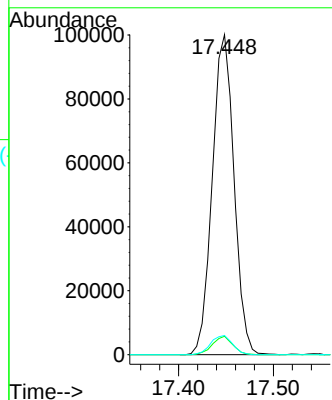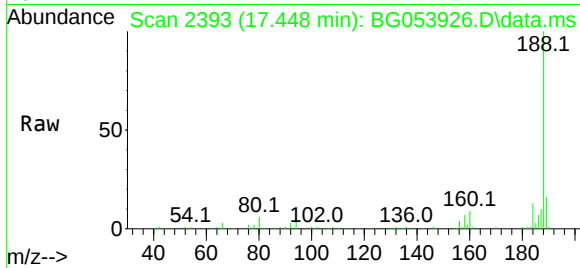

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.726 min Scan# 3121
Delta R.T. -0.006 min
Lab File: BG053926.D
Acq: 15 Jun 2022 19:53

Tgt Ion:240 Resp: 194420
Ion Ratio Lower Upper
240 100
120 5.3 4.6 7.0
236 23.5 20.2 30.4


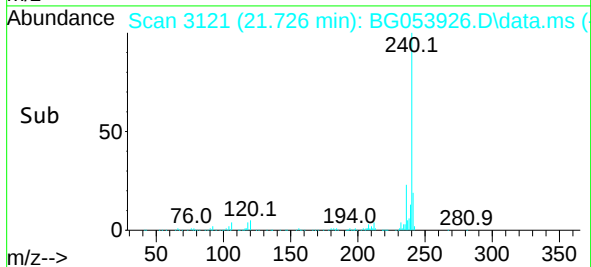
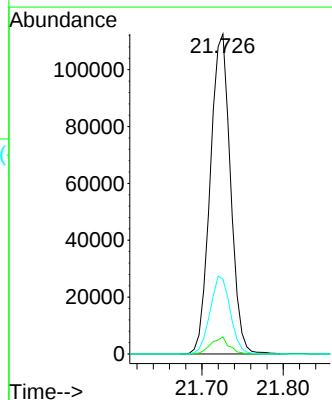
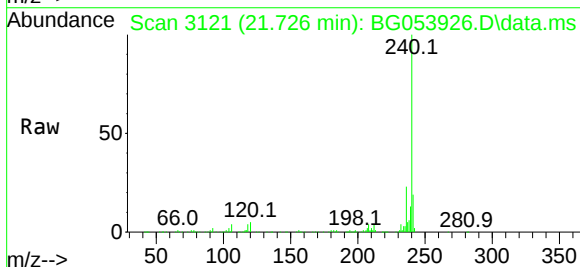




#79
 Terphenyl-d14
 Concen: 94.142 ng
 RT: 20.057 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BG053926.D
 Acq: 15 Jun 2022 19:53

Instrument :
 BNA_G
 ClientSampleId :
 MW-50D

Tgt Ion:244 Resp: 908754
 Ion Ratio Lower Upper
 244 100
 212 7.0 6.5 9.7
 122 5.3 5.0 7.4

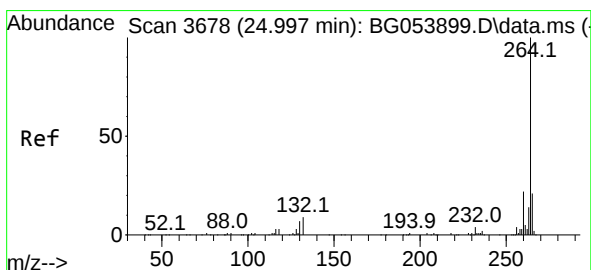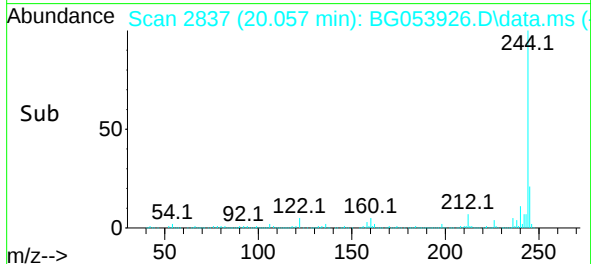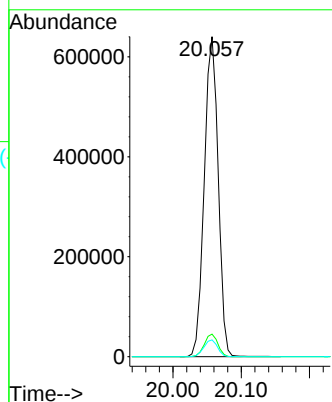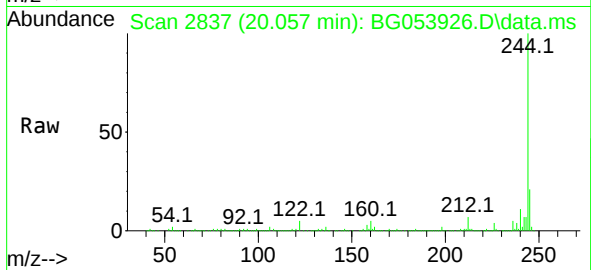

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.987 min Scan# 3676
 Delta R.T. 0.000 min
 Lab File: BG053926.D
 Acq: 15 Jun 2022 19:53

Tgt Ion:264 Resp: 202848
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.0 28.6
 265 22.1 17.4 26.2

