

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
 Data File : BG053927.D
 Acq On : 15 Jun 2022 20:33
 Operator : CG/JU
 Sample : N3354-22
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FB061422

Quant Time: Jun 16 01:26:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 13 15:49:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.087	152	18640	20.000	ng	0.00
21) Naphthalene-d8	10.890	136	73159	20.000	ng	# 0.00
39) Acenaphthene-d10	14.703	164	55754	20.000	ng	0.00
64) Phenanthrene-d10	17.447	188	154248	20.000	ng	# 0.00
76) Chrysene-d12	21.724	240	190107	20.000	ng	0.00
86) Perylene-d12	24.979	264	199429	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.649	112	63094	64.716	ng	0.00
7) Phenol-d6	7.235	99	49828	37.675	ng	0.00
23) Nitrobenzene-d5	9.239	82	135930	104.413	ng	0.00
42) 2,4,6-Tribromophenol	16.190	330	159909	178.512	ng	0.00
45) 2-Fluorobiphenyl	13.334	172	392802	102.448	ng	0.00
79) Terphenyl-d14	20.056	244	982997	104.143	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053927.D
Acq On : 15 Jun 2022 20:33
Operator : CG/JU
Sample : N3354-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB061422

Quant Time: Jun 16 01:26:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration




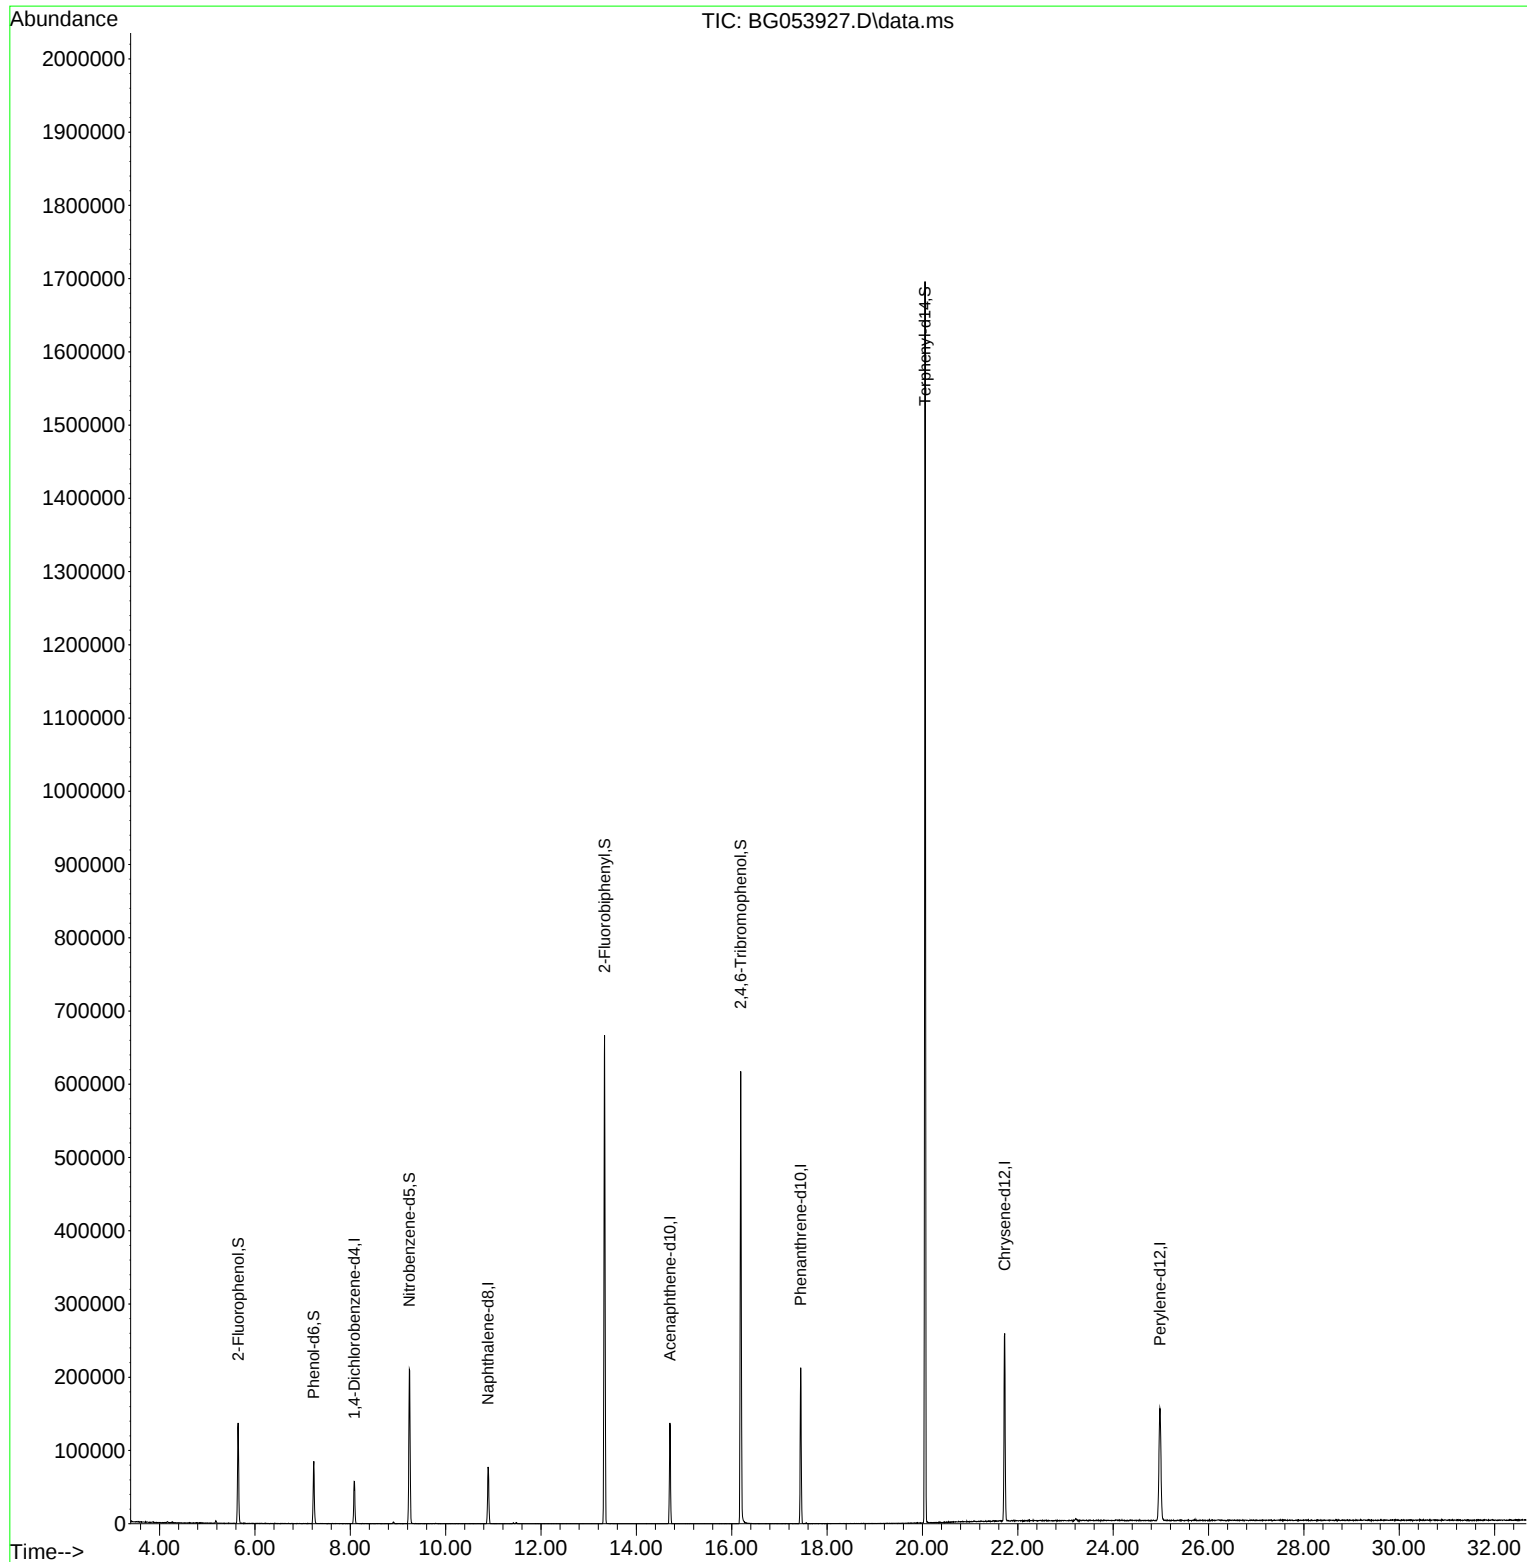


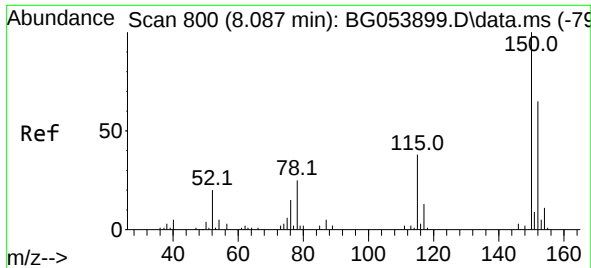

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.087 min Scan# 80
Delta R.T. -0.002 min
Lab File: BG053927.D
Acq: 15 Jun 2022 20:33




Instrument :
BNA_G
ClientSampleId :
FB061422


Tgt Ion:152 Resp: 18640
Ion Ratio Lower Upper
152 100
150 151.3 131.6 197.4
115 53.8 50.9 76.3

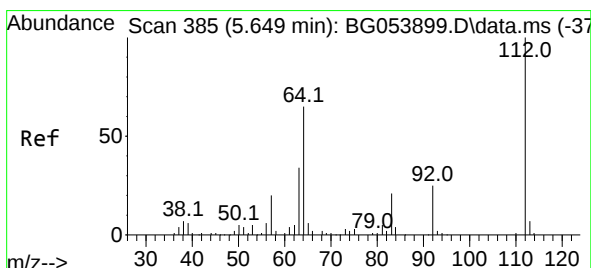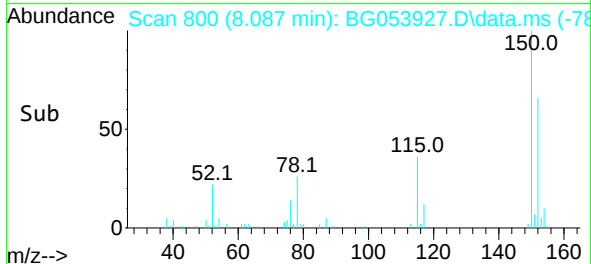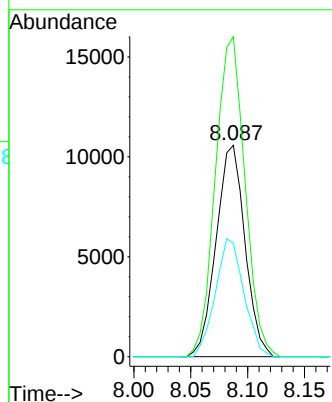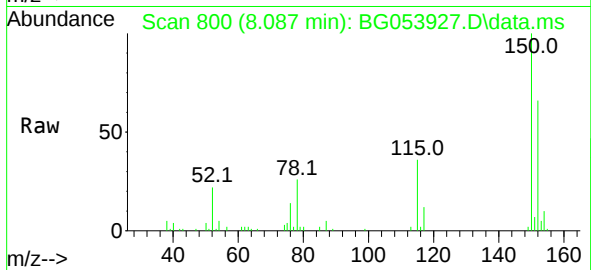

#5
2-Fluorophenol
Concen: 64.716 ng
RT: 5.649 min Scan# 385
Delta R.T. -0.001 min
Lab File: BG053927.D
Acq: 15 Jun 2022 20:33

Tgt Ion:112 Resp: 63094
Ion Ratio Lower Upper
112 100
64 61.8 55.1 82.7
63 35.3 30.4 45.6


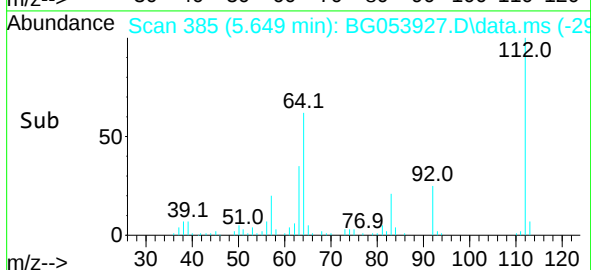
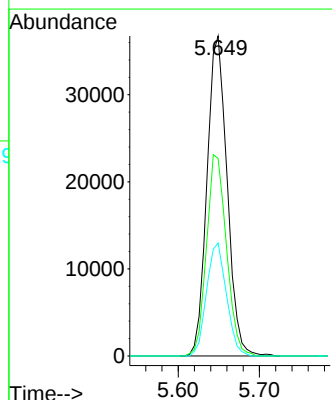
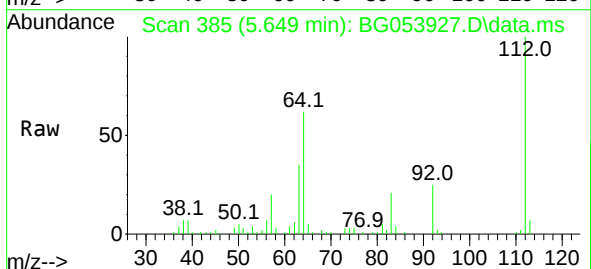


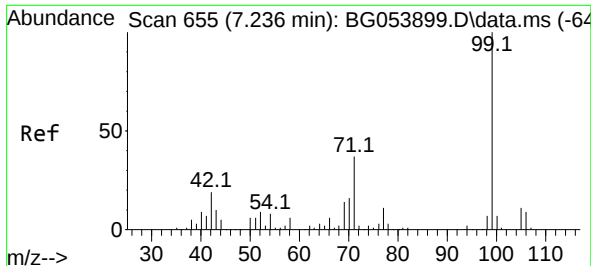

#7
Phenol-d6
Concen: 37.675 ng
RT: 7.235 min Scan# 61
Delta R.T. -0.001 min
Lab File: BG053927.D
Acq: 15 Jun 2022 20:33




Instrument :
BNA_G
ClientSampleId :
FB061422


Tgt Ion: 99 Resp: 49828
Ion Ratio Lower Upper
99 100
42 21.4 17.0 25.6
71 40.4 33.8 50.8

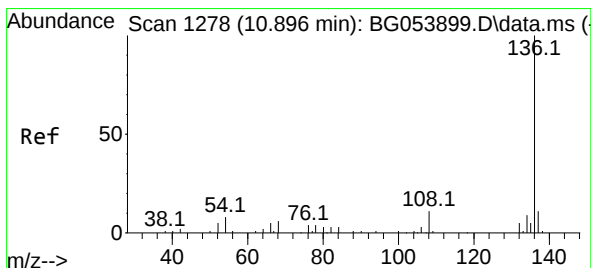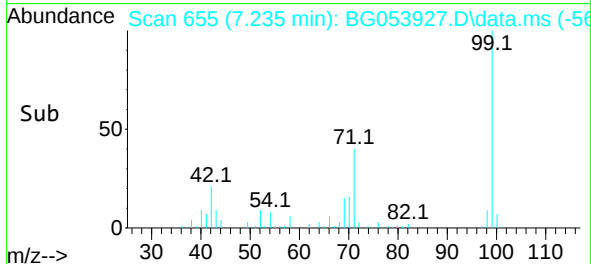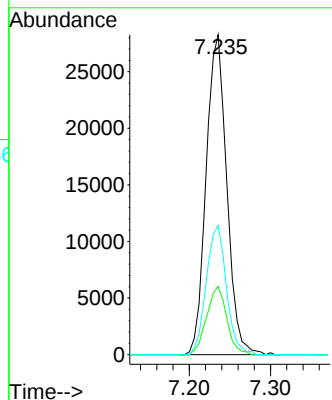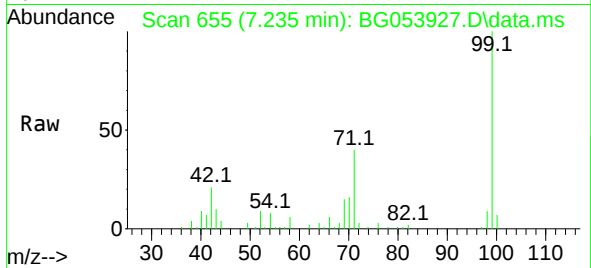

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.890 min Scan# 1277
Delta R.T. -0.007 min
Lab File: BG053927.D
Acq: 15 Jun 2022 20:33

Tgt Ion: 136 Resp: 73159
Ion Ratio Lower Upper
136 100
137 10.6 8.5 12.7
54 7.8 7.4 11.2
68 4.4 4.9 7.3#


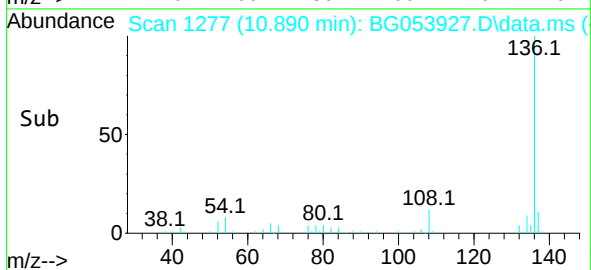
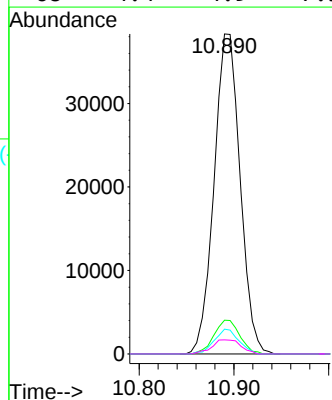
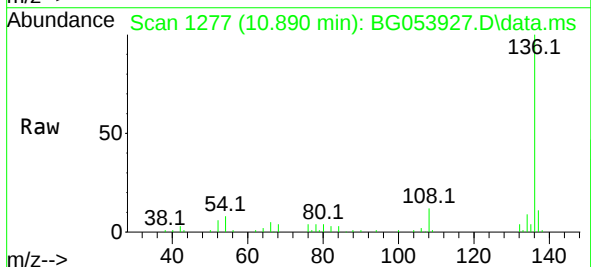


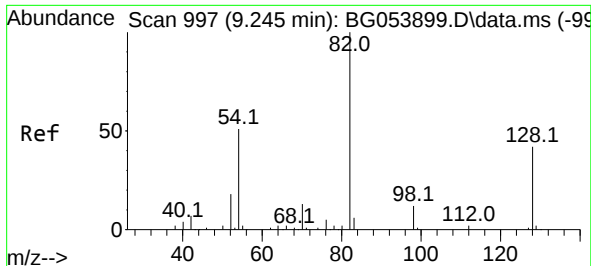

#23
Nitrobenzene-d5
Concen: 104.413 ng
RT: 9.239 min Scan# 996
Delta R.T. -0.007 min
Lab File: BG053927.D
Acq: 15 Jun 2022 20:33




Instrument :
BNA_G
ClientSampleId :
FB061422


Tgt Ion: 82 Resp: 135930
Ion Ratio Lower Upper
82 100
128 41.4 27.9 41.9
54 51.9 41.2 61.8

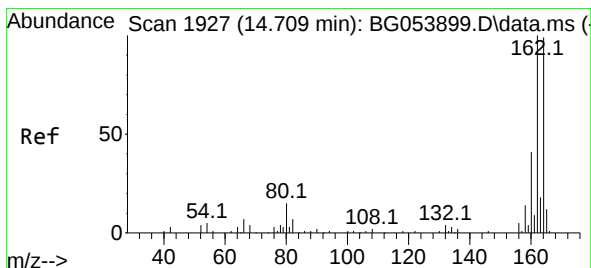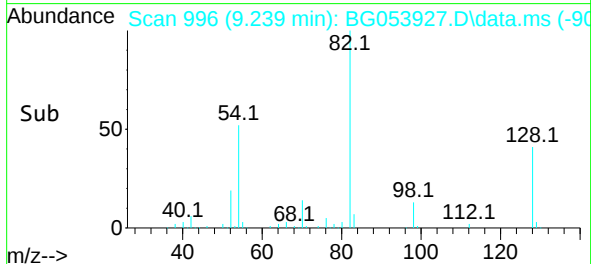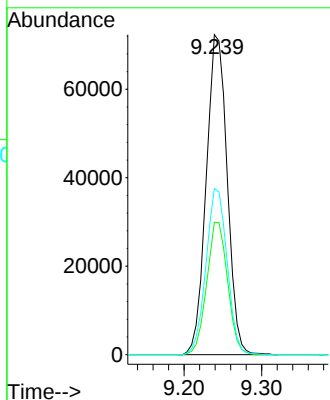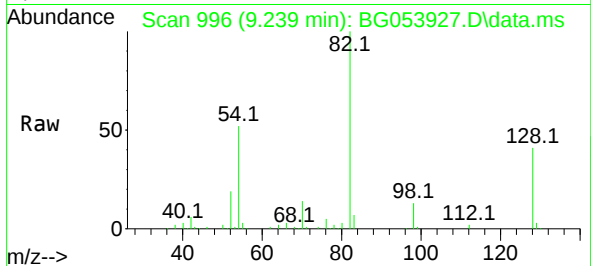

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.703 min Scan# 1926
Delta R.T. -0.007 min
Lab File: BG053927.D
Acq: 15 Jun 2022 20:33

Tgt Ion:164 Resp: 55754
Ion Ratio Lower Upper
164 100
162 103.7 82.3 123.5
160 44.2 34.2 51.2


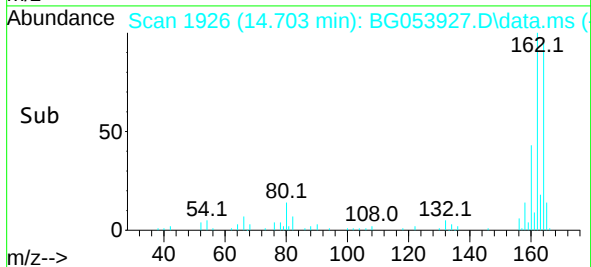
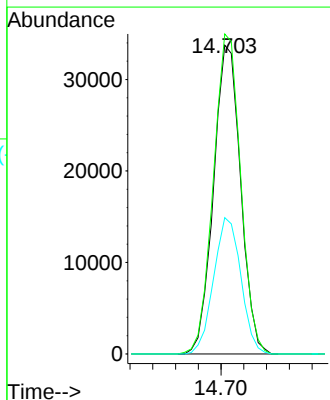
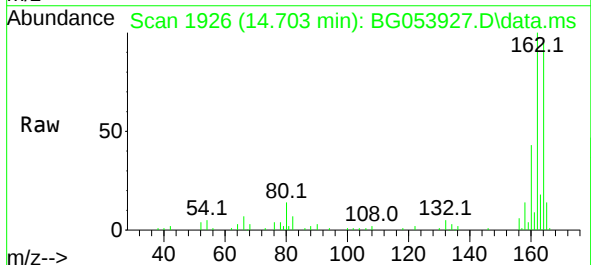


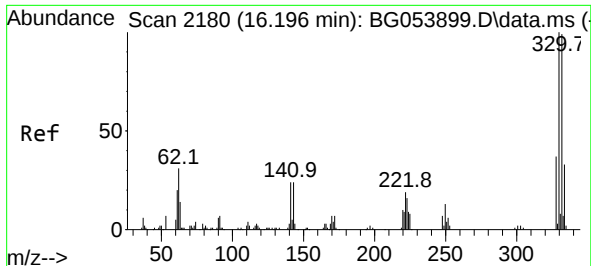

#42
2,4,6-Tribromophenol
Concen: 178.512 ng
RT: 16.190 min Scan# 21
Delta R.T. -0.001 min
Lab File: BG053927.D
Acq: 15 Jun 2022 20:33




Instrument :
BNA_G
ClientSampleId :
FB061422


Tgt Ion:330 Resp: 159909
Ion Ratio Lower Upper
330 100
332 95.9 76.0 114.0
141 22.1 27.1 40.7#

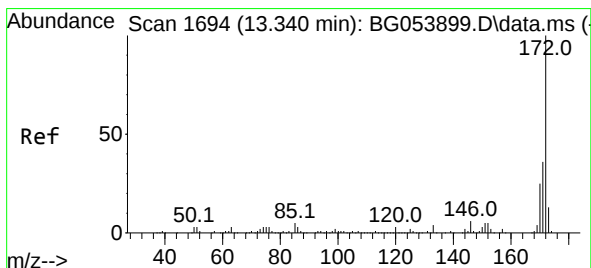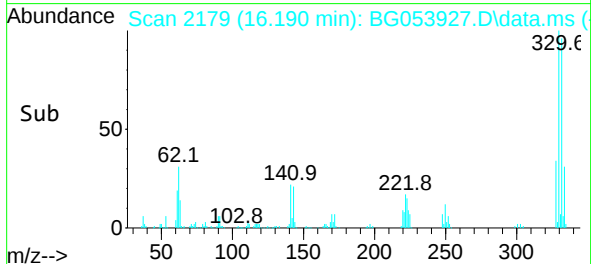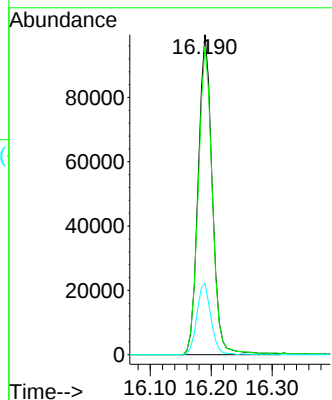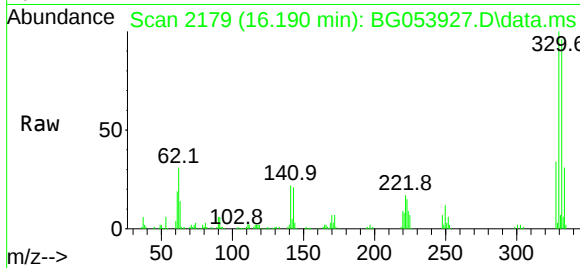

#45
2-Fluorobiphenyl
Concen: 102.448 ng
RT: 13.334 min Scan# 1693
Delta R.T. -0.001 min
Lab File: BG053927.D
Acq: 15 Jun 2022 20:33

Tgt Ion:172 Resp: 392802
Ion Ratio Lower Upper
172 100
171 37.2 28.5 42.7
170 24.0 18.9 28.3


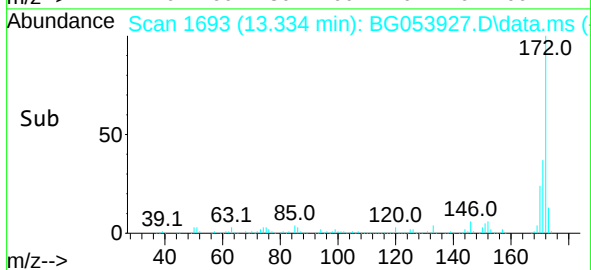
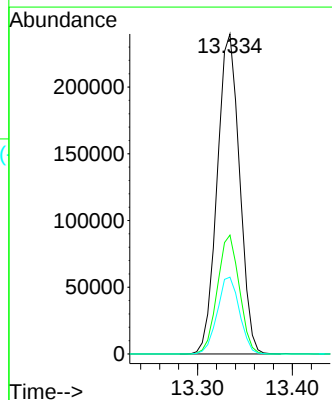
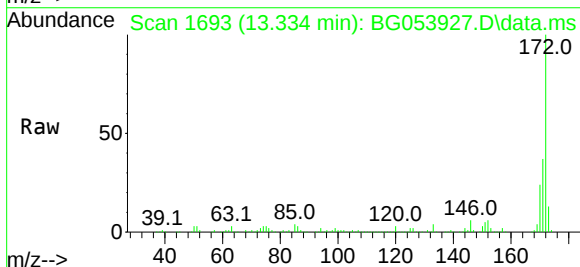


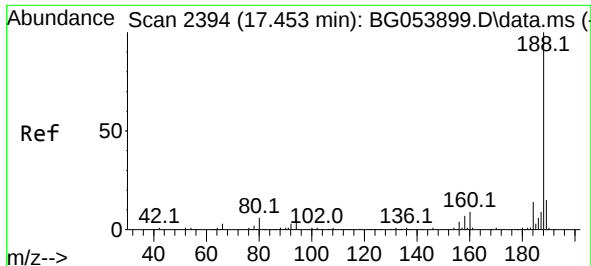

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.447 min Scan# 21
Delta R.T. -0.007 min
Lab File: BG053927.D
Acq: 15 Jun 2022 20:33




Instrument :
BNA_G
ClientSampleId :
FB061422


Tgt Ion:188 Resp: 154248
Ion Ratio Lower Upper
188 100
94 4.9 5.4 8.0#
80 5.6 6.8 10.2#

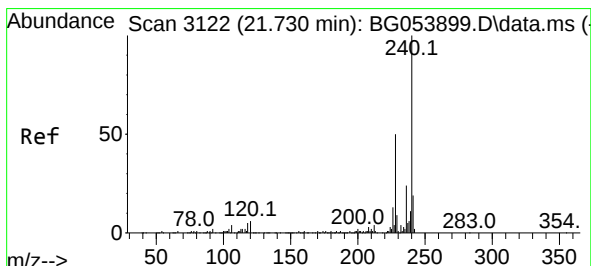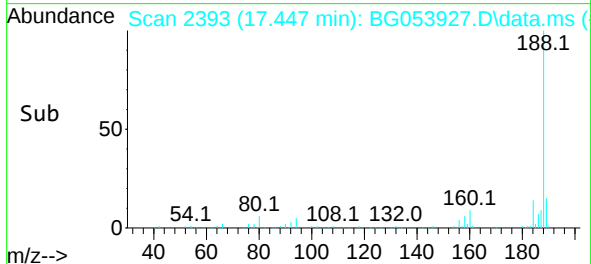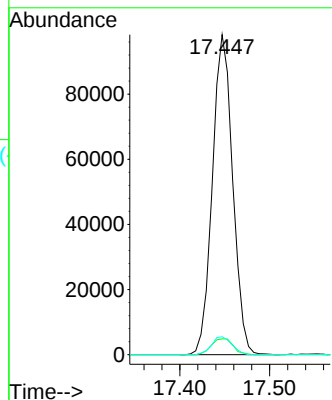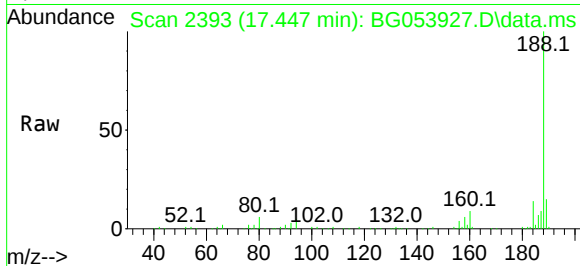

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.724 min Scan# 3121
Delta R.T. -0.007 min
Lab File: BG053927.D
Acq: 15 Jun 2022 20:33

Tgt Ion:240 Resp: 190107
Ion Ratio Lower Upper
240 100
120 4.9 4.6 7.0
236 25.3 20.2 30.4

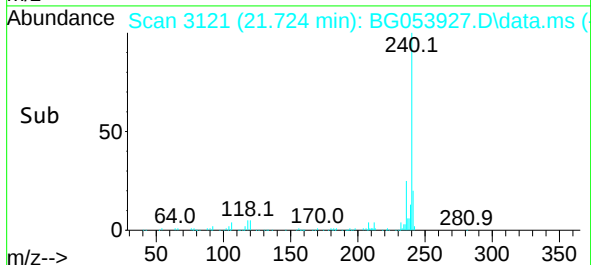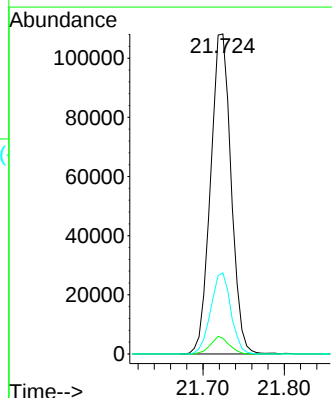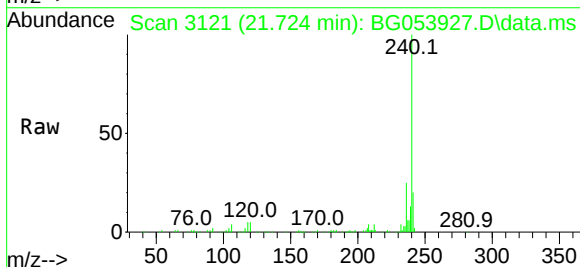

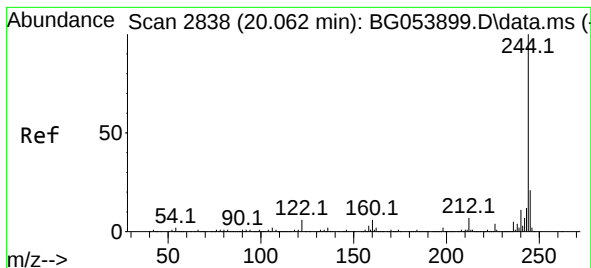

#79

Terphenyl-d14

Concen: 104.143 ng

RT: 20.056 min Scan# 21

Delta R.T. -0.001 min

Lab File: BG053927.D

Acq: 15 Jun 2022 20:33

Instrument :

BNA_G

ClientSampleId :

FB061422





Tgt Ion:244 Resp: 982997

Ion Ratio Lower Upper

244 100

212 7.2 6.5 9.7

122 5.3 5.0 7.4

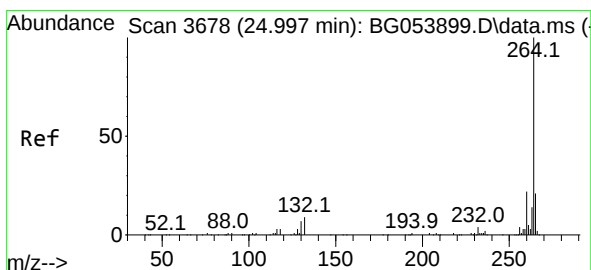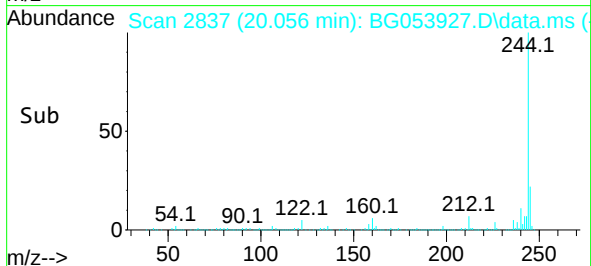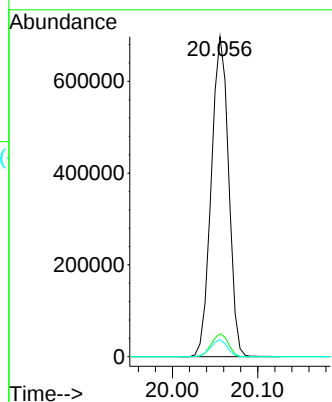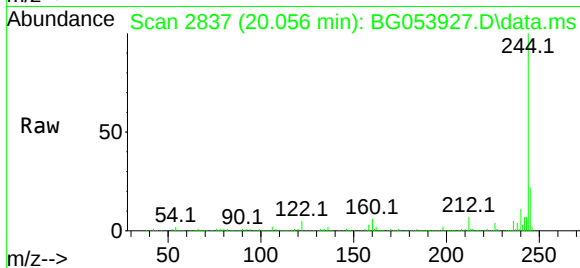

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.979 min Scan# 3675

Delta R.T. -0.007 min

Lab File: BG053927.D

Acq: 15 Jun 2022 20:33

Tgt Ion:264 Resp: 199429

Ion Ratio Lower Upper

264 100

260 23.6 19.0 28.6

265 20.9 17.4 26.2

