

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
 Data File : BG053927.D
 Acq On : 15 Jun 2022 20:33
 Operator : CG/JU
 Sample : N3354-22
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FB061422

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053927.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.649	377	385	394	rBV	137268	232413	9.95%	3.378%
2	7.235	648	655	666	rBV	85113	147858	6.33%	2.149%
3	8.082	793	799	807	rBV	57657	101724	4.36%	1.479%
4	9.239	989	996	1008	rBV	210782	398296	17.06%	5.790%
5	10.890	1270	1277	1286	rBB	77586	144604	6.19%	2.102%
6	13.334	1685	1693	1702	rBV	666627	1083521	46.41%	15.750%
7	14.703	1918	1926	1933	rBB	137574	226379	9.70%	3.291%
8	16.190	2172	2179	2200	rBV	617536	984653	42.17%	14.313%
9	17.447	2386	2393	2400	rBV	212955	328209	14.06%	4.771%
10	20.056	2831	2837	2843	rBV	1694508	2334912	100.00%	33.941%
11	21.724	3114	3121	3129	rVB	255726	441295	18.90%	6.415%
12	24.979	3662	3675	3689	rBV2	153634	455509	19.51%	6.621%




Sum of corrected areas: 6879373

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053927.D
Acq On : 15 Jun 2022 20:33
Operator : CG/JU
Sample : N3354-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB061422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

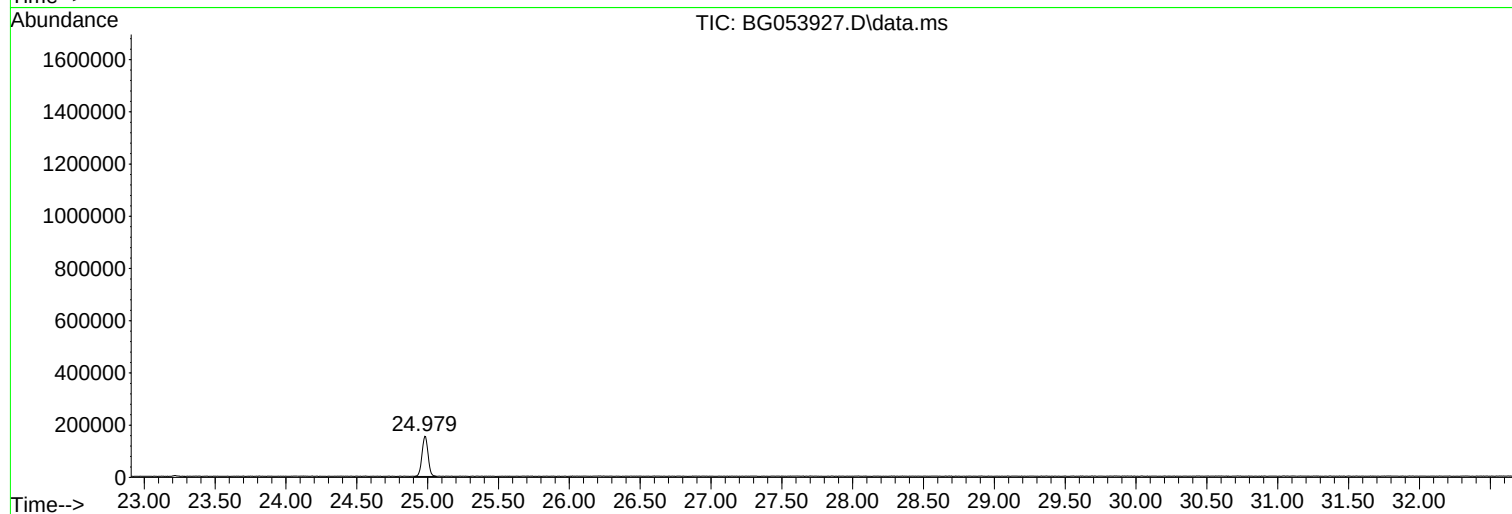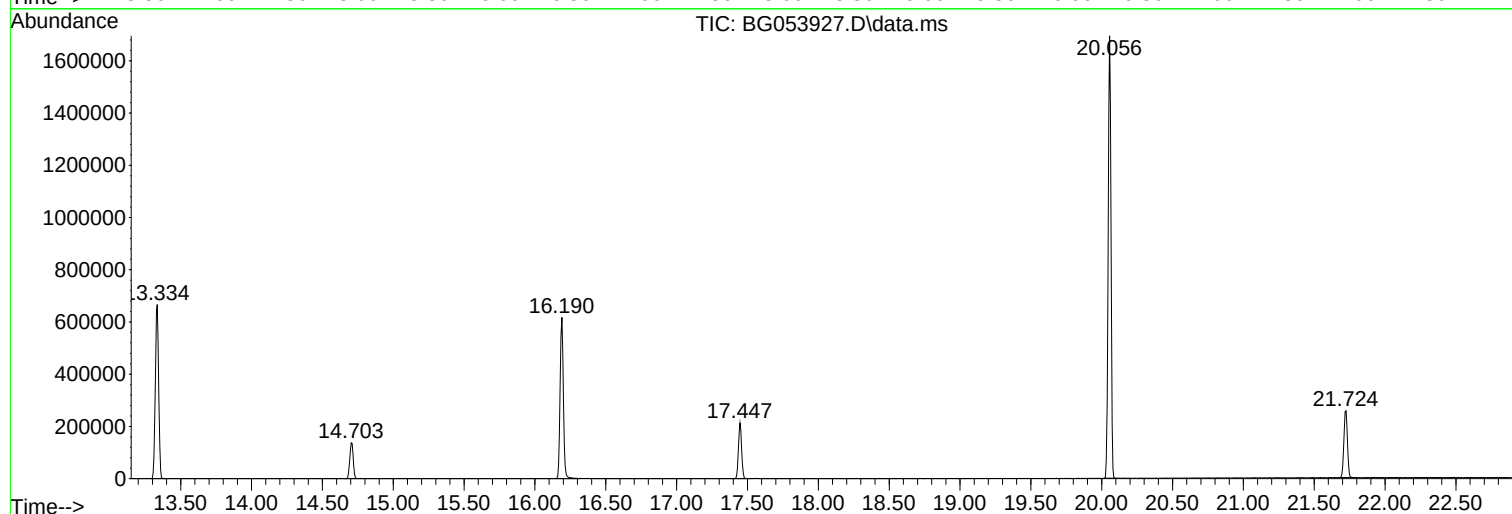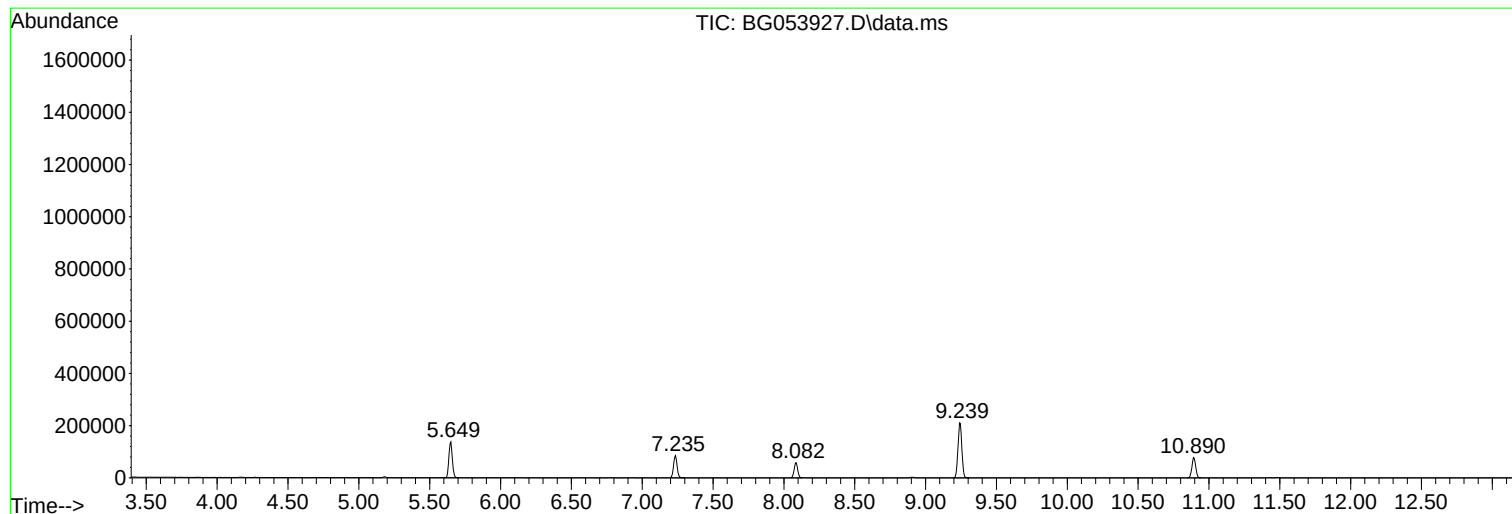

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053927.D
Acq On : 15 Jun 2022 20:33
Operator : CG/JU
Sample : N3354-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB061422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053927.D
Acq On : 15 Jun 2022 20:33
Operator : CG/JU
Sample : N3354-22
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB061422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------