

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
 Data File : BG053928.D
 Acq On : 15 Jun 2022 21:12
 Operator : CG/JU
 Sample : N3354-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-46

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG053928.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.644	377	384	396	rBV	158386	272565	12.66%	3.843%
2	7.230	648	654	662	rBV	96061	174634	8.11%	2.462%
3	8.082	792	799	807	rBB	64301	110358	5.13%	1.556%
4	9.245	988	997	1005	rBV	235902	439088	20.39%	6.191%
5	10.891	1269	1277	1286	rBB	84310	158863	7.38%	2.240%
6	13.335	1685	1693	1704	rBB	729496	1190054	55.27%	16.780%
7	14.704	1918	1926	1934	rBV	157182	248924	11.56%	3.510%
8	16.190	2172	2179	2192	rBV	643477	1030608	47.86%	14.531%
9	17.448	2386	2393	2401	rBV	225426	348498	16.18%	4.914%
10	20.056	2830	2837	2843	rBV	1557976	2153320	100.00%	30.362%
11	21.367	3055	3060	3072	rBV2	34004	62966	2.92%	0.888%
12	21.725	3110	3121	3128	rBV2	252567	442082	20.53%	6.233%
13	24.986	3664	3676	3692	rVB2	151633	460285	21.38%	6.490%




Sum of corrected areas: 7092245

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053928.D
Acq On : 15 Jun 2022 21:12
Operator : CG/JU
Sample : N3354-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-46

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

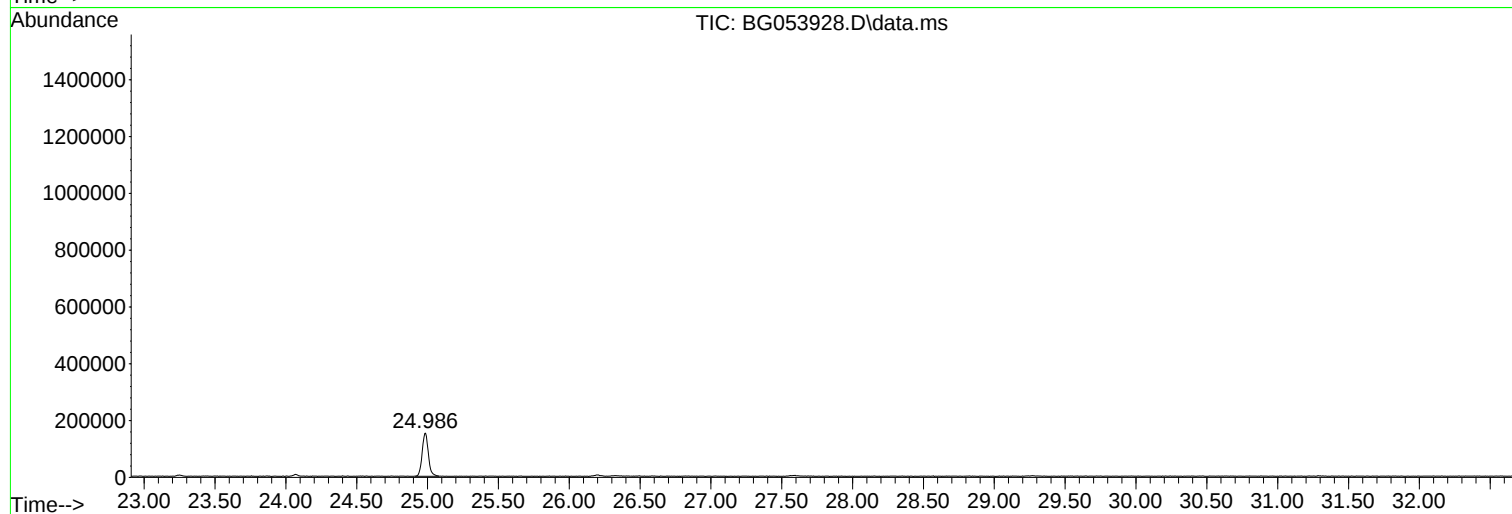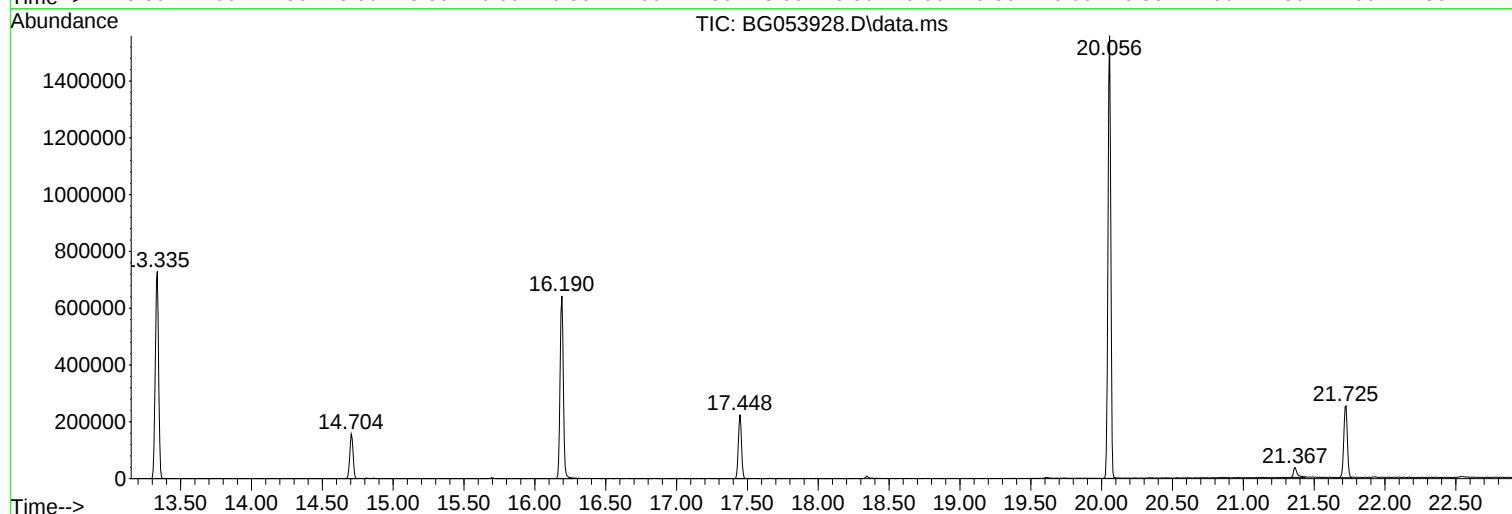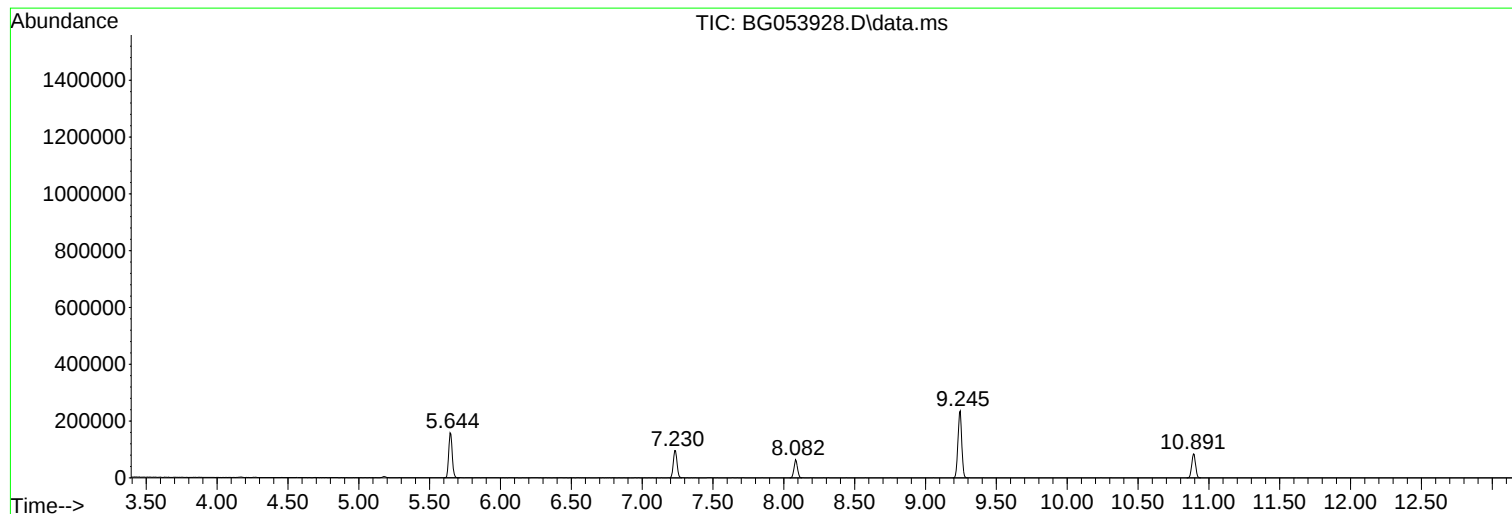

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053928.D
Acq On : 15 Jun 2022 21:12
Operator : CG/JU
Sample : N3354-01
Misc :
ALS Vial : 14 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
MW-46

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentafluoropropionic acid, ... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.366	2.85 ng	62966	Chrysene-d12	21.725	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94
2	Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
3	1-Tetracosene	336	C24H48	010192-32-2	91
4	Behenic alcohol	326	C22H46O	000661-19-8	91
5	Heptafluorobutyric acid, hexadec...	438	C20H33F7O2	006385-15-5	90

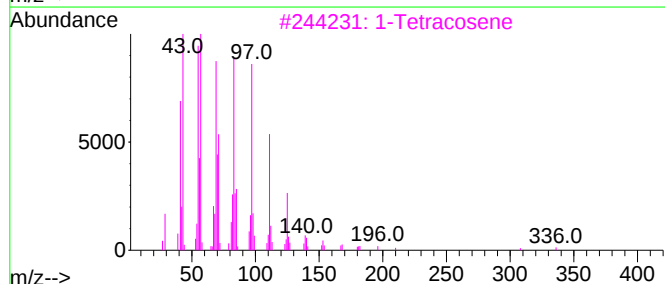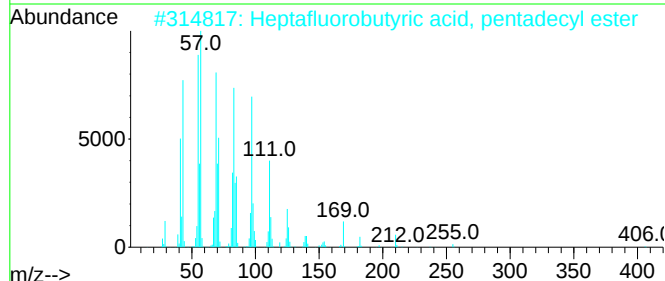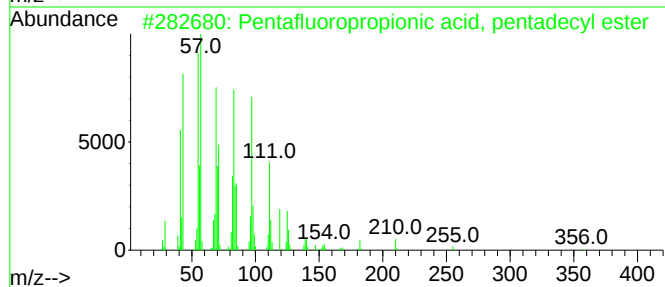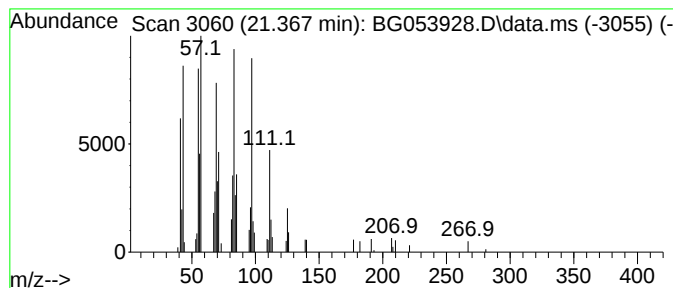

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053928.D
Acq On : 15 Jun 2022 21:12
Operator : CG/JU
Sample : N3354-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-46

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentafluoroprop...	21.366	2.9	ng	62966	5	21.725	442082	20.0