
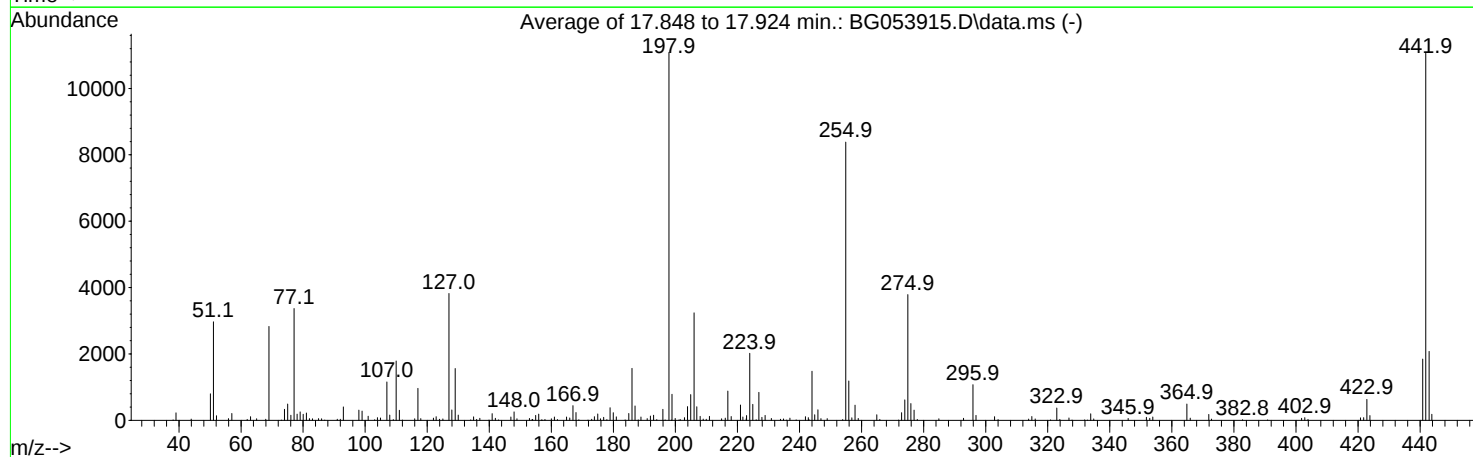


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
 Data File : BG053915.D
 Acq On : 15 Jun 2022 9:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 15:49:31 2022

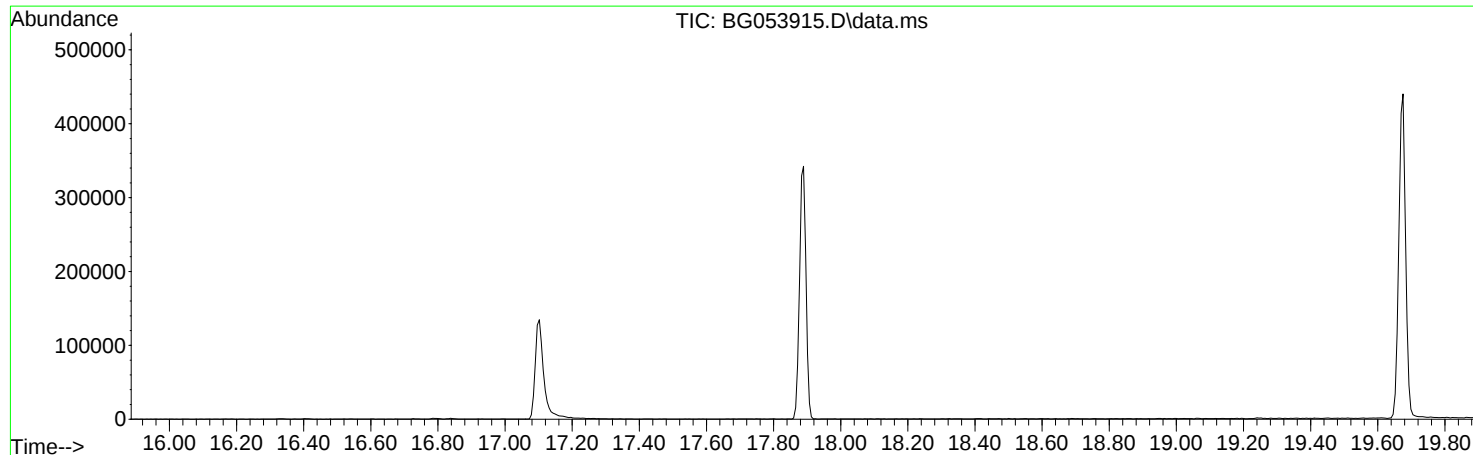




AutoFind: Averaged scan 2461 to 2474; Bkg corrected with scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	2968	PASS
68	69	0.00	2	1.2	34	PASS
69	198	0.00	100	25.5	2828	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.5	3825	PASS
197	198	0.00	2	0.1	15	PASS
198	198	100	100	100.0	11083	PASS
199	198	5	9	7.1	786	PASS
275	198	10	60	34.2	3788	PASS
365	198	1	100	4.4	493	PASS
441	198	0.01	100	16.7	1846	PASS
442	442	50	100	100.0	11057	PASS
443	442	15	24	18.8	2078	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053915.D
Acq On : 15 Jun 2022 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 15 17:23:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

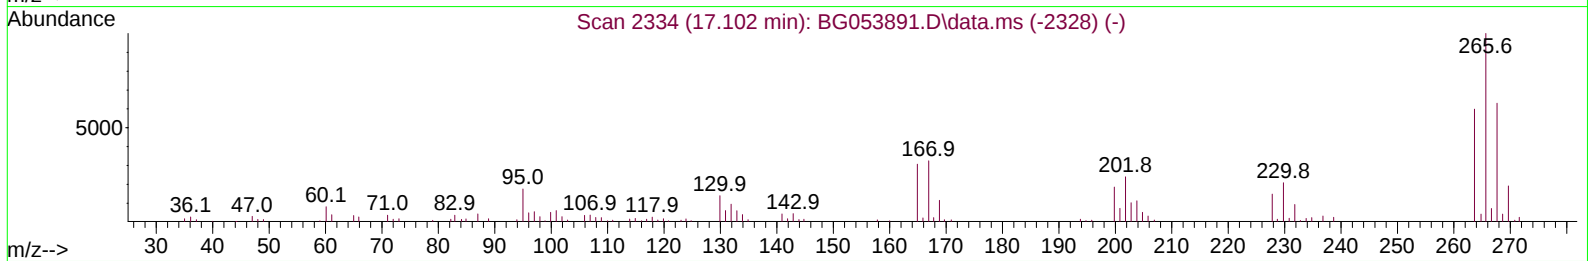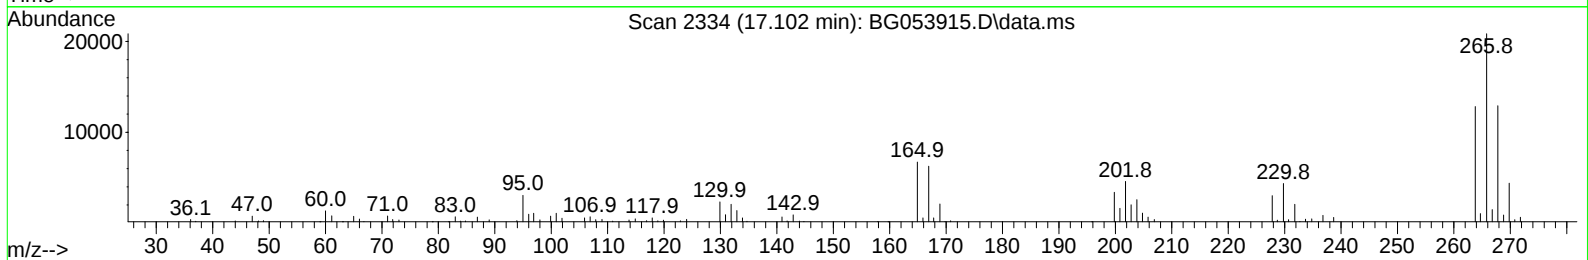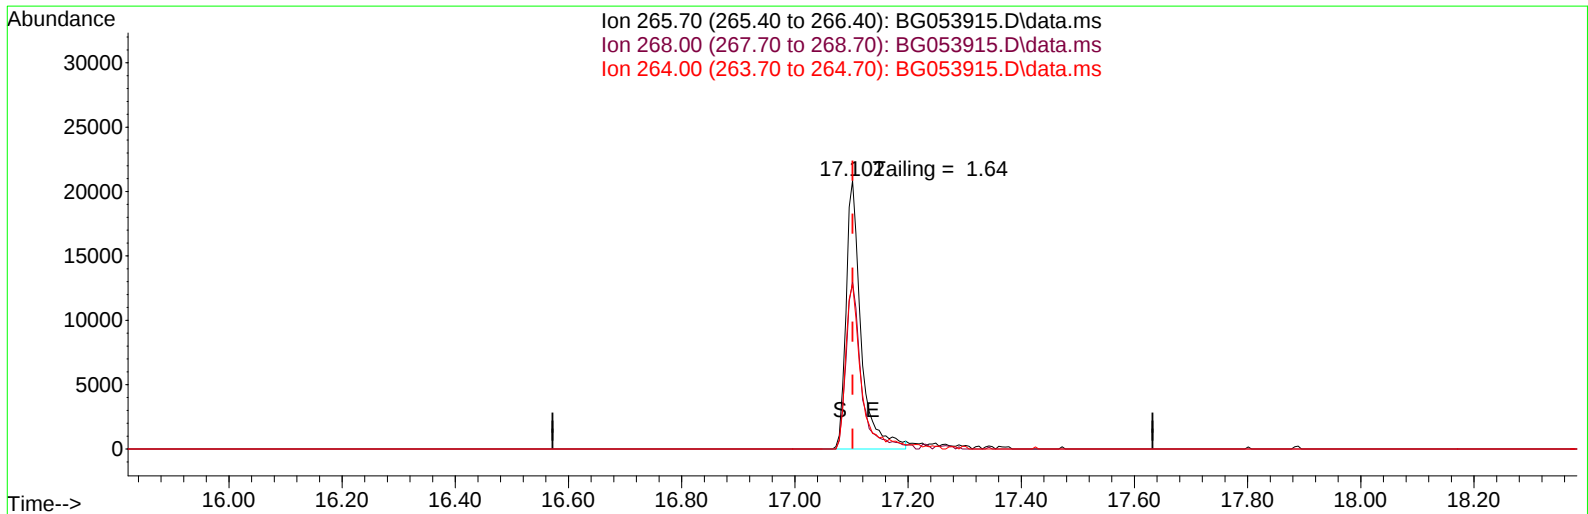

TIC: BG053915.D\data.ms

(70) Pentachlorophenol (C)

17.102min (+ 0.000) 87365.66 ng




response 39426

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.95
264.00	66.20	66.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061522\
Data File : BG053915.D
Acq On : 15 Jun 2022 9:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 15 17:23:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 15:49:31 2022
Response via : Initial Calibration

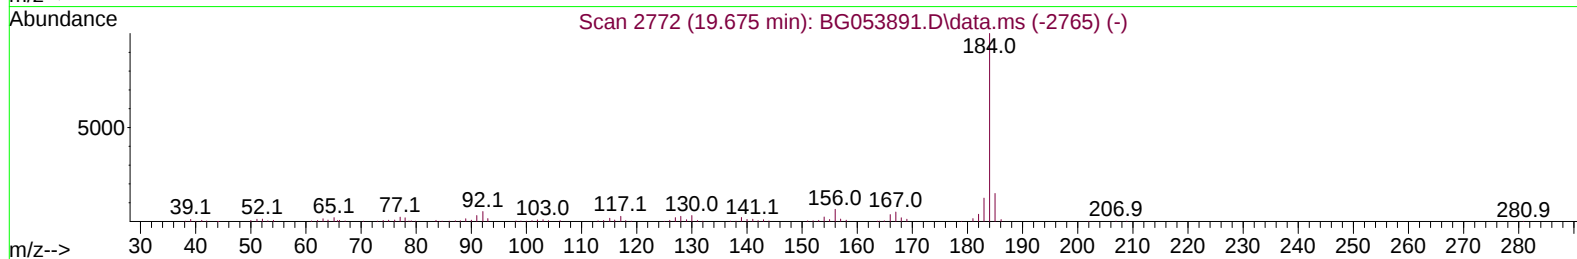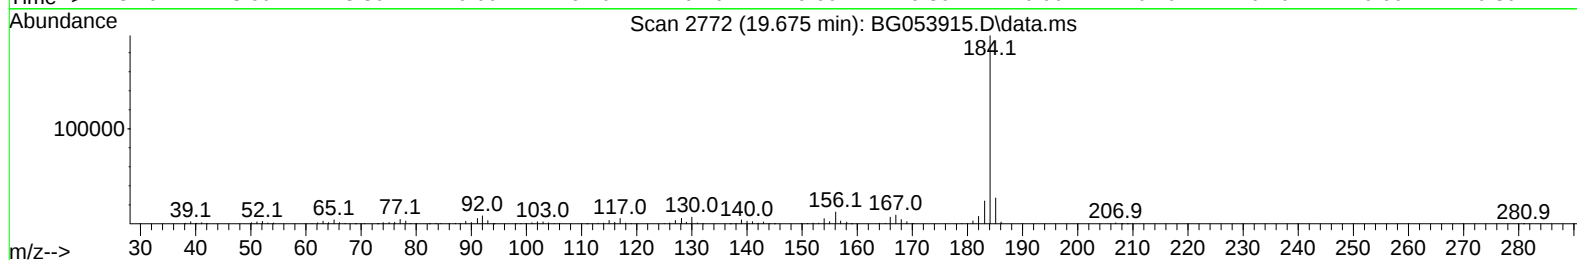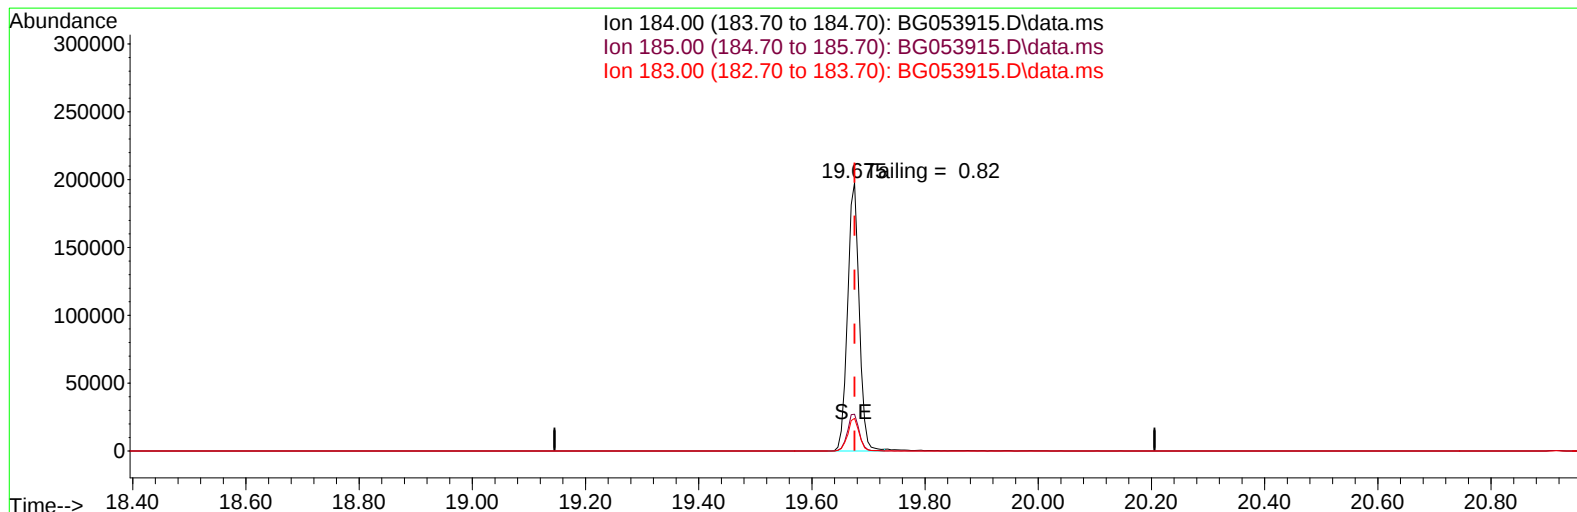

TIC: BG053915.D\data.ms

(77) Benzidine

19.675min (+ 0.000) 0.00 ng

response 283665

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.76
183.00	11.10	12.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/15/2022	BNA_G	<u>BG053915.D</u>
Compound Name	Response	Retention Time
DDT	154408	20.91
DDD	841	20.47
DDE	0	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
841	155249	0.54

Instrument :
BNA_G
ClientSampleId :
DFTPP