


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061615\
 Data File : BG017705.D
 Acq On : 17 Jun 2015 1:34
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\625-TERPINEOL-BG061615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 17 07:04:19 2015

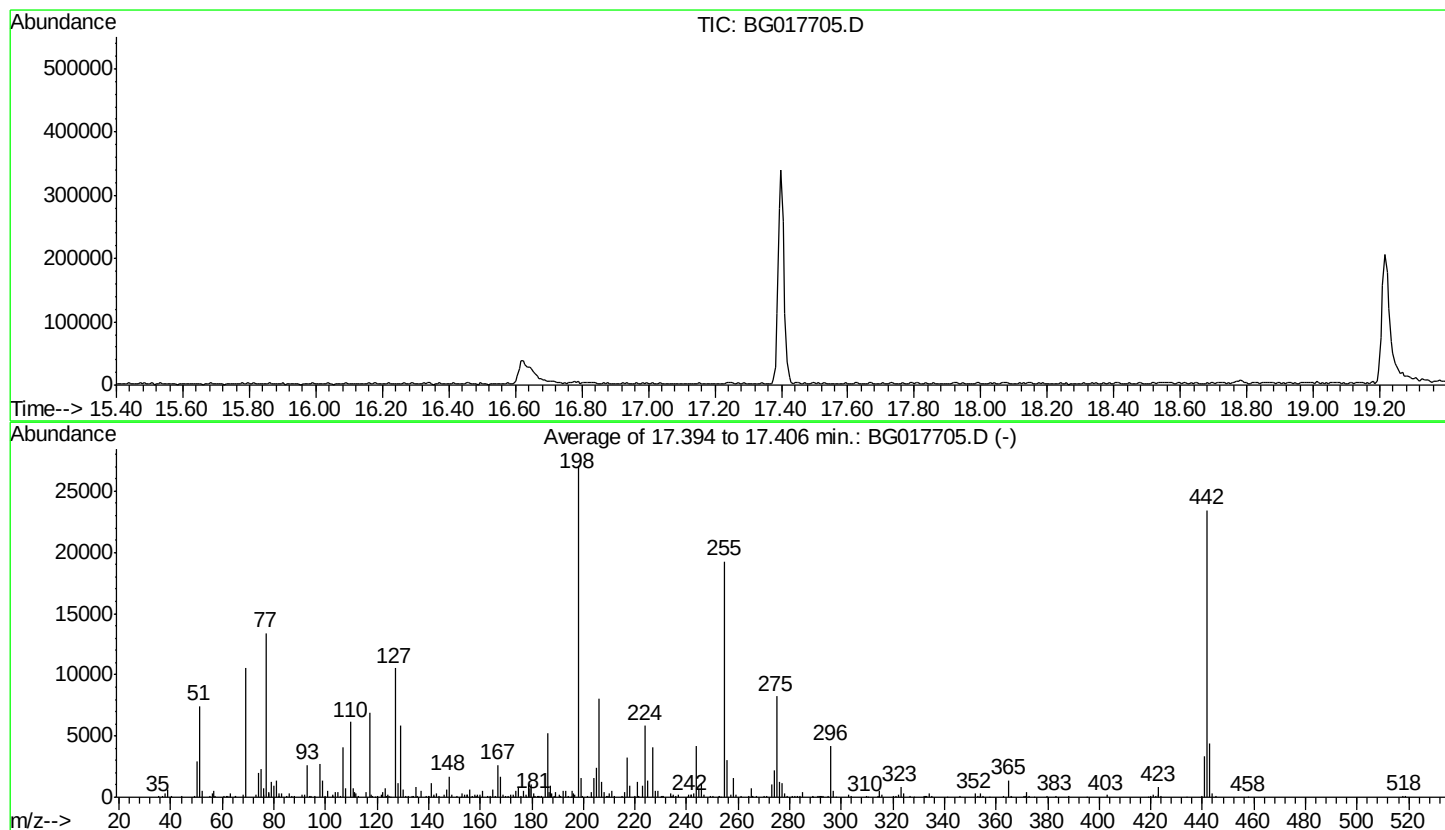

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	30	60	27.5	7459	FAIL*
68	69	0.00	2	1.7	181	PASS
69	198	0.00	100	39.0	10569	PASS
70	69	0.00	2	0.0	0	PASS
127	198	40	60	39.0	10549	FAIL*
197	198	0.00	1	0.6	175	PASS
198	198	100	100	100.0	27082	PASS
199	198	5	9	5.6	1527	PASS
275	198	10	30	30.4	8242	FAIL*
365	198	1	100	5.2	1398	PASS
441	443	0.01	100	75.6	3352	PASS
442	198	40	100	86.7	23472	PASS
443	442	17	23	18.9	4432	PASS