

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061616\
 Data File : BG022378.D
 Acq On : 16 Jun 2016 22:58
 Operator : UM/SJ
 Sample : H3569-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-06-COMP

Quant Time: Jun 17 02:25:25 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 13 17:40:23 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	22622	20.00	ng	-0.04
21) Naphthalene-d8	10.88	136	115155	20.00	ng	-0.03
38) Acenaphthene-d10	14.69	164	72075	20.00	ng	-0.03
63) Phenanthrene-d10	17.44	188	150870	20.00	ng	-0.03
75) Chrysene-d12	21.71	240	131236	20.00	ng	-0.03
86) Perylene-d12	24.97	264	123281	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	185871	158.86	ng	-0.01
7) Phenol-d6	7.25	99	271751	147.72	ng	0.00
23) Nitrobenzene-d5	9.23	82	154585	93.59	ng	-0.03
41) 2,4,6-Tribromophenol	16.19	330	87066	106.91	ng	-0.03
44) 2-Fluorobiphenyl	13.32	172	394006	83.31	ng	-0.03
78) Terphenyl-d14	20.03	244	455453	82.39	ng	-0.03
Target Compounds						Qvalue
49) Dimethylphthalate	14.14	163	115219	19.28	ng	100
70) Phenanthrene	17.48	178	29803	3.64	ng	# 96
71) Anthracene	17.48	178	29803	3.67	ng	95
74) Fluoranthene	19.49	202	39859	4.23	ng	98
77) Pyrene	19.85	202	55190	6.76	ng	99
80) Benzo(a)anthracene	21.68	228	21648	2.94	ng	97
82) Chrysene	21.75	228	23602	3.30	ng	96
87) Benzo(b)fluoranthene	23.93	252	21332	2.97	ng	# 91
88) Benzo(k)fluoranthene	23.93	252	21332	3.01	ng	# 90
89) Benzo(a)pyrene	24.81	252	17977	2.61	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061616\
Data File : BG022378.D
Acq On : 16 Jun 2016 22:58
Operator : UM/SJ
Sample : H3569-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-06-COMP

Quant Time: Jun 17 02:25:25 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

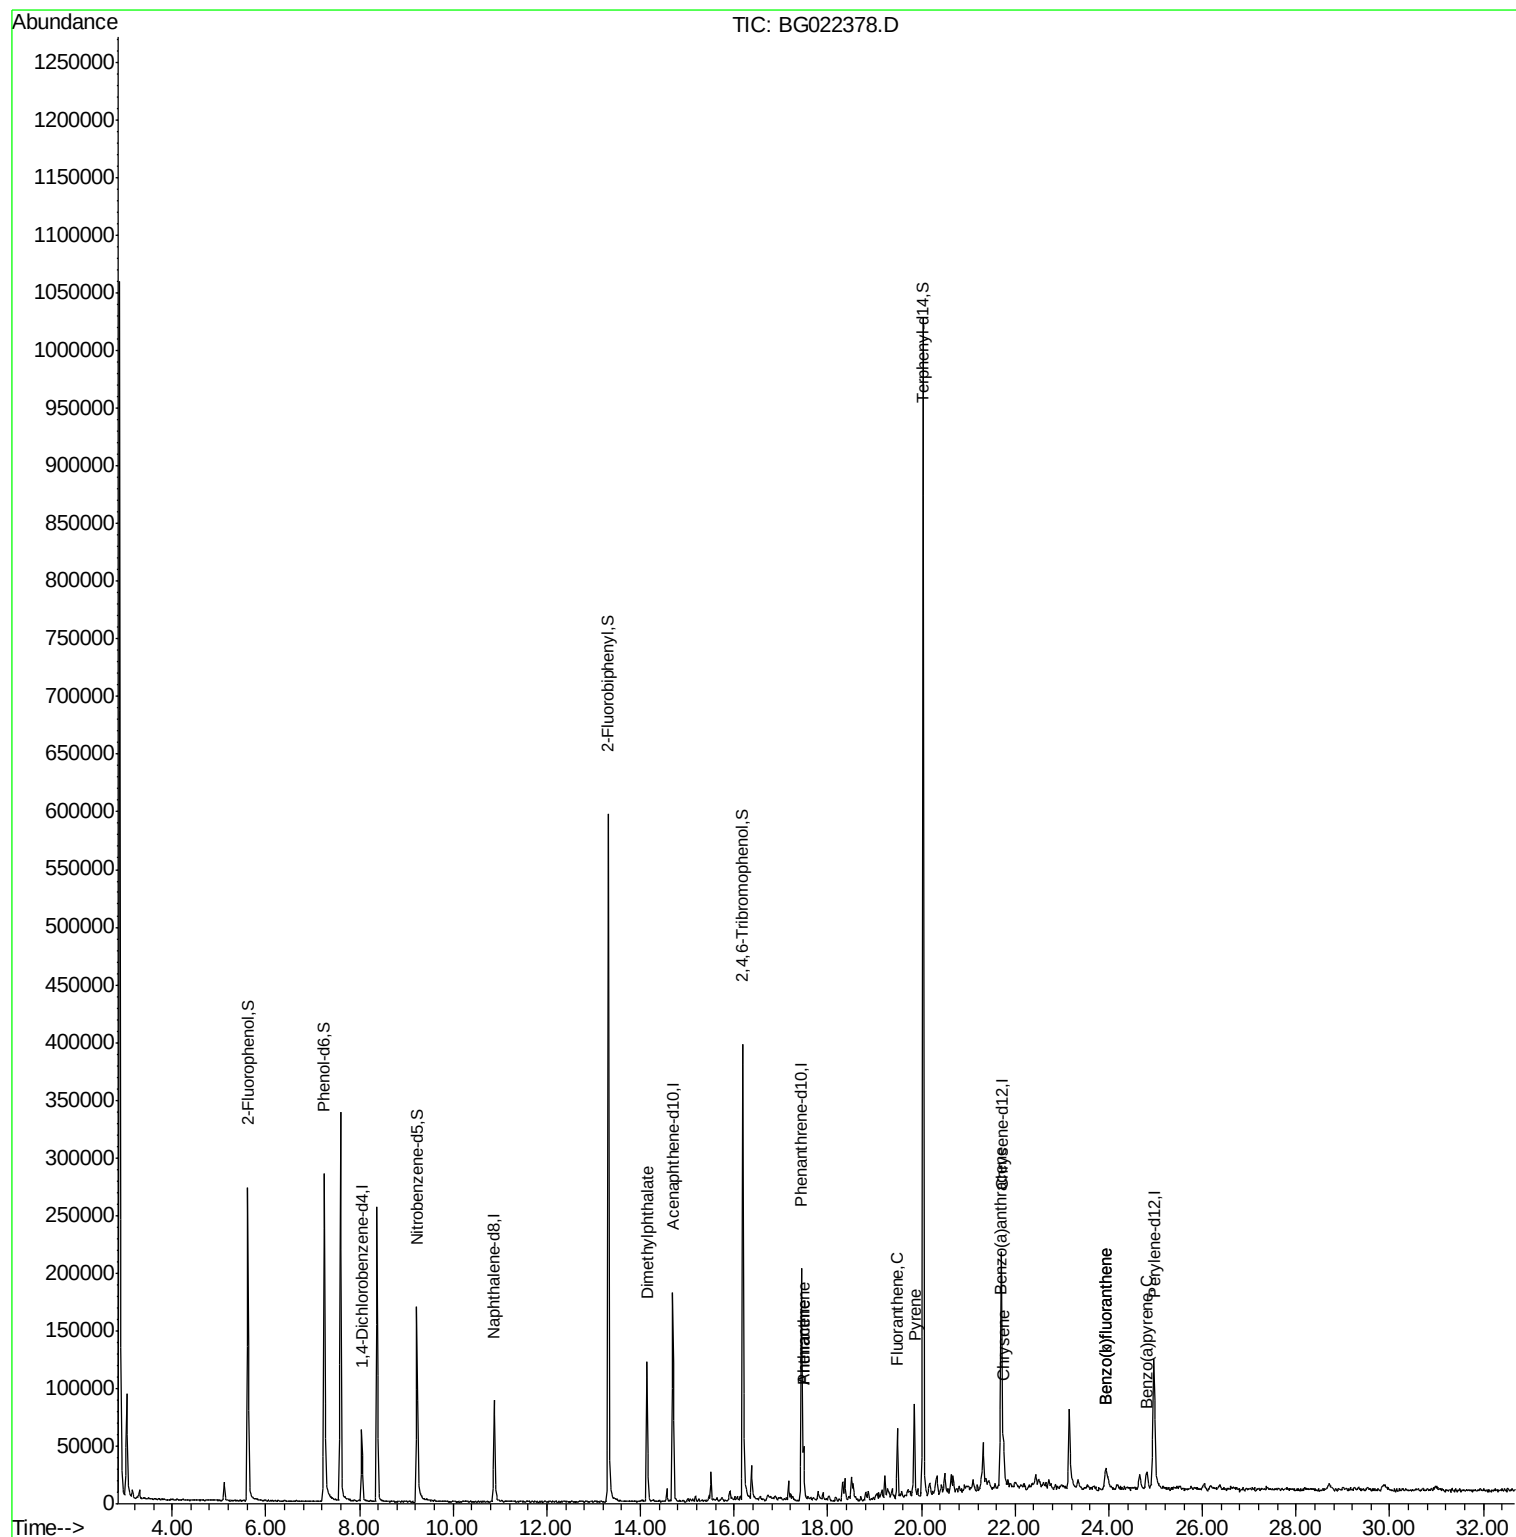




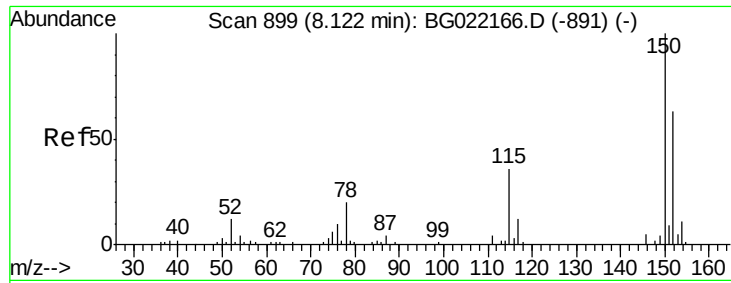


#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.05 min Scan# 887
Delta R.T. -0.04 min
Lab File: BG022378.D
Acq: 16 Jun 2016 22:58

Instrument :
BNA_G
ClientSampleId :
SB-06-COMP




Tgt Ion:152 Resp: 22622
Ion Ratio Lower Upper
152 100
150 173.4 130.1 195.1
115 56.1 62.2 93.2#

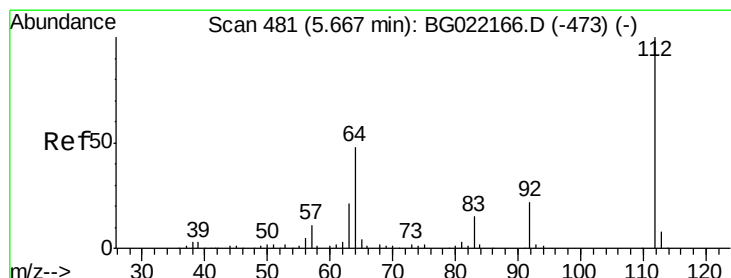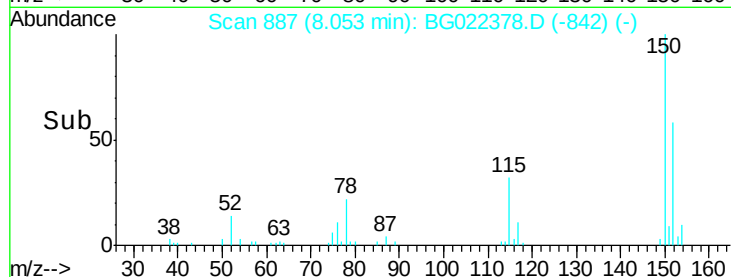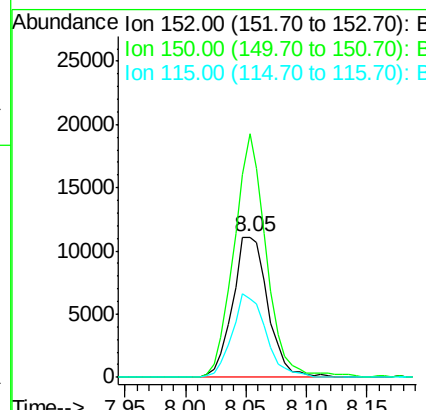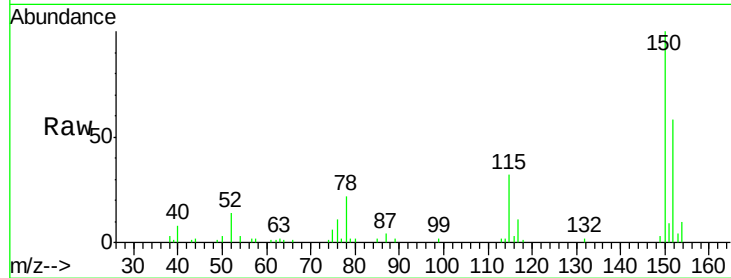


#5

2-Fluorophenol
Concen: 158.86 ng
RT: 5.62 min Scan# 473
Delta R.T. -0.01 min
Lab File: BG022378.D
Acq: 16 Jun 2016 22:58

Tgt Ion:112 Resp: 185871
Ion Ratio Lower Upper
112 100
64 51.0 51.1 76.7#
63 24.9 24.6 37.0

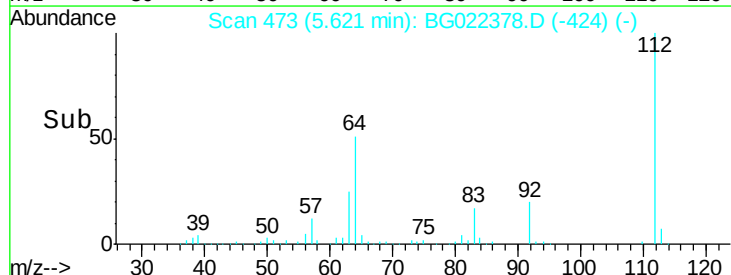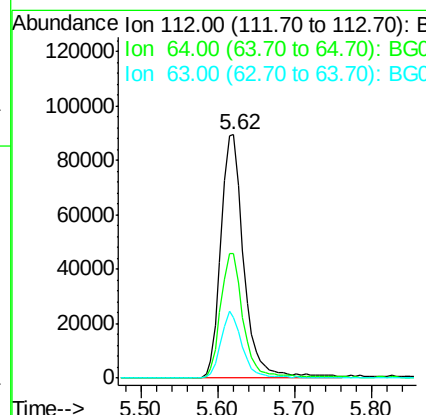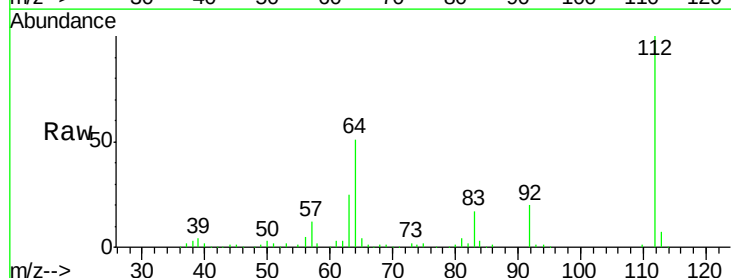

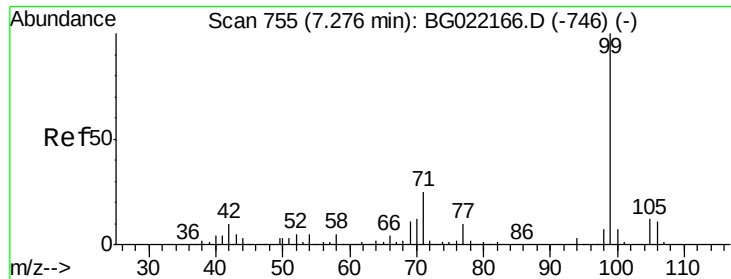

#7

Phenol-d6

Concen: 147.72 ng

RT: 7.25 min Scan# 750

Delta R.T. -0.00 min

Lab File: BG022378.D

Acq: 16 Jun 2016 22:58

Instrument :

BNA_G

ClientSampleId :

SB-06-COMP


Tgt Ion: 99 Resp: 271751

Ion Ratio Lower Upper

99 100

42 10.7 16.4 24.6#




71 26.6 25.0 37.4

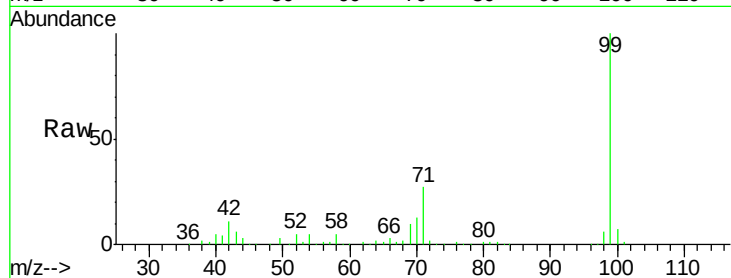

Abundance Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

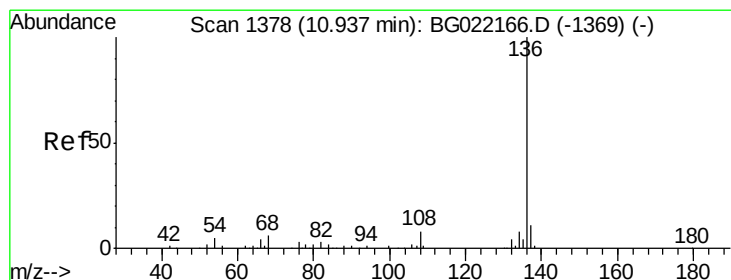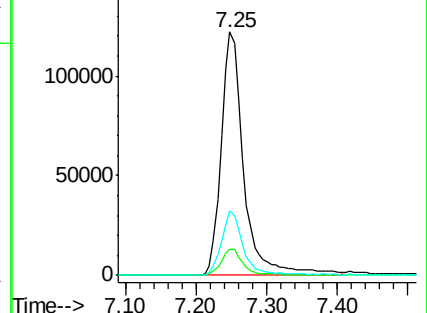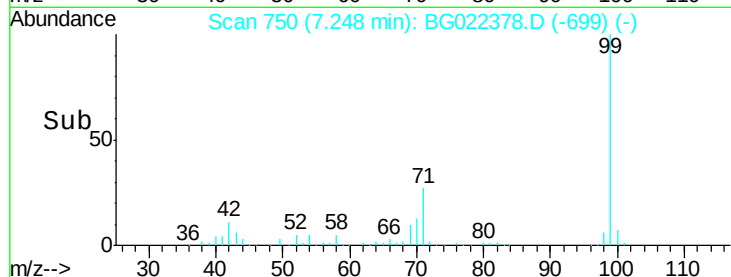

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.88 min Scan# 1368

Delta R.T. -0.03 min

Lab File: BG022378.D

Acq: 16 Jun 2016 22:58

Tgt Ion: 136 Resp: 115155


Ion Ratio Lower Upper

136 100

137 10.8 9.0 13.4

54 6.5 9.6 14.4#

68 5.7 6.4 9.6#


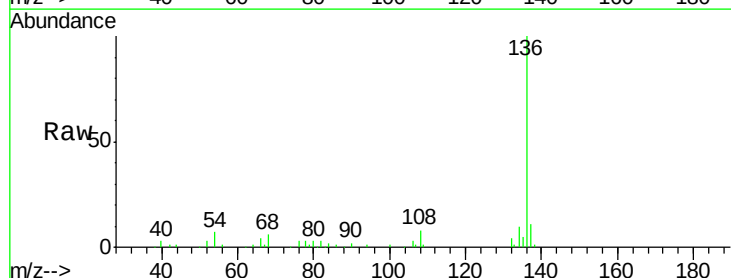



Abundance Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

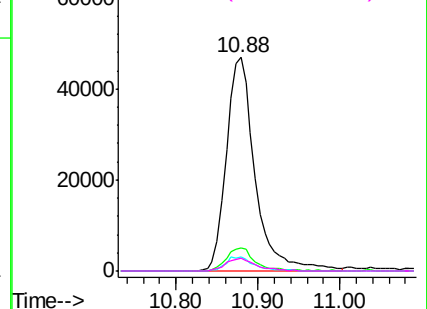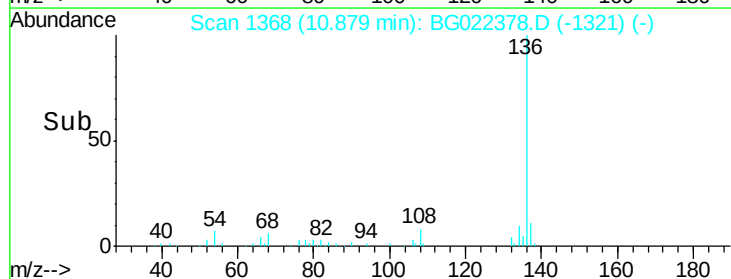


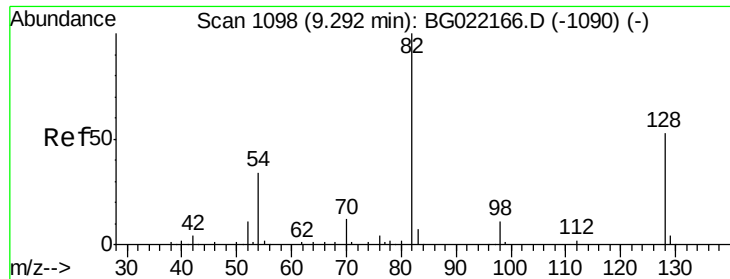




#23
 Nitrobenzene-d5
 Concen: 93.59 ng
 RT: 9.23 min Scan# 1087
 Delta R.T. -0.03 min
 Lab File: BG022378.D
 Acq: 16 Jun 2016 22:58

Instrument :
 BNA_G
 ClientSampleId :
 SB-06-COMP

Tgt Ion: 82 Resp: 154585
 Ion Ratio Lower Upper
 82 100
 128 46.4 33.4 50.0
 54 37.3 46.1 69.1#

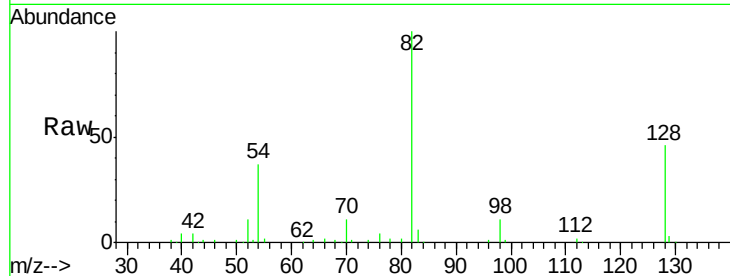


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC


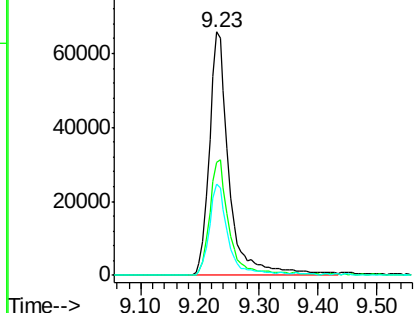



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.69 min Scan# 2017
 Delta R.T. -0.03 min
 Lab File: BG022378.D
 Acq: 16 Jun 2016 22:58

Tgt Ion: 164 Resp: 72075
 Ion Ratio Lower Upper
 164 100
 162 105.1 78.0 117.0
 160 50.3 32.9 49.3#



Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

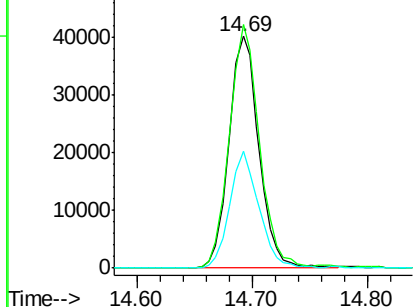







#41
 2,4,6-Tribromophenol
 Concen: 106.91 ng
 RT: 16.19 min Scan# 2272
 Delta R.T. -0.03 min
 Lab File: BG022378.D
 Acq: 16 Jun 2016 22:58

Instrument :
 BNA_G
 ClientSampleId :
 SB-06-COMP

Tgt Ion:330 Resp: 87066
 Ion Ratio Lower Upper
 330 100
 332 99.5 78.0 117.0
 141 47.0 33.8 50.8

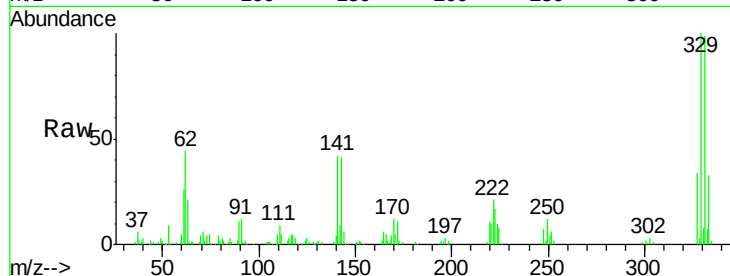


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


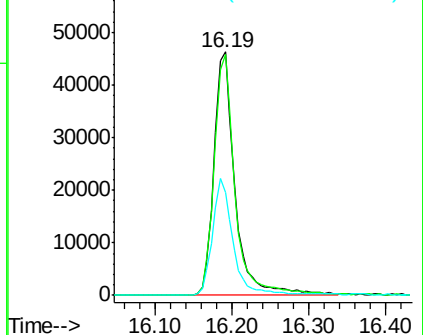



#44
 2-Fluorobiphenyl
 Concen: 83.31 ng
 RT: 13.32 min Scan# 1783
 Delta R.T. -0.03 min
 Lab File: BG022378.D
 Acq: 16 Jun 2016 22:58

Tgt Ion:172 Resp: 394006
 Ion Ratio Lower Upper
 172 100
 171 38.4 27.8 41.6
 170 26.5 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

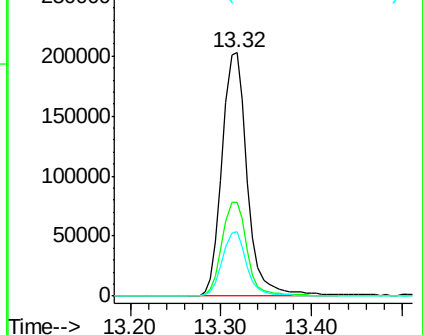

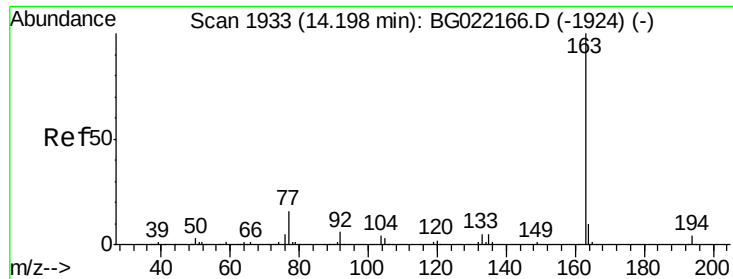

#49

Dimethylphthalate

Concen: 19.28 ng

RT: 14.14 min Scan# 1923

Delta R.T. -0.03 min

Lab File: BG022378.D

Acq: 16 Jun 2016 22:58





Instrument :

BNA_G

ClientSampleId :

SB-06-COMP

Tgt Ion:	163	Resp:	115219
Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.0	4.6
164	10.1	8.1	12.1

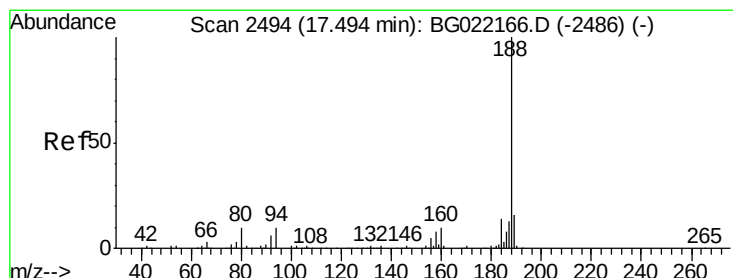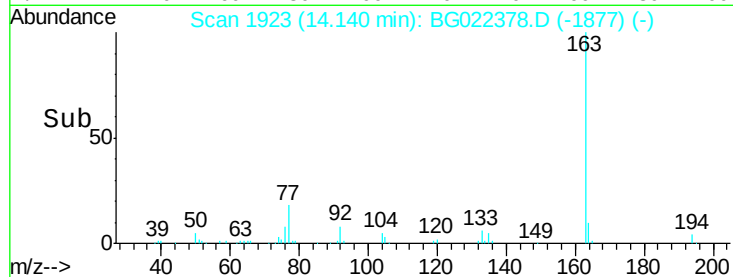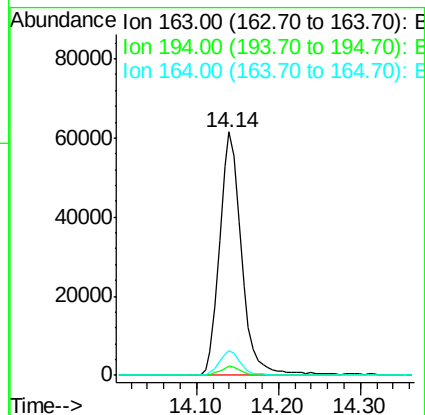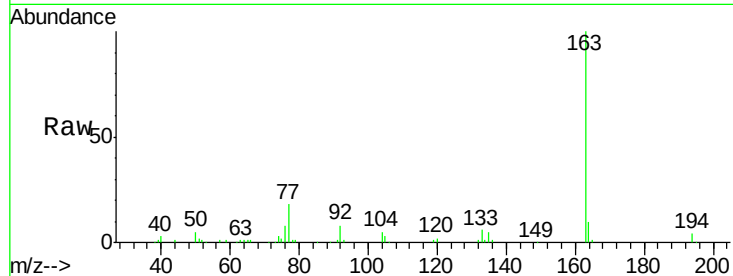

#63

Phenanthrene-d10

Concen: 20.00 ng




RT: 17.44 min Scan# 2484


Delta R.T. -0.03 min

Lab File: BG022378.D

Acq: 16 Jun 2016 22:58

Tgt Ion:	188	Resp:	150870
Ion	Ratio	Lower	Upper
188	100		
94	11.2	7.5	11.3
80	13.1	8.6	13.0#

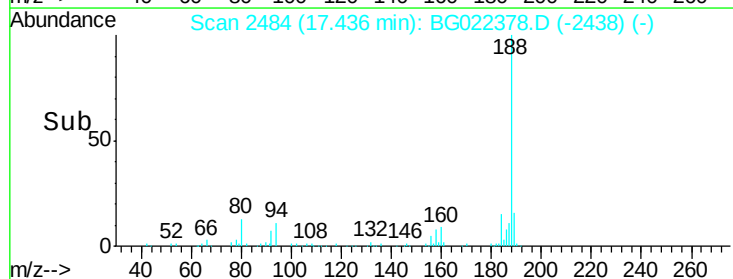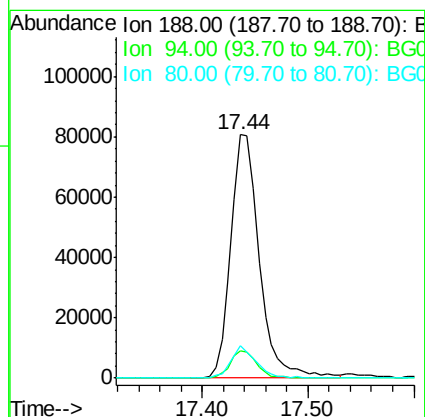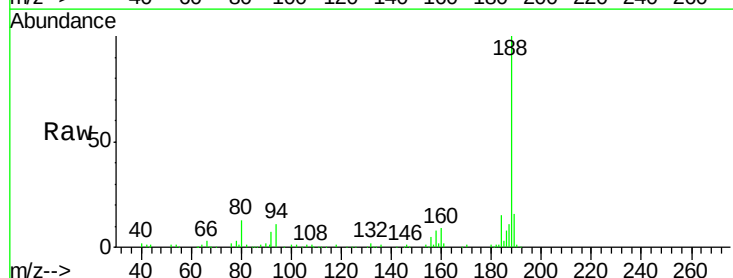



#70

Phenanthrene

Concen: 3.64 ng

RT: 17.48 min Scan# 2492

Delta R.T. -0.03 min

Lab File: BG022378.D

Acq: 16 Jun 2016 22:58

Instrument :

BNA_G

ClientSampleId :

SB-06-COMP


Tgt Ion:178 Resp: 29803

Ion Ratio Lower Upper

178 100

176 20.1 16.2 24.4




179 18.2 12.0 18.0#

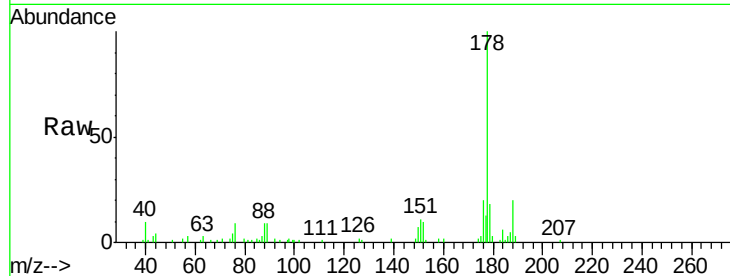

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

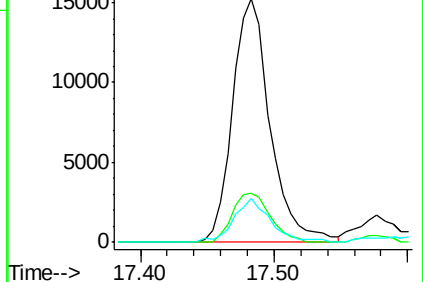

#71

Anthracene

Concen: 3.67 ng

RT: 17.48 min Scan# 2492

Delta R.T. -0.12 min

Lab File: BG022378.D

Acq: 16 Jun 2016 22:58


Tgt Ion:178 Resp: 29803

Ion Ratio Lower Upper

178 100

176 20.1 15.0 22.4



179 18.2 12.2 18.4

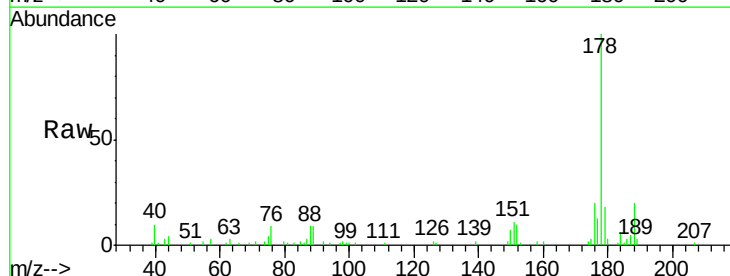


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

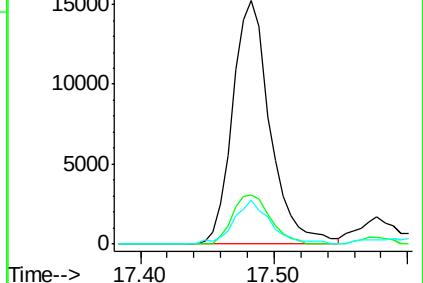



#74

Fluoranthene

Concen: 4.23 ng

RT: 19.49 min Scan# 2833

Delta R.T. -0.03 min

Lab File: BG022378.D

Acq: 16 Jun 2016 22:58

Instrument :

BNA_G

ClientSampleId :

SB-06-COMP


Tgt Ion:202 Resp: 39859

Ion Ratio Lower Upper

202 100

101 11.8 0.0 31.0




203 17.2 0.0 37.9



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

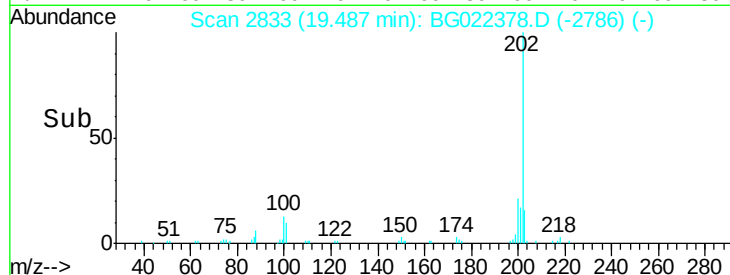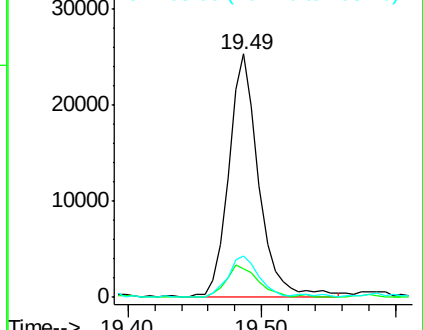

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.71 min Scan# 3211

Delta R.T. -0.03 min

Lab File: BG022378.D

Acq: 16 Jun 2016 22:58


Tgt Ion:240 Resp: 131236

Ion Ratio Lower Upper

240 100

120 13.5 8.4 12.6#



236 25.4 19.6 29.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E




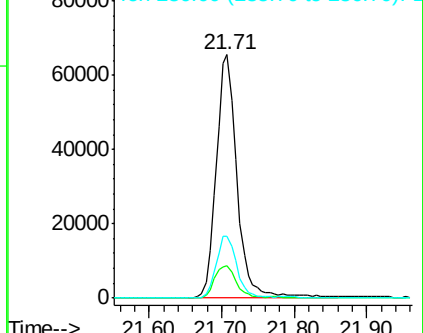




#77
 Pyrene
 Concen: 6.76 ng
 RT: 19.85 min Scan# 2895
 Delta R.T. -0.03 min
 Lab File: BG022378.D
 Acq: 16 Jun 2016 22:58




Instrument :
 BNA_G
 ClientSampleId :
 SB-06-COMP


Tgt Ion:202 Resp: 55190
 Ion Ratio Lower Upper
 202 100
 200 23.0 18.2 27.2
 203 18.6 15.0 22.4

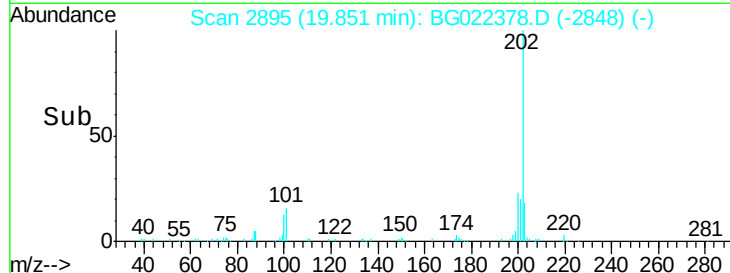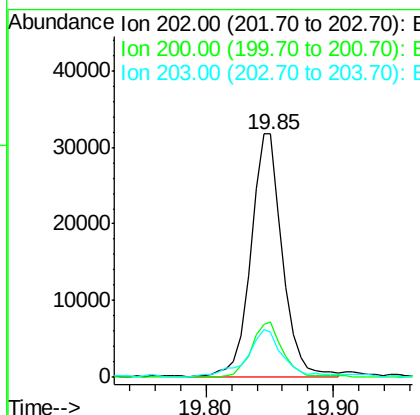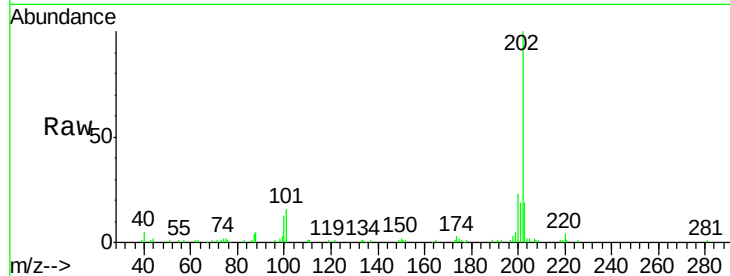

#78
 Terphenyl-d14
 Concen: 82.39 ng
 RT: 20.03 min Scan# 2926
 Delta R.T. -0.03 min
 Lab File: BG022378.D
 Acq: 16 Jun 2016 22:58

Tgt Ion:244 Resp: 455453
 Ion Ratio Lower Upper
 244 100
 212 8.0 6.5 9.7
 122 14.4 8.6 12.8#



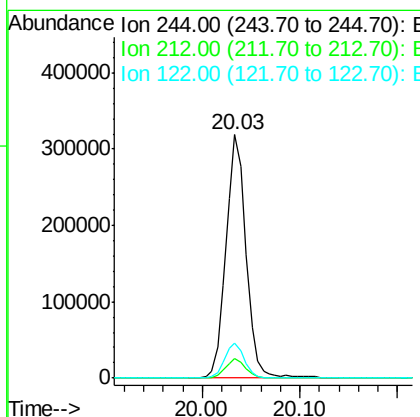
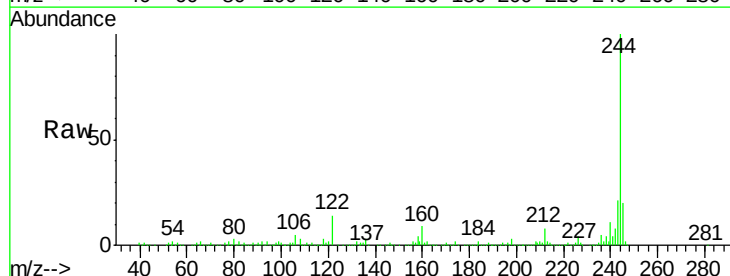


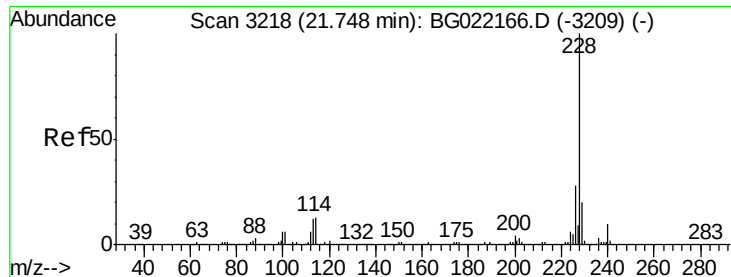

#80
Benzo(a)anthracene
Concen: 2.94 ng
RT: 21.68 min Scan# 3207
Delta R.T. -0.04 min
Lab File: BG022378.D
Acq: 16 Jun 2016 22:58




Instrument :
BNA_G
ClientSampleId :
SB-06-COMP


Tgt Ion:228 Resp: 21648
Ion Ratio Lower Upper
228 100
226 28.6 22.6 34.0
229 22.9 16.1 24.1

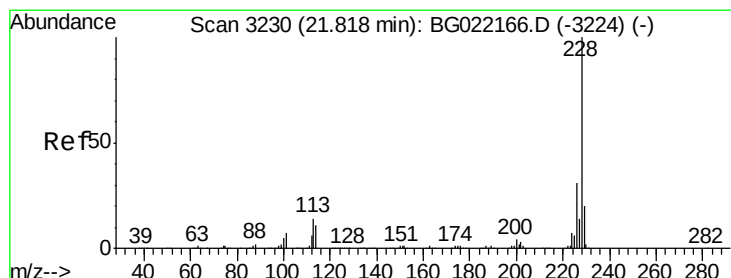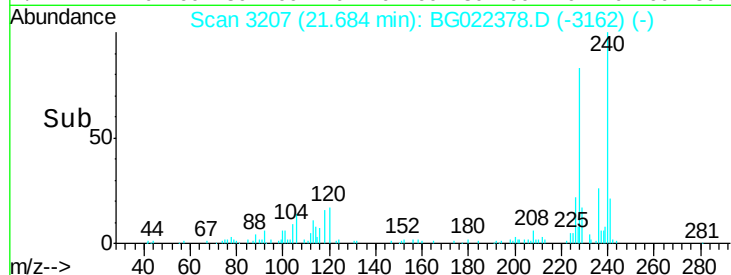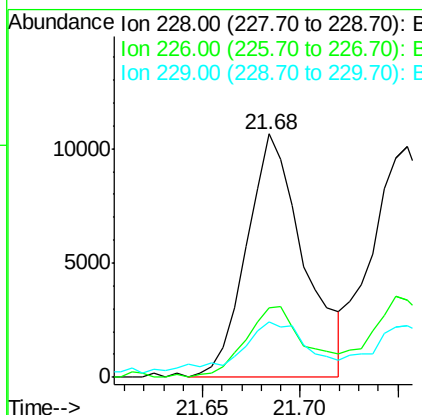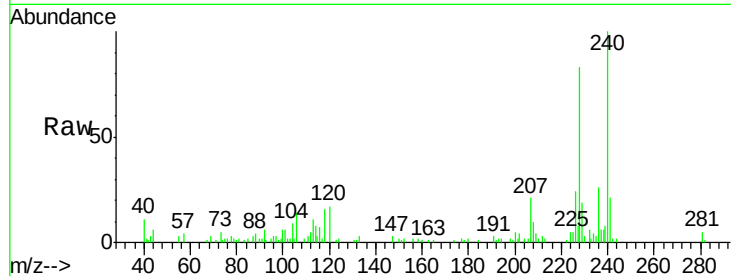

#82
Chrysene
Concen: 3.30 ng
RT: 21.75 min Scan# 3219
Delta R.T. -0.03 min
Lab File: BG022378.D
Acq: 16 Jun 2016 22:58

Tgt Ion:228 Resp: 23602
Ion Ratio Lower Upper
228 100
226 33.4 25.4 38.0
229 22.6 15.9 23.9


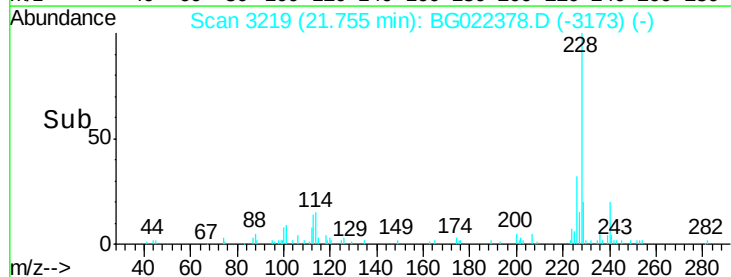
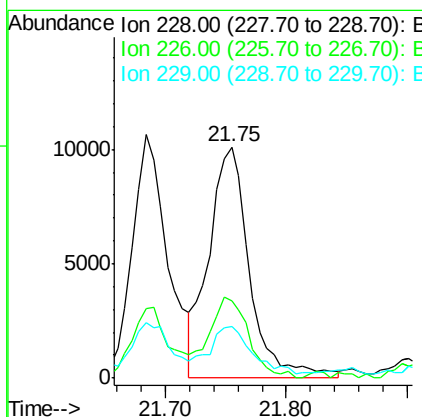
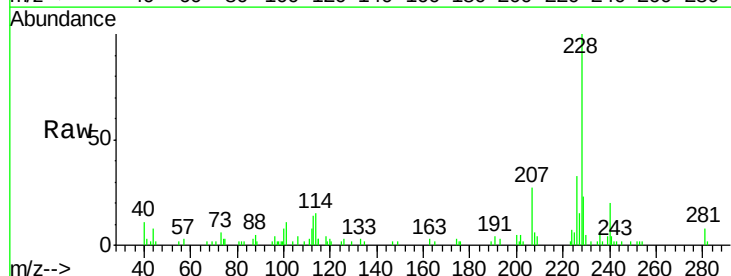




#86
Perylene-d12
Concen: 20.00 ng
RT: 24.97 min Scan# 3766
Delta R.T. -0.04 min
Lab File: BG022378.D
Acq: 16 Jun 2016 22:58




Instrument :
BNA_G
ClientSampleId :
SB-06-COMP


Tgt Ion:264 Resp: 123281
Ion Ratio Lower Upper
264 100
260 25.4 20.2 30.4
265 20.5 17.8 26.8

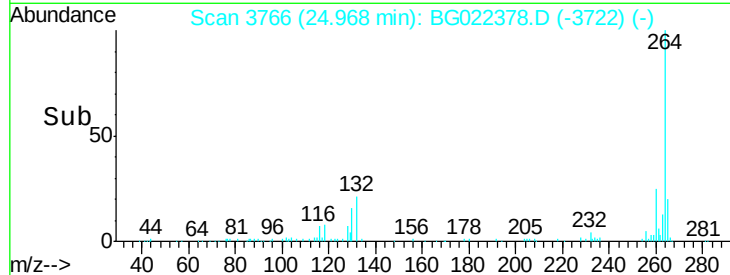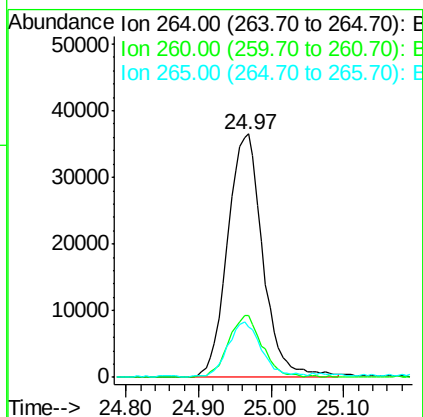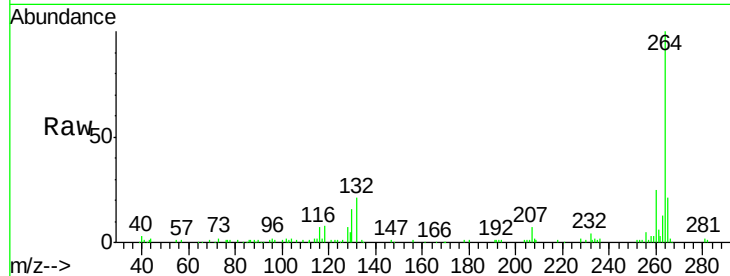

#87
Benzo(b)fluoranthene
Concen: 2.97 ng
RT: 23.93 min Scan# 3590
Delta R.T. -0.03 min
Lab File: BG022378.D
Acq: 16 Jun 2016 22:58

Tgt Ion:252 Resp: 21332
Ion Ratio Lower Upper
252 100
253 17.9 17.5 26.3
125 14.6 8.6 13.0#

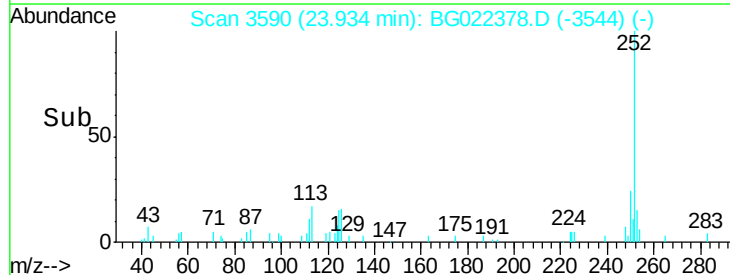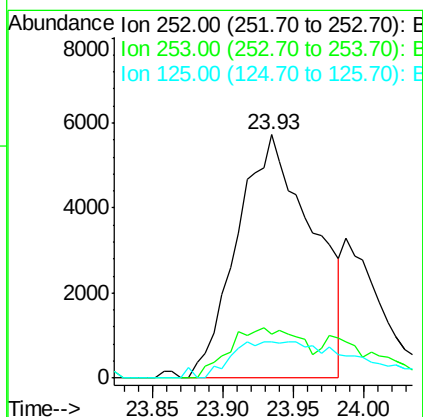

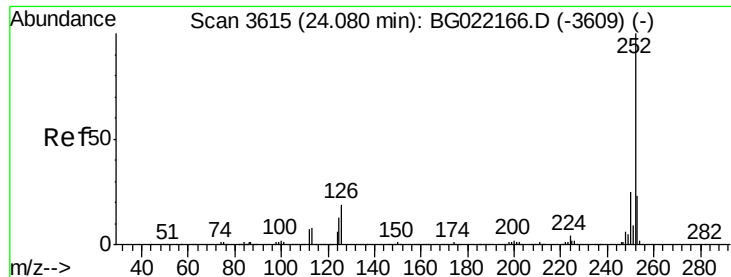

#88

Benzo(k)fluoranthene

Concen: 3.01 ng

RT: 23.93 min Scan# 3590

Delta R.T. -0.11 min

Lab File: BG022378.D

Acq: 16 Jun 2016 22:58

Instrument :

BNA_G

ClientSampleId :

SB-06-COMP


Tgt Ion:252 Resp: 21332

Ion Ratio Lower Upper

252 100

253 17.9 17.8 26.8




125 14.6 8.3 12.5#

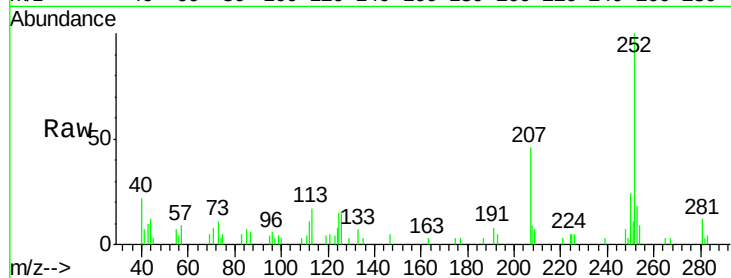

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

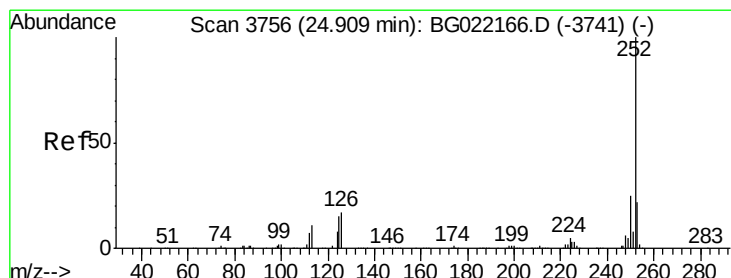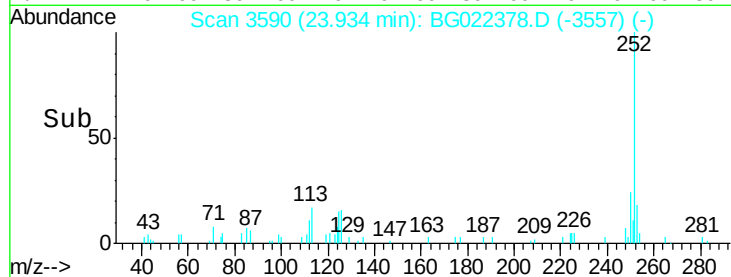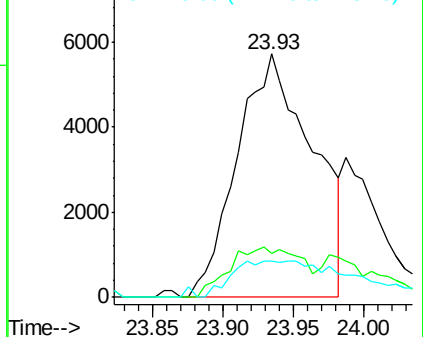

#89

Benzo(a)pyrene

Concen: 2.61 ng

RT: 24.81 min Scan# 3739

Delta R.T. -0.05 min

Lab File: BG022378.D

Acq: 16 Jun 2016 22:58


Tgt Ion:252 Resp: 17977

Ion Ratio Lower Upper

252 100

253 24.6 17.1 25.7

125 17.3 9.6 14.4#

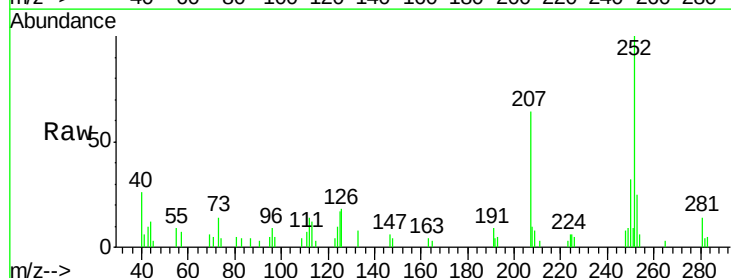

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

