
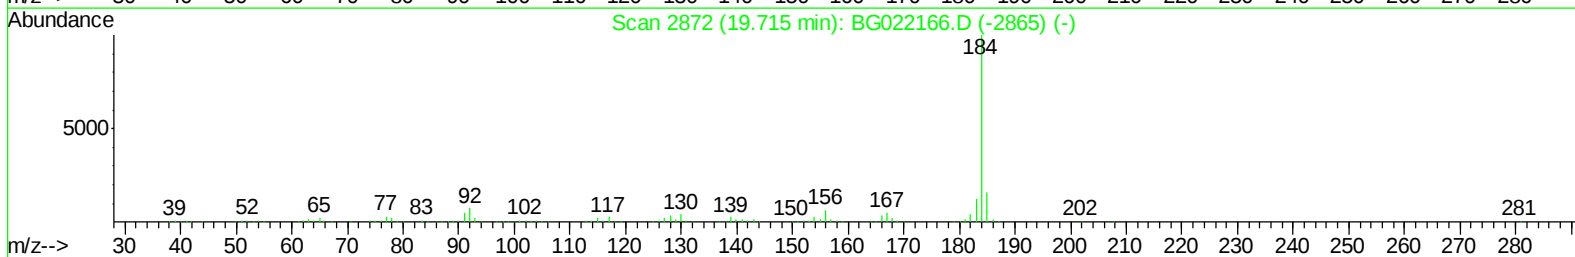
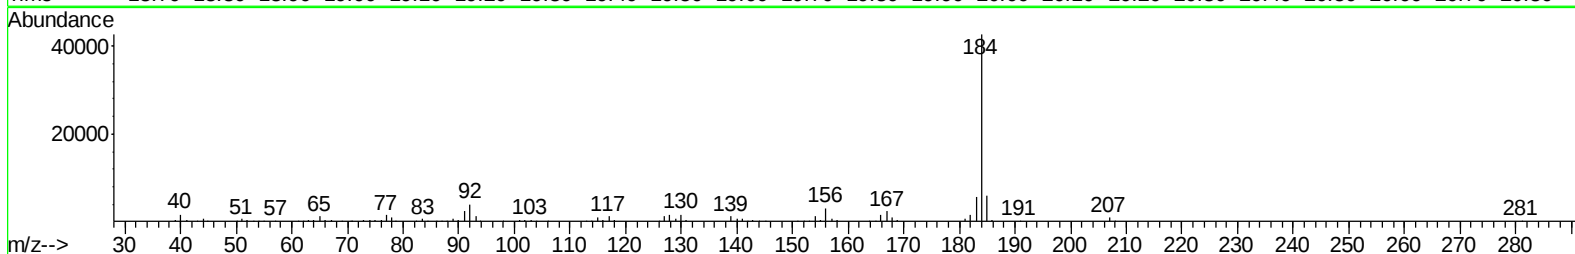


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061616\
Data File : BG022364.D
Acq On : 16 Jun 2016 13:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 08:00:38 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

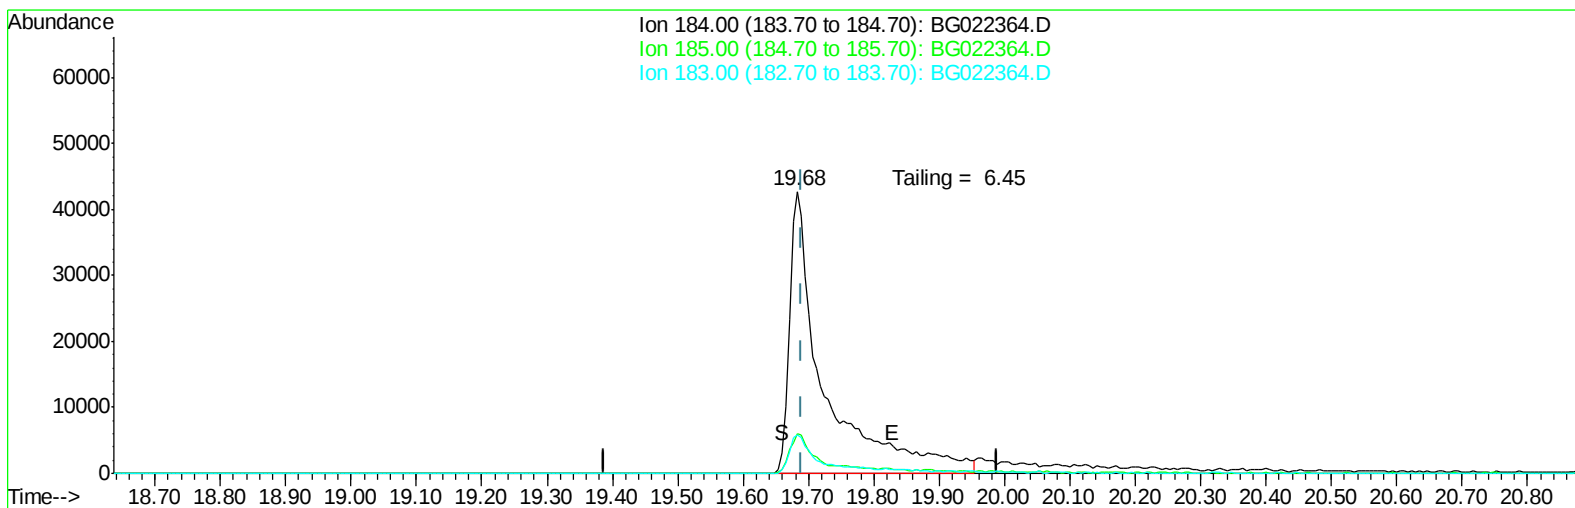

TIC: BG022364.D

(76) Benzidine




19.683min (-0.006) 0.00ng

response 145343

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.17
183.00	12.80	13.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061616\
Data File : BG022364.D
Acq On : 16 Jun 2016 13:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 08:00:38 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

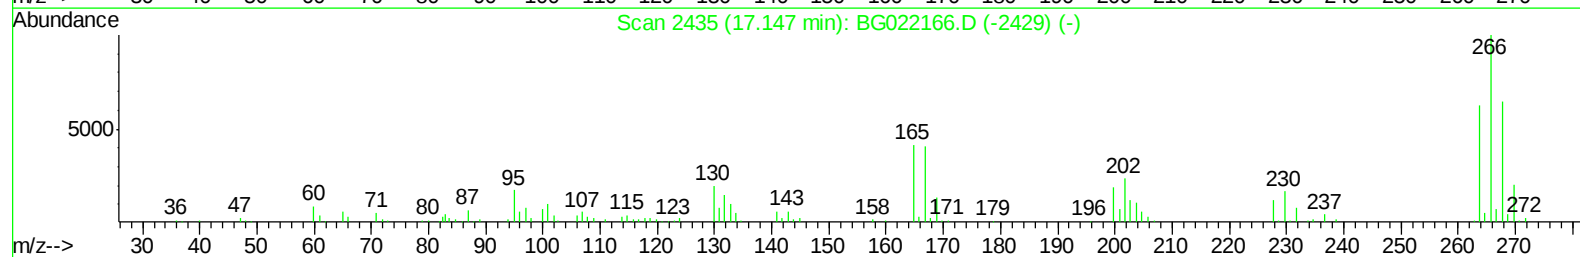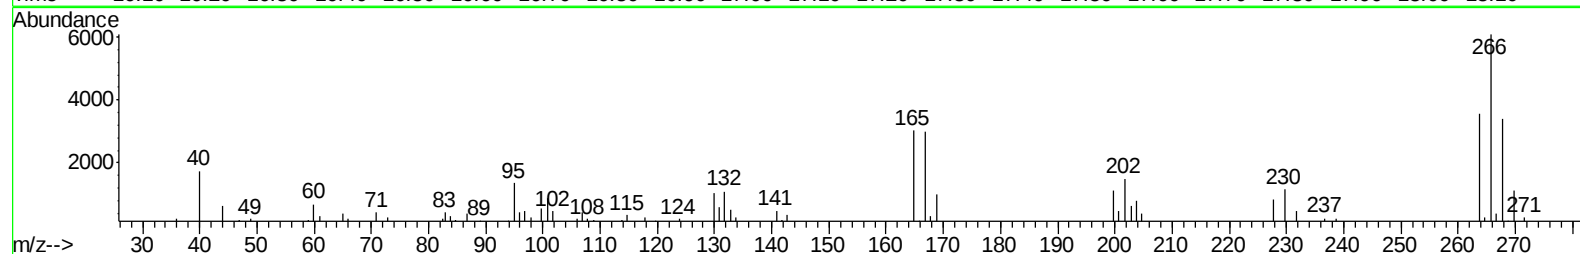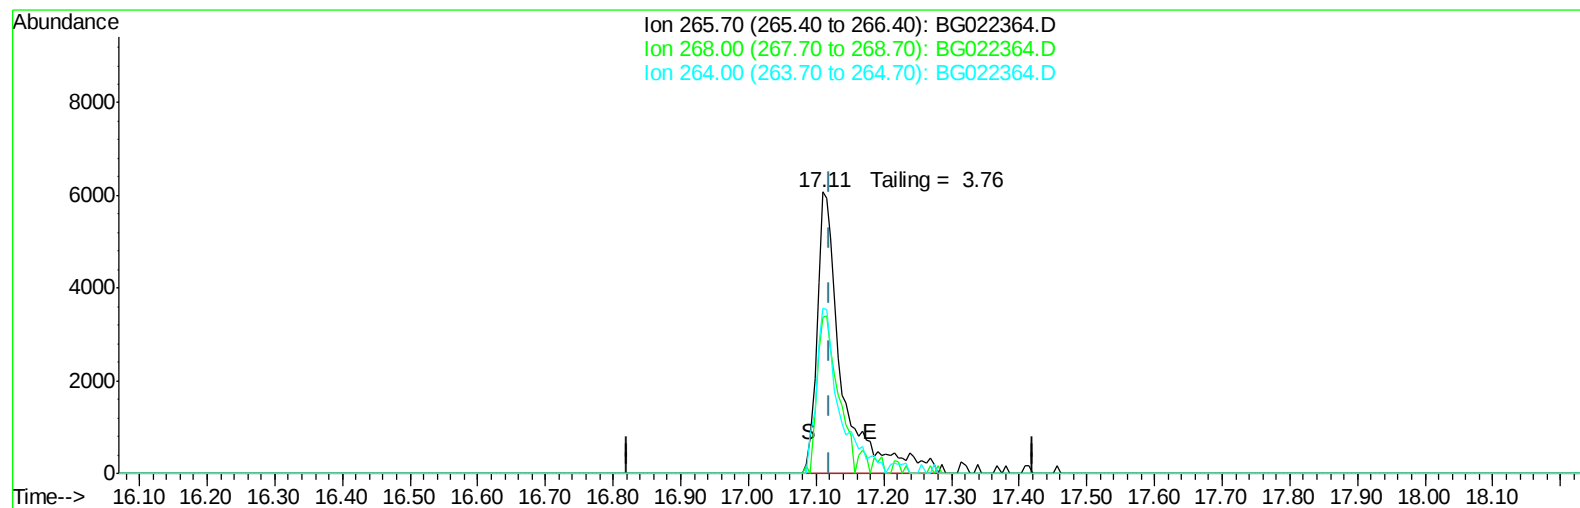

TIC: BG022364.D

(69) Pentachlorophenol (C)

17.109min (-0.012) 0.00ng

response 14857

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	58.14
264.00	67.20	63.59
0.00	0.00	0.00