

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061616\
 Data File : BG022368.D
 Acq On : 16 Jun 2016 16:17
 Operator : UM/SJ
 Sample : H3569-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-07-COMP

Quant Time: Jun 17 02:22:30 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 13 17:40:23 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	23723	20.00	ng	-0.04
21) Naphthalene-d8	10.87	136	120023	20.00	ng	-0.03
38) Acenaphthene-d10	14.69	164	74731	20.00	ng	-0.03
63) Phenanthrene-d10	17.44	188	164283	20.00	ng	-0.03
75) Chrysene-d12	21.71	240	144780	20.00	ng	-0.03
86) Perylene-d12	24.96	264	130437	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	151420	123.41	ng	-0.02
7) Phenol-d6	7.26	99	224772	116.51	ng	0.00
23) Nitrobenzene-d5	9.23	82	122318	71.05	ng	-0.03
41) 2,4,6-Tribromophenol	16.19	330	73167	86.65	ng	-0.03
44) 2-Fluorobiphenyl	13.31	172	320460	65.35	ng	-0.03
78) Terphenyl-d14	20.03	244	419330	68.76	ng	-0.02
Target Compounds						Qvalue
49) Dimethylphthalate	14.14	163	87070	14.05	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061616\
Data File : BG022368.D
Acq On : 16 Jun 2016 16:17
Operator : UM/SJ
Sample : H3569-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-07-COMP

Quant Time: Jun 17 02:22:30 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

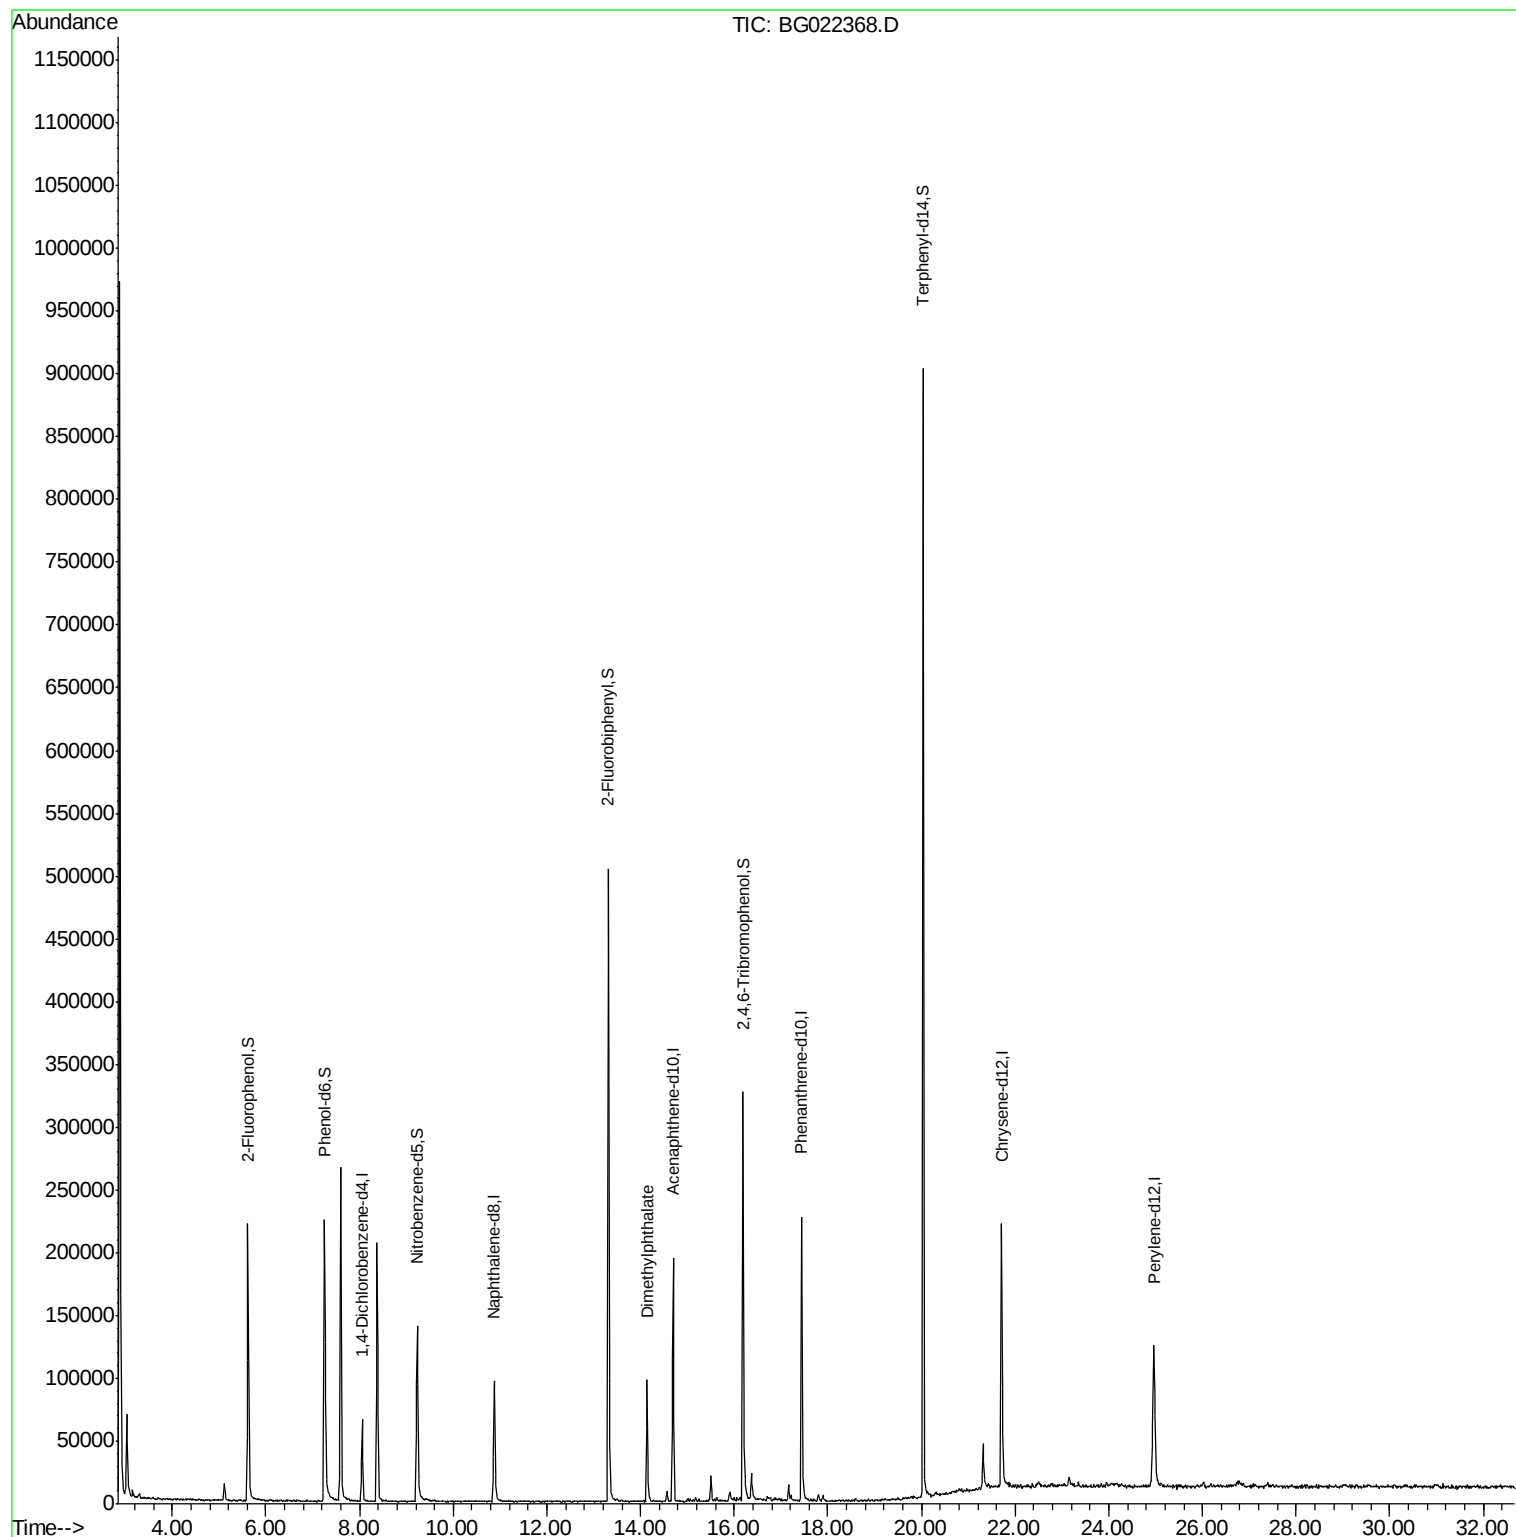




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.05 min Scan# 888
Delta R.T. -0.04 min
Lab File: BG022368.D
Acq: 16 Jun 2016 16:17

Instrument :
BNA_G
ClientSampleId :
SB-07-COMP

Tot Ion:152 Resp: 23723
Ion Ratio Lower Upper
152 100
150 157.9 130.1 195.1
115 59.6 62.2 93.2#

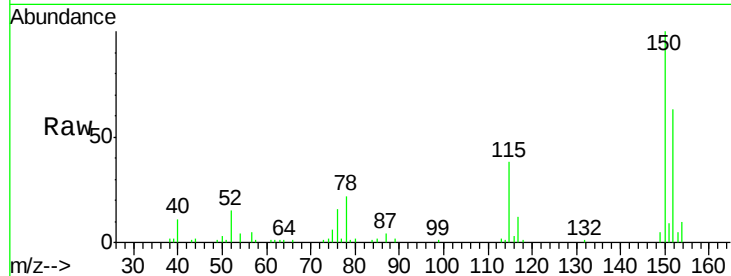


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

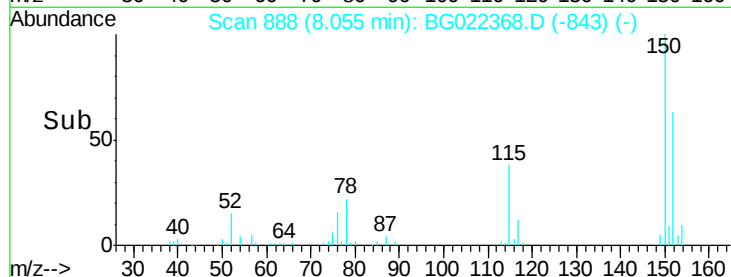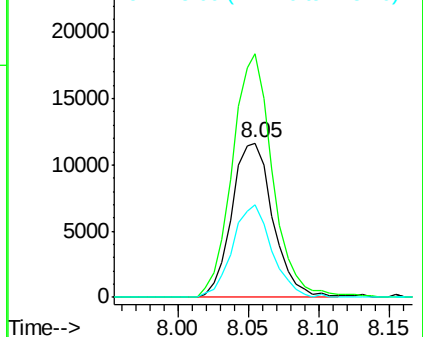



#5

2-Fluorophenol
Concen: 123.41 ng
RT: 5.62 min Scan# 473
Delta R.T. -0.02 min
Lab File: BG022368.D
Acq: 16 Jun 2016 16:17

Tgt Ion:112 Resp: 151420
Ion Ratio Lower Upper
112 100
64 50.7 51.1 76.7#
63 25.5 24.6 37.0

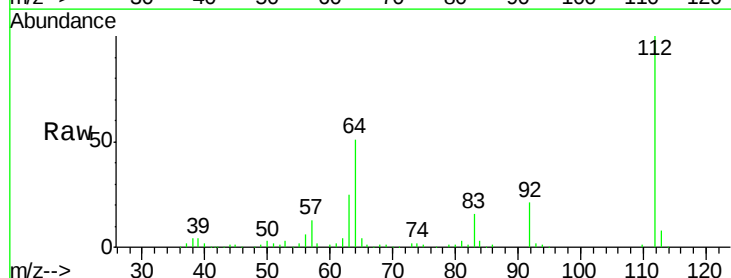

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

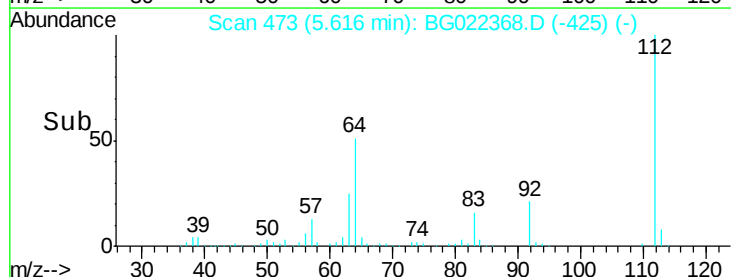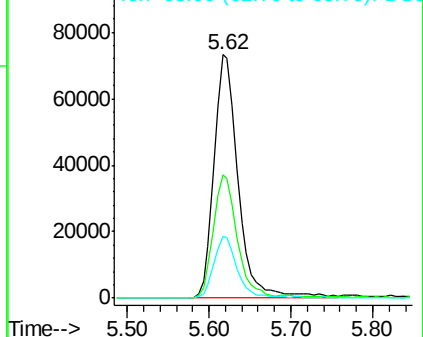



#7

Phenol-d6

Concen: 116.51 ng

RT: 7.26 min Scan# 752

Delta R.T. 0.01 min

Lab File: BG022368.D

Acq: 16 Jun 2016 16:17

Instrument :

BNA_G

ClientSampleId :

SB-07-COMP


Tot Ion: 99 Resp: 224772

Ion Ratio Lower Upper



99 100

42 10.0 16.4 24.6#

71 25.2 25.0 37.4

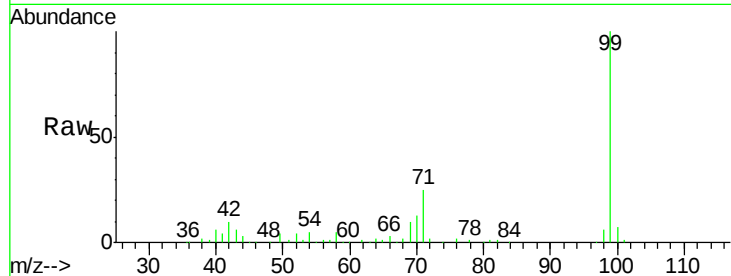

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

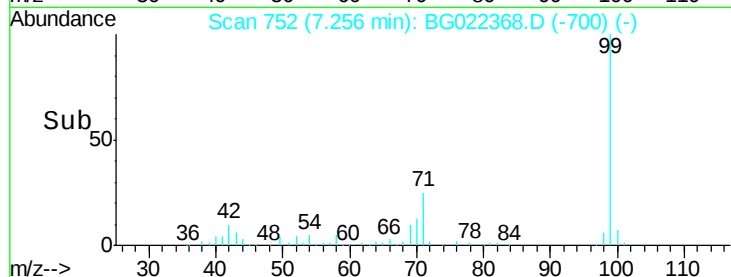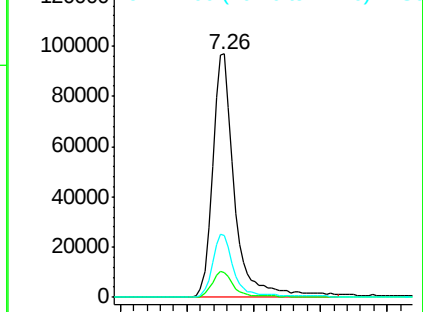

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.87 min Scan# 1368

Delta R.T. -0.03 min

Lab File: BG022368.D

Acq: 16 Jun 2016 16:17

Tgt Ion: 136 Resp: 120023


Ion Ratio Lower Upper

136 100



137 11.1 9.0 13.4

54 6.0 9.6 14.4#

68 5.9 6.4 9.6#

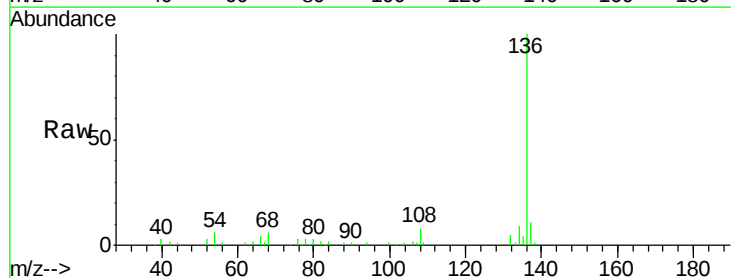

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

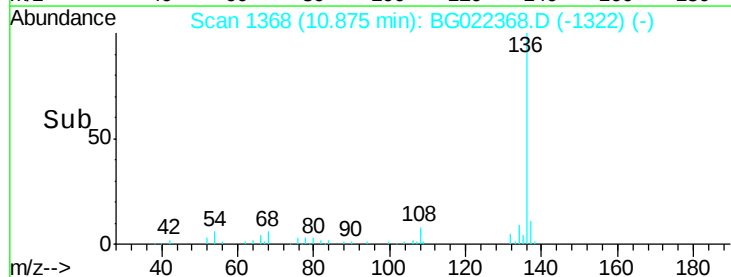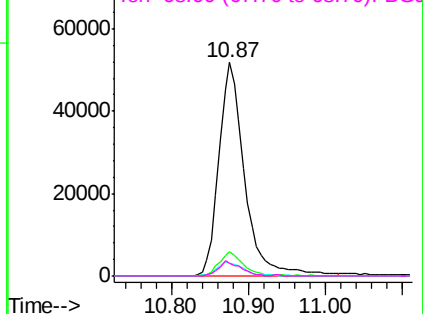






#23
Nitrobenzene-d5
Concen: 71.05 ng
RT: 9.23 min Scan# 1088
Delta R.T. -0.03 min
Lab File: BG022368.D
Acq: 16 Jun 2016 16:17

Instrument :
BNA_G
ClientSampleId :
SB-07-COMP

Tot Ion	82	Resp	122318
Ion Ratio	100		
Lower	33.4		
Upper	50.0		
54	37.0	46.1	69.1#

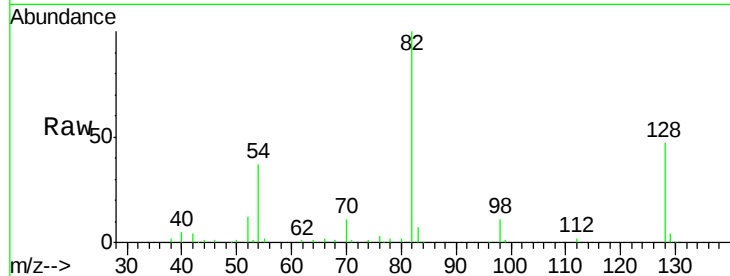


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

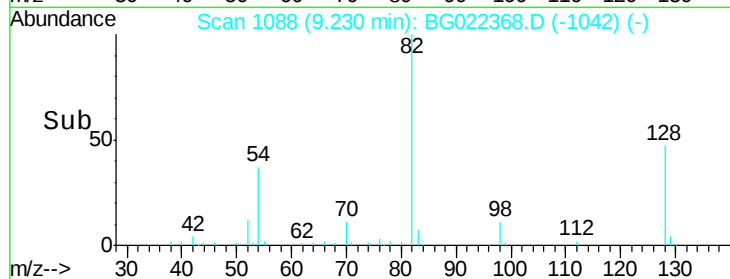
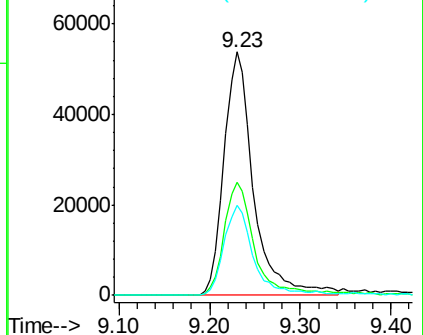



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.69 min Scan# 2018
Delta R.T. -0.03 min
Lab File: BG022368.D
Acq: 16 Jun 2016 16:17

Tgt Ion	164	Resp	74731
Ion Ratio	100		
Lower	78.0		
Upper	117.0		
162	109.5	32.9	49.3

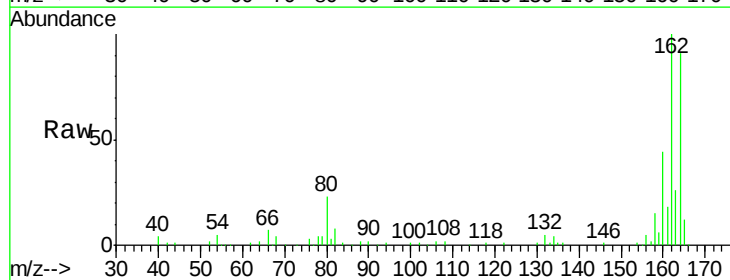

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

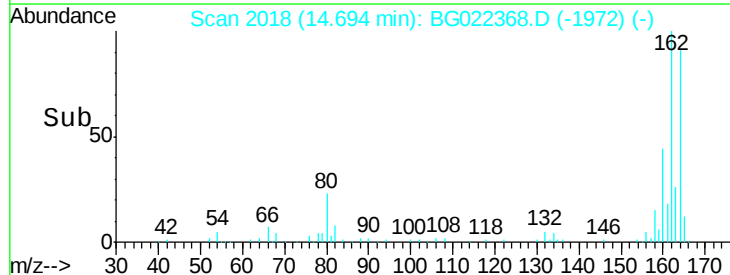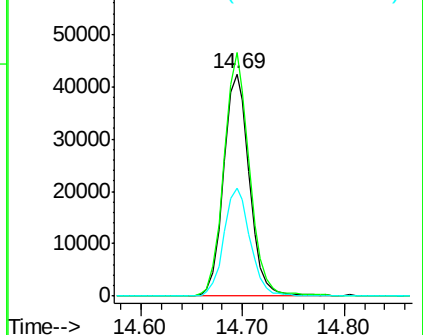


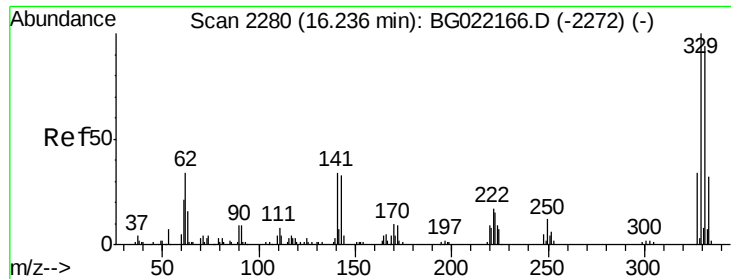




#41
 2,4,6-Tribromophenol
 Concen: 86.65 ng
 RT: 16.19 min Scan# 2272
 Delta R.T. -0.03 min
 Lab File: BG022368.D
 Acq: 16 Jun 2016 16:17

Instrument :
 BNA_G
 ClientSampleId :
 SB-07-COMP

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.7	78.0	117.0
141	46.5	33.8	50.8

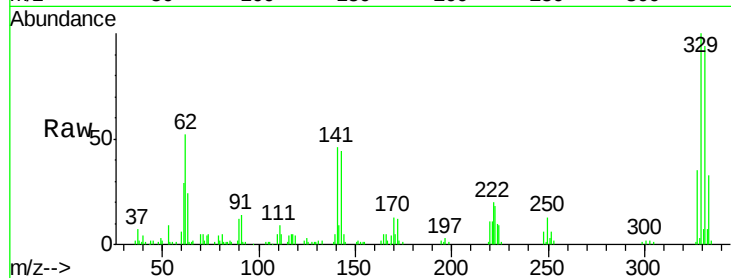


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

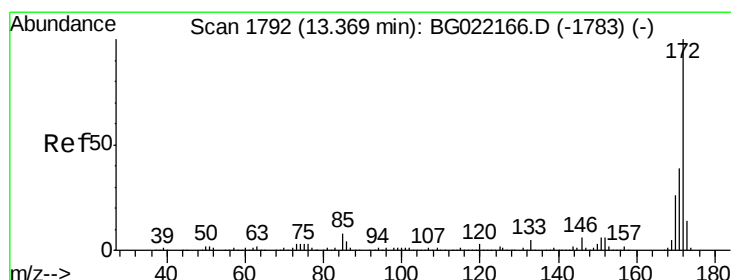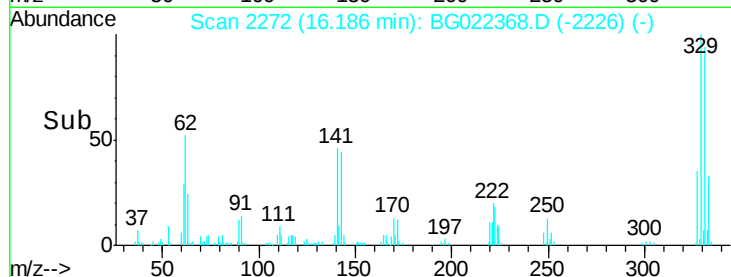
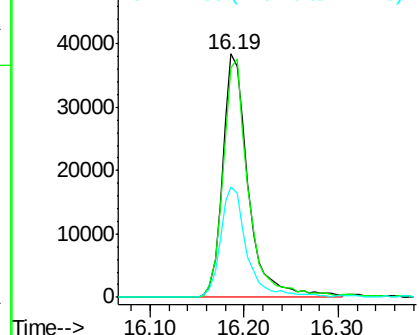



#44
 2-Fluorobiphenyl
 Concen: 65.35 ng
 RT: 13.31 min Scan# 1783
 Delta R.T. -0.03 min
 Lab File: BG022368.D
 Acq: 16 Jun 2016 16:17

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.9	27.8	41.6
170	25.6	19.6	29.4

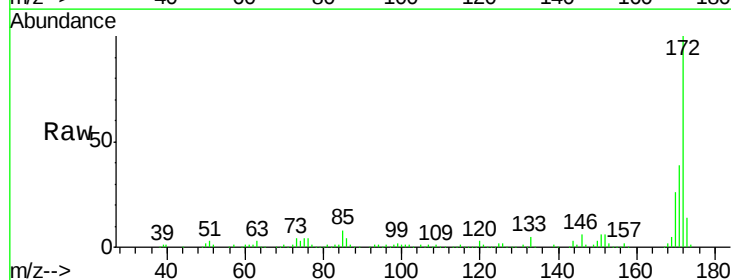

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

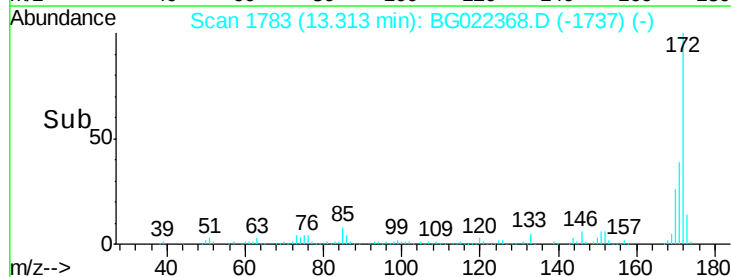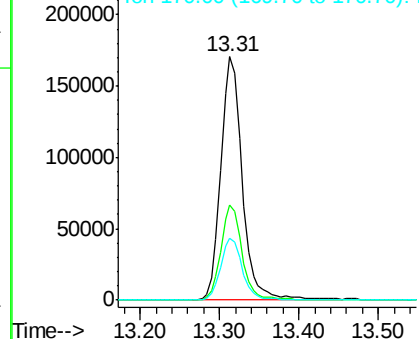

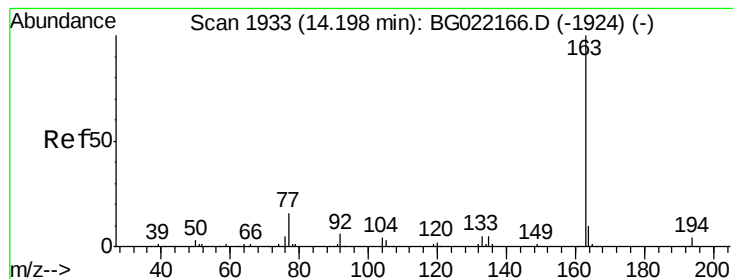

#49

Dimethylphthalate

Concen: 14.05 ng

RT: 14.14 min Scan# 1924

Delta R.T. -0.03 min

Lab File: BG022368.D

Acq: 16 Jun 2016 16:17

Instrument :

BNA_G

ClientSampleId :

SB-07-COMP


Tot Ion:163 Resp: 87070

Ion Ratio Lower Upper

163 100

194 4.2 3.0 4.6




164 10.3 8.1 12.1

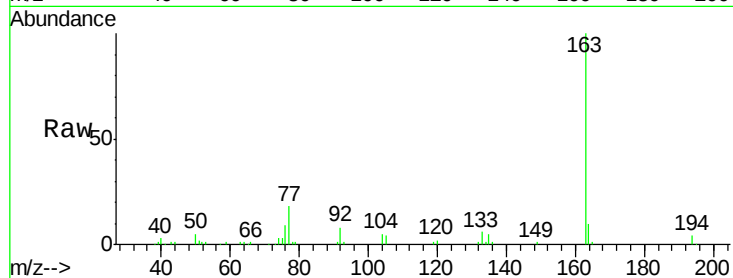

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

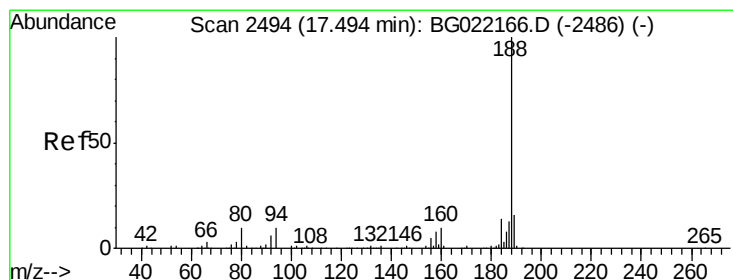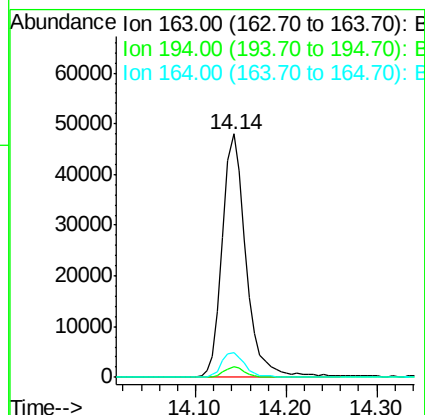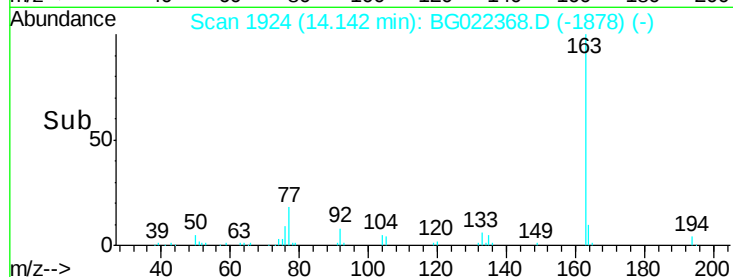

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.44 min Scan# 2485

Delta R.T. -0.03 min

Lab File: BG022368.D

Acq: 16 Jun 2016 16:17


Tgt Ion:188 Resp: 164283

Ion Ratio Lower Upper

188 100

94 10.4 7.5 11.3



80 12.7 8.6 13.0

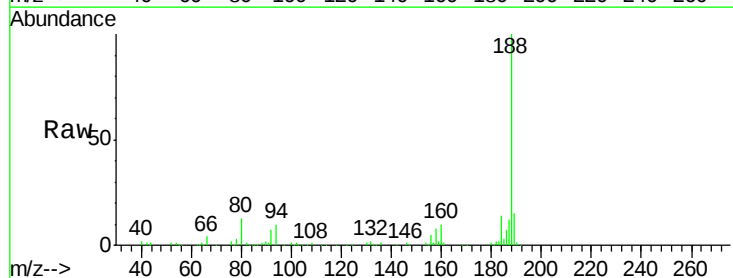

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

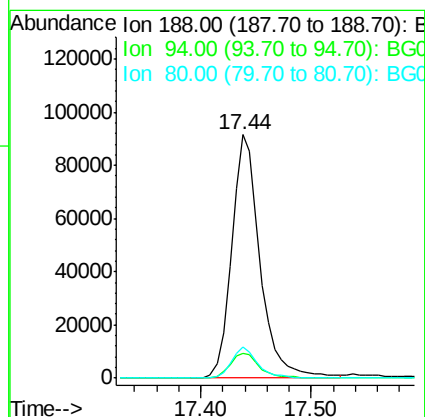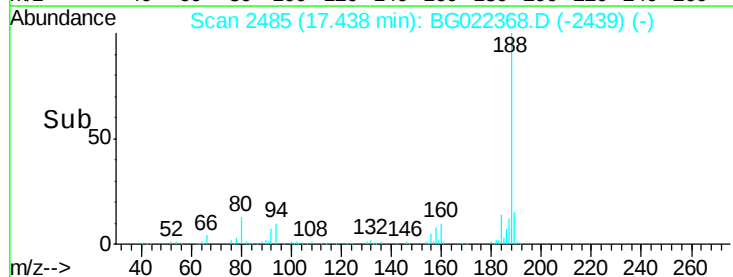



#75

Chrvsene-d12

Concen: 20.00 ng

RT: 21.71 min Scan# 3212

Delta R.T. -0.03 min

Lab File: BG022368.D

Acq: 16 Jun 2016 16:17

Instrument :

BNA_G

ClientSampleId :

SB-07-COMP


Tot Ion:240 Resp: 144780

Ion Ratio Lower Upper

240 100

120 12.4 8.4 12.6




236 26.6 19.6 29.4

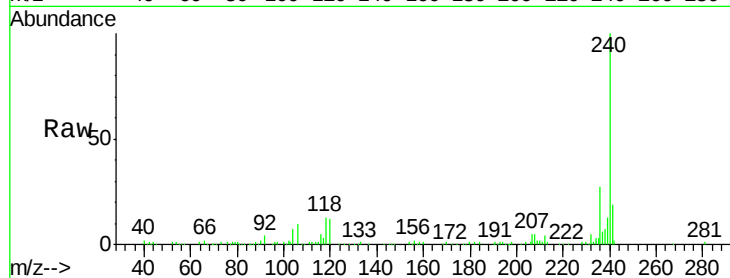

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

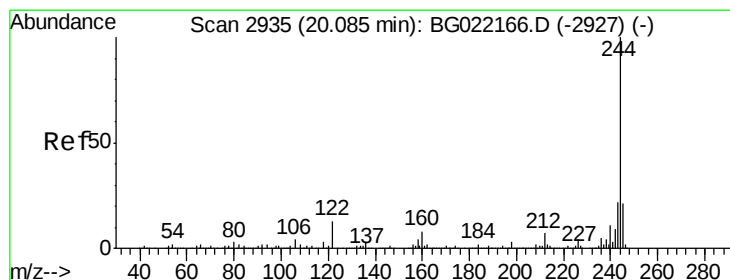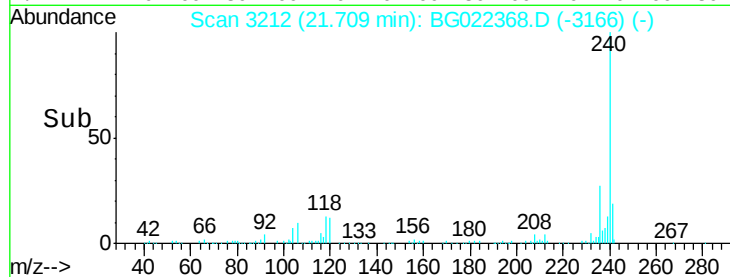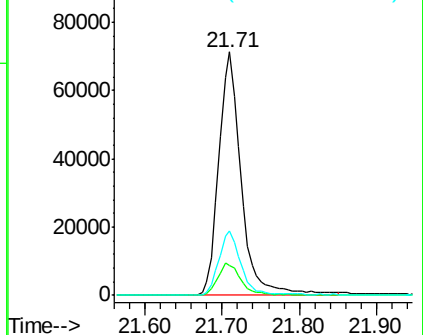

#78

Terphenyl-d14

Concen: 68.76 ng

RT: 20.03 min Scan# 2927

Delta R.T. -0.02 min

Lab File: BG022368.D

Acq: 16 Jun 2016 16:17


Tgt Ion:244 Resp: 419330

Ion Ratio Lower Upper

244 100

212 7.6 6.5 9.7



122 13.9 8.6 12.8#

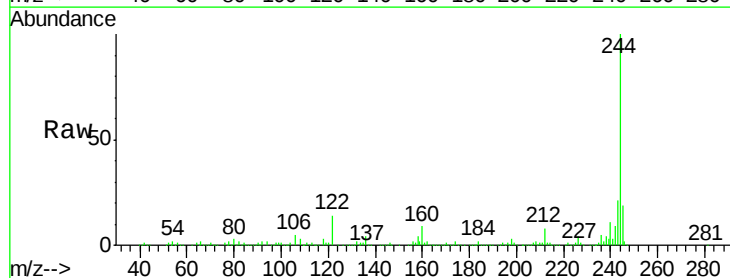


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

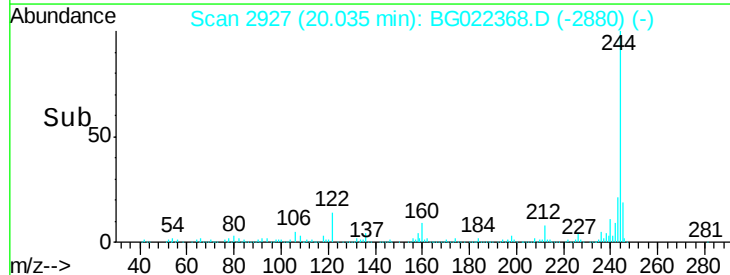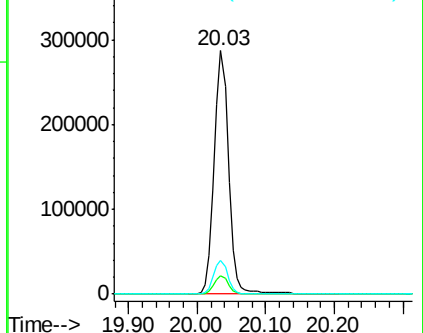


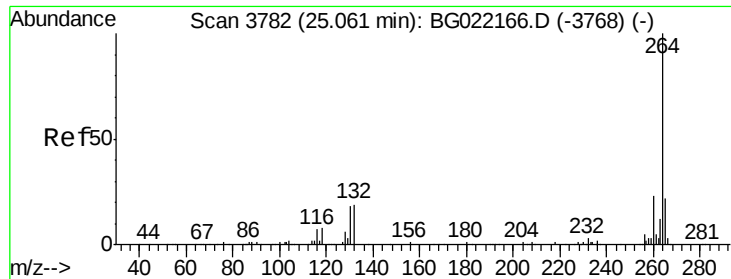

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 24.96 min Scan# 3766
 Delta R.T. -0.05 min
 Lab File: BG022368.D
 Acq: 16 Jun 2016 16:17

Instrument :
 BNA_G
 ClientSampleId :
 SB-07-COMP

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.4	20.2	30.4
265	20.6	17.8	26.8

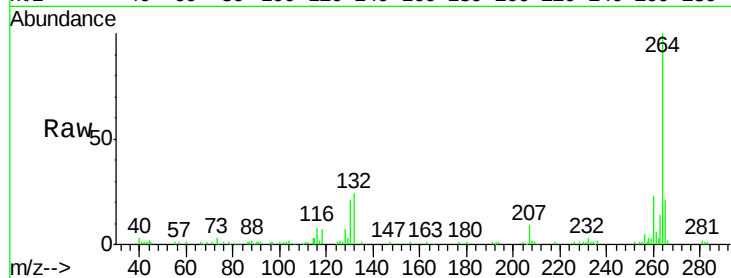

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

