


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061616\
 Data File : BG022364.D
 Acq On : 16 Jun 2016 13:31
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 17:40:23 2016

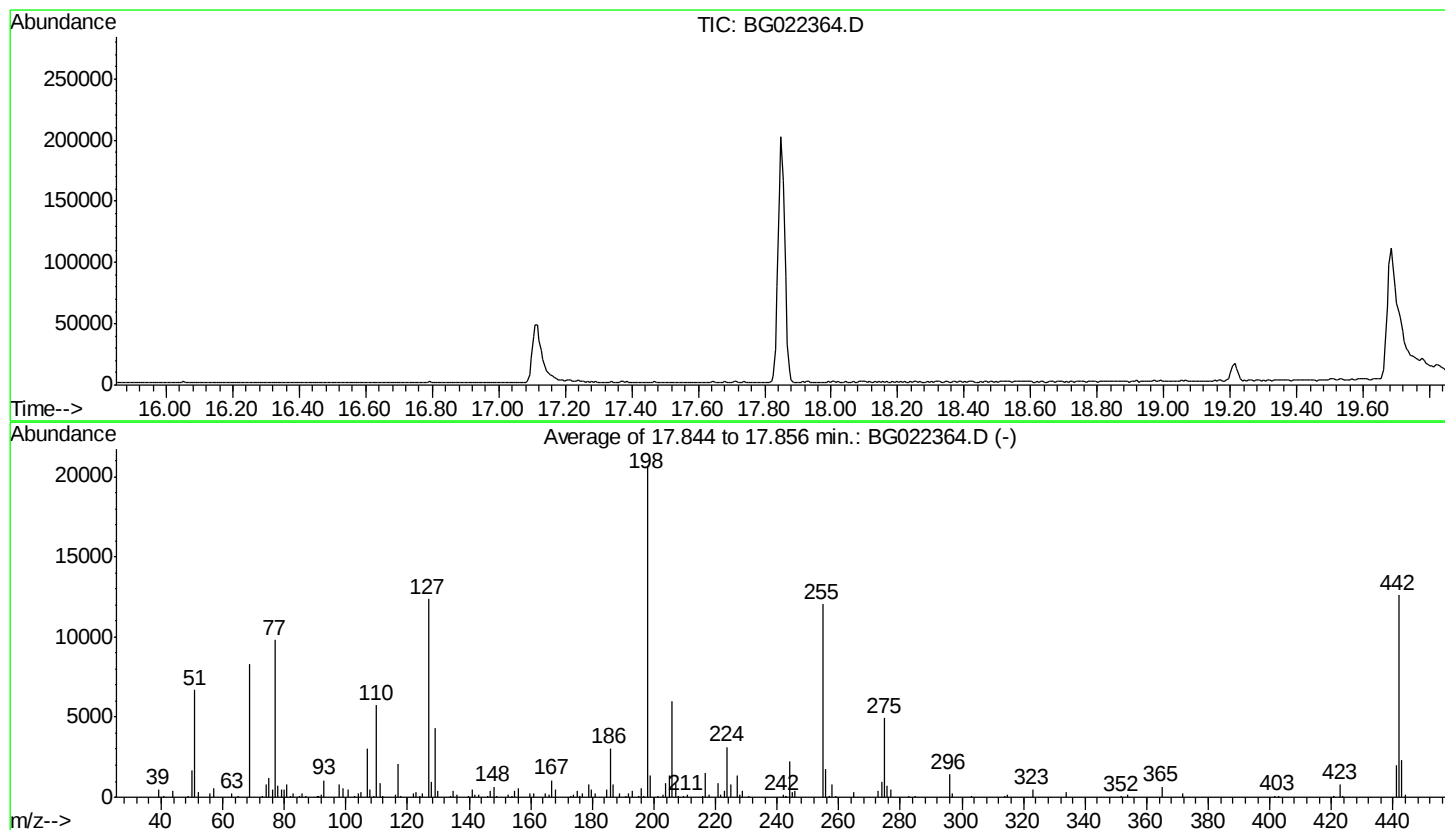

AutoFind: Scans 2554, 2555, 2556; Background Corrected with Scan 2548

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	6684	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.0	8279	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.7	12352	PASS
197	198	0.00	2	0.3	68	PASS
198	198	100	100	100.0	20682	PASS
199	198	5	9	6.6	1367	PASS
275	198	10	60	23.8	4914	PASS
365	198	1	100	3.3	673	PASS
441	442	0.01	24	16.1	2029	PASS
442	198	50	100	61.0	12610	PASS
443	442	15	24	18.5	2330	PASS