


Data Path : Z:\HPCHEM1\BNA G\DATA\BG061616\
 Data File : BG022382.D
 Acq On : 17 Jun 2016 1:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 17:40:23 2016

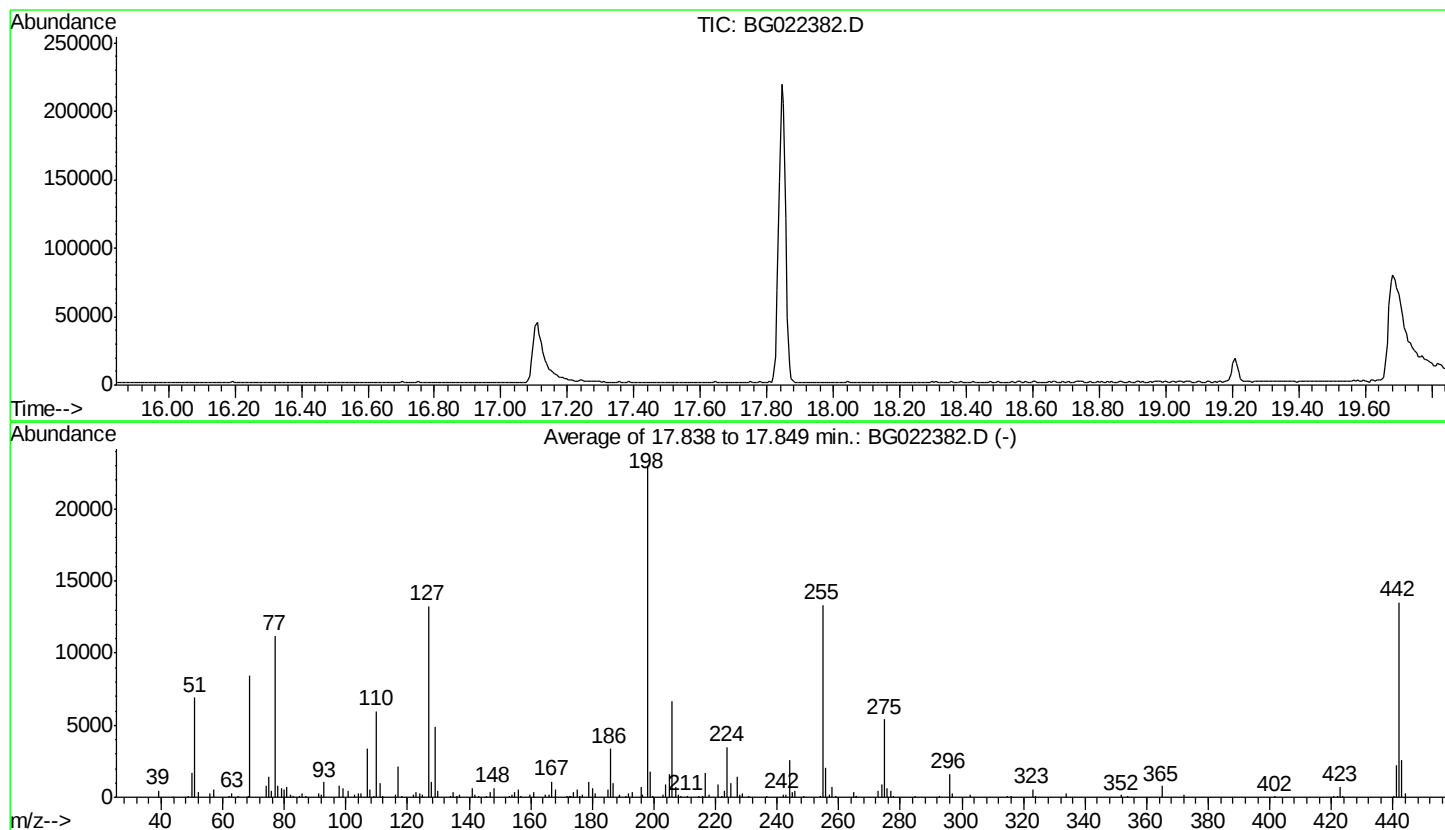

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	6913	PASS
68	69	0.00	2	0.8	65	PASS
69	198	0.00	100	36.7	8445	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.5	13240	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23018	PASS
199	198	5	9	7.6	1746	PASS
275	198	10	60	23.5	5411	PASS
365	198	1	100	3.4	790	PASS
441	442	0.01	24	16.5	2228	PASS
442	198	50	100	58.7	13516	PASS
443	442	15	24	19.0	2565	PASS