

Data File : BG027482.D
Acq On : 16 Jun 2017 22:03
Operator : SJ/MA
Sample : PB99730BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK30

Quant Time: Jun 16 22:57:20 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 16 22:56:07 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.52	152	40733	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	204160	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.11	164	137338	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.86	188	338922	20.00	ng/ul	0.00
75) Chrysene-d12	22.23	240	349792	20.00	ng/ul	0.00
83) Perylene-d12	25.89	264	333752	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	4.08	96	6395	6.28	ng/uL	0.00
5) Phenol-d5	7.66	99	126929	28.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.83	67	97975	32.54	ng/ul	0.00
9) 2-Chlorophenol-d4	8.05	132	91874	31.48	ng/ul	0.00
13) 4-Methylphenol-d8	9.20	113	105889	30.66	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	47714	32.17	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	54279	34.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	91467	30.73	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	142820	37.90	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	369984	32.18	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	420878	31.78	ng/ul	0.00
51) 4-Nitrophenol-d4	15.27	143	63046	28.03	ng/ul	0.00
57) Fluorene-d10	16.09	176	321762	29.83	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.19	200	57846	27.48	ng/ul	0.00
70) Anthracene-d10	17.96	188	526859	33.34	ng/ul	0.00
76) Pyrene-d10	20.22	212	572550	33.52	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.64	264	493830	32.86	ng/ul	0.00

Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	9.19	70	3253	1.08 ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG027482.D

Acq On : 16 Jun 2017 22:03

Operator : SJ/MA

Sample : PB99730BL

Misc :

ALS Vial : 16 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

SBLK30


Quant Time: Jun 16 22:57:20 2017




Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Jun 16 22:56:07 2017

Response via : Initial Calibration

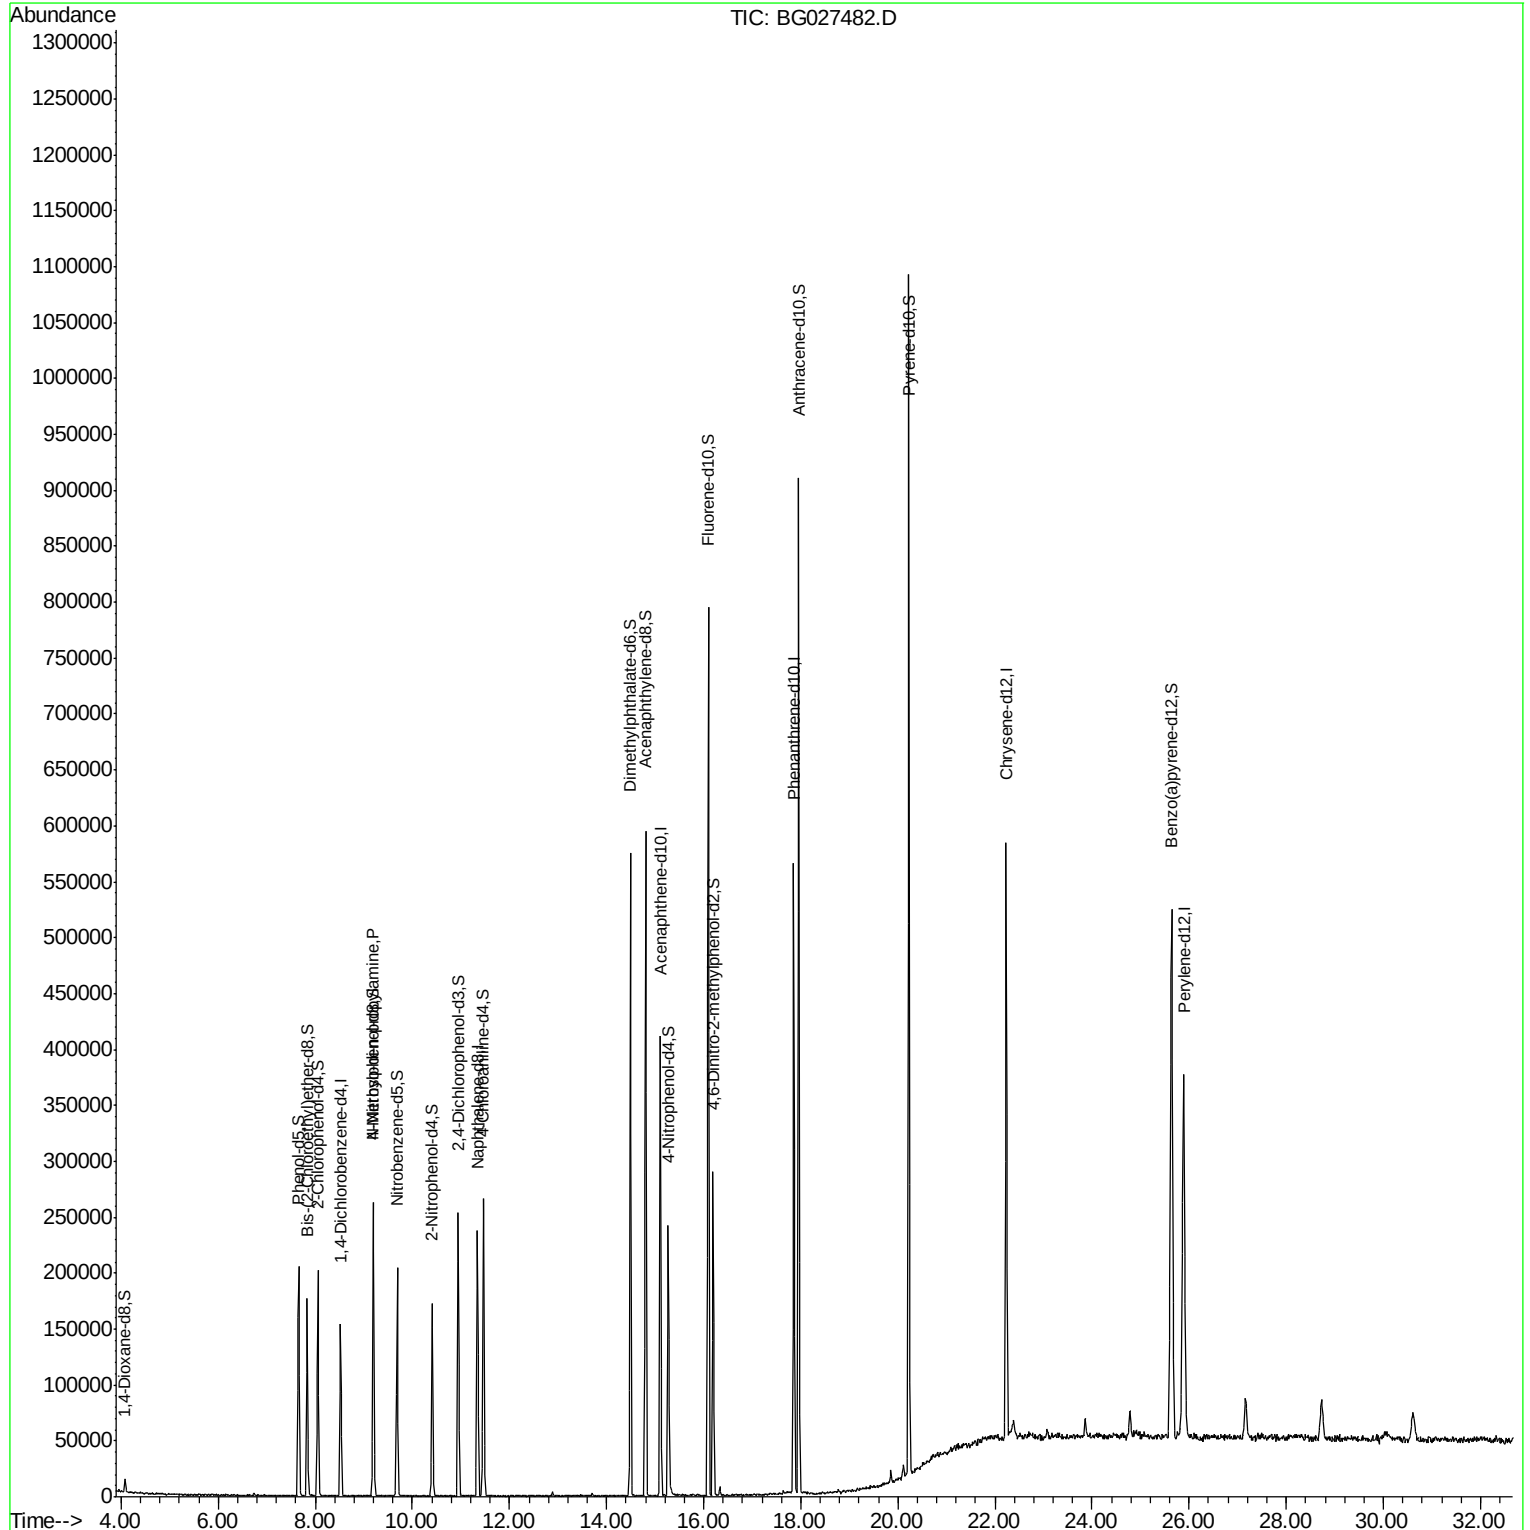

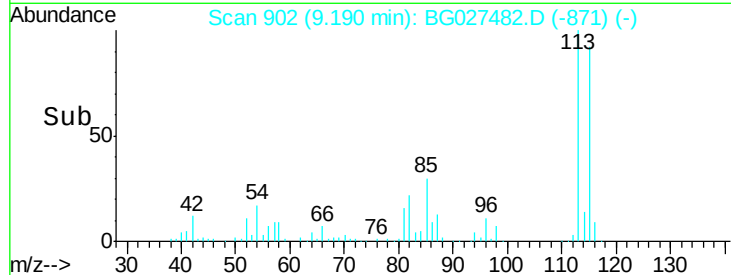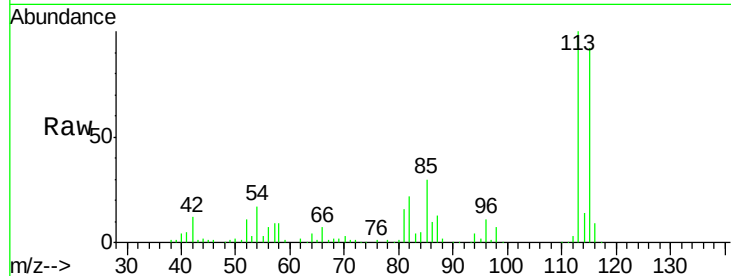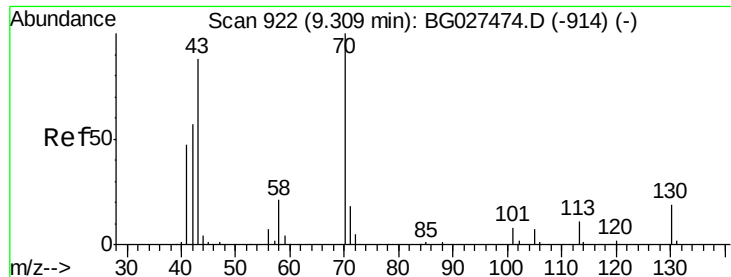

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.08 ng/ul
 RT: 9.19 min Scan# 902
 Delta R.T. -0.12 min
 Lab File: BG027482.D
 Acq: 16 Jun 2017 22:03

Instrument :
 BNA_G
 ClientSampleId :
 SBLK30

Tgt Ion:	70	Resp:	3253
Ion	Ratio	Lower	Upper
70	100		
42	367.8	59.0	88.6#
101	0.0	6.6	9.8#
130	0.0	15.6	23.4#

