

Data File : BG027483.D
Acq On : 16 Jun 2017 22:42
Operator : SJ/MA
Sample : PB99744BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK44

Quant Time: Jun 16 23:40:13 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 16 22:56:07 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.52	152	41133	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	206859	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.11	164	141883	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.86	188	362867	20.00	ng/ul	0.00
75) Chrysene-d12	22.23	240	373990	20.00	ng/ul	0.00
83) Perylene-d12	25.89	264	358897	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	4.08	96	7768	7.55	ng/uL	0.00
5) Phenol-d5	7.66	99	160344	35.95	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.83	67	118411	38.95	ng/ul	0.00
9) 2-Chlorophenol-d4	8.05	132	111849	37.95	ng/ul	0.00
13) 4-Methylphenol-d8	9.20	113	131002	37.56	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	59548	39.63	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	65855	41.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	112089	37.16	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	181418	47.52	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	484646	40.80	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	538995	39.39	ng/ul	0.00
51) 4-Nitrophenol-d4	15.27	143	84341	36.29	ng/ul	0.00
57) Fluorene-d10	16.09	176	423280	37.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.19	200	78288	34.74	ng/ul	0.00
70) Anthracene-d10	17.96	188	692708	40.94	ng/ul	0.00
76) Pyrene-d10	20.22	212	757852	41.49	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.64	264	667439	41.30	ng/ul	0.00

Target Compounds				Qvalue		
15) N-Nitroso-di-n-propylamine	9.20	70	3457	1.14	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG027483.D

Acq On : 16 Jun 2017 22:42

Operator : SJ/MA

Sample : PB99744BL

Misc :

ALS Vial : 17 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

SBLK44


Quant Time: Jun 16 23:40:13 2017




Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Jun 16 22:56:07 2017

Response via : Initial Calibration

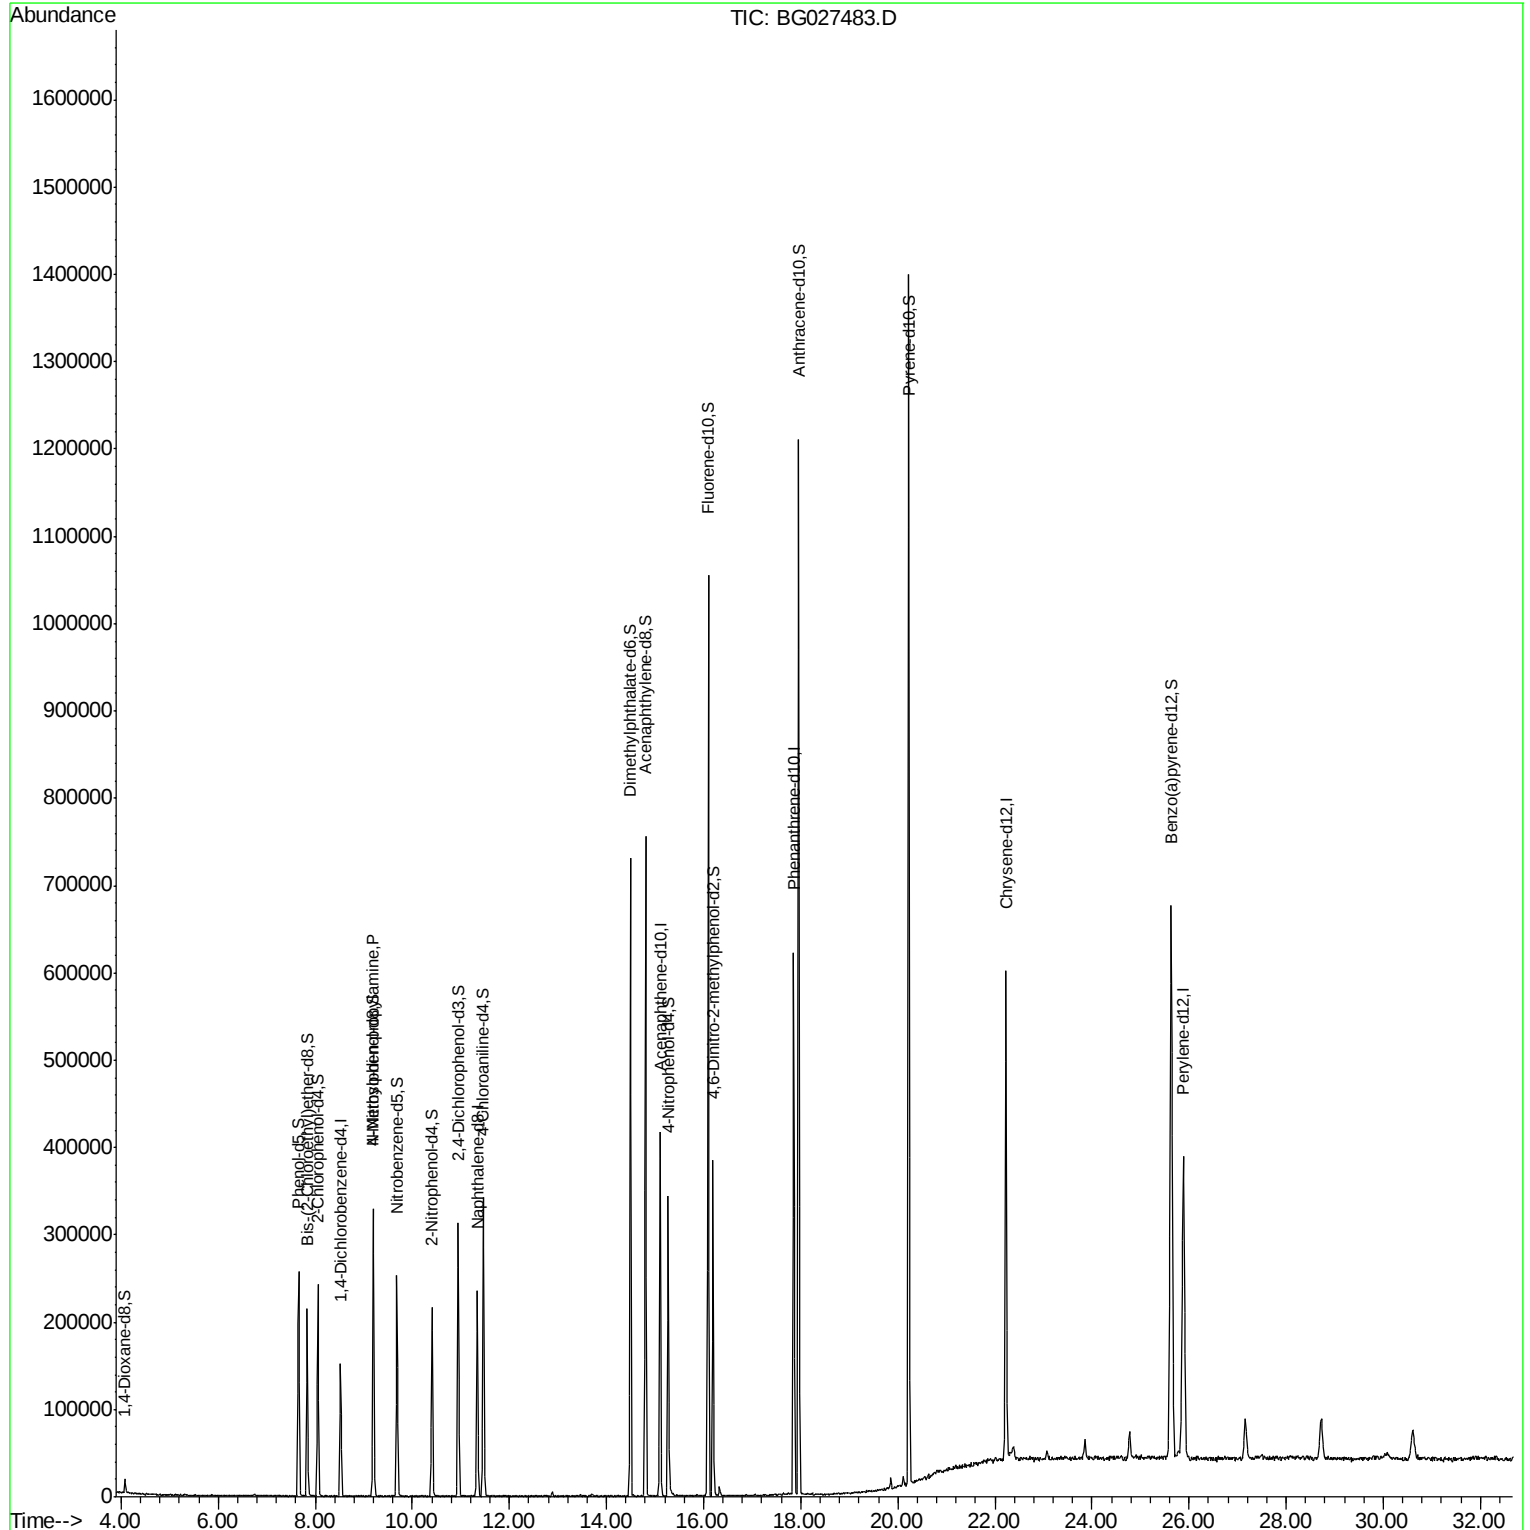

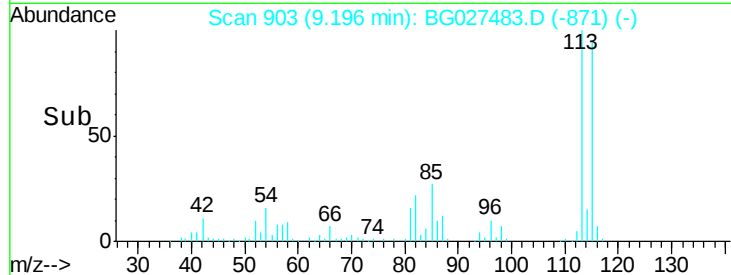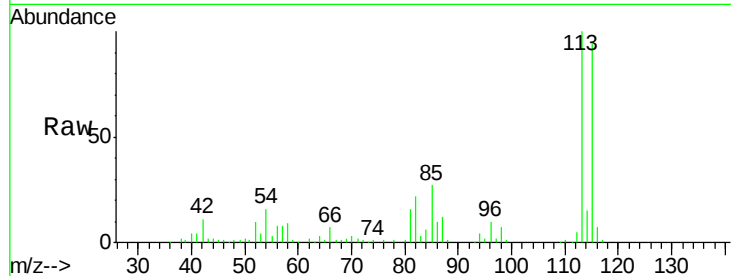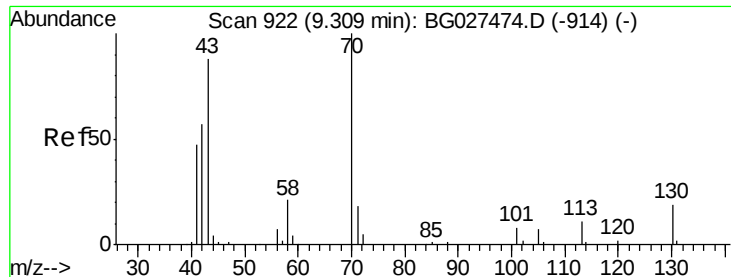

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.14 ng/ul
 RT: 9.20 min Scan# 903
 Delta R.T. -0.11 min
 Lab File: BG027483.D
 Acq: 16 Jun 2017 22:42

Instrument :
 BNA_G
 ClientSampleId :
 SBLK44

Tgt Ion:	70	Resp:	3457
Ion Ratio	Lower	Upper	
70	100		
42	378.1	59.0	88.6#
101	0.0	6.6	9.8#
130	0.0	15.6	23.4#

