

Data File : BG027498.D
Acq On : 17 Jun 2017 8:35
Operator : SJ/MA
Sample : PB99687BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK87

Quant Time: Jun 19 00:58:03 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 19 00:57:08 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.52	152	42726	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	221068	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.11	164	148725	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.86	188	361142	20.00	ng/ul	0.00
75) Chrysene-d12	22.23	240	375539	20.00	ng/ul	0.00
83) Perylene-d12	25.88	264	363364	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	4.08	96	7753	7.26	ng/uL	0.00
5) Phenol-d5	7.65	99	167636	36.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.83	67	126247	39.98	ng/ul	0.00
9) 2-Chlorophenol-d4	8.05	132	117435	38.36	ng/ul	0.00
13) 4-Methylphenol-d8	9.20	113	137302	37.90	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	62127	38.69	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	68233	39.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	118639	36.81	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	187285	45.90	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	476247	38.25	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	542627	37.84	ng/ul	0.00
51) 4-Nitrophenol-d4	15.27	143	81687	33.53	ng/ul	0.00
57) Fluorene-d10	16.09	176	421339	36.07	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.19	200	78972	35.21	ng/ul	0.00
70) Anthracene-d10	17.96	188	689919	40.97	ng/ul	0.00
76) Pyrene-d10	20.23	212	750987	40.95	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.64	264	671125	41.02	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	9.19	70	4156	1.31 ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG027498.D
Acq On : 17 Jun 2017 8:35
Operator : SJ/MA
Sample : PB99687BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK87

Quant Time: Jun 19 00:58:03 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 19 00:57:08 2017
Response via : Initial Calibration

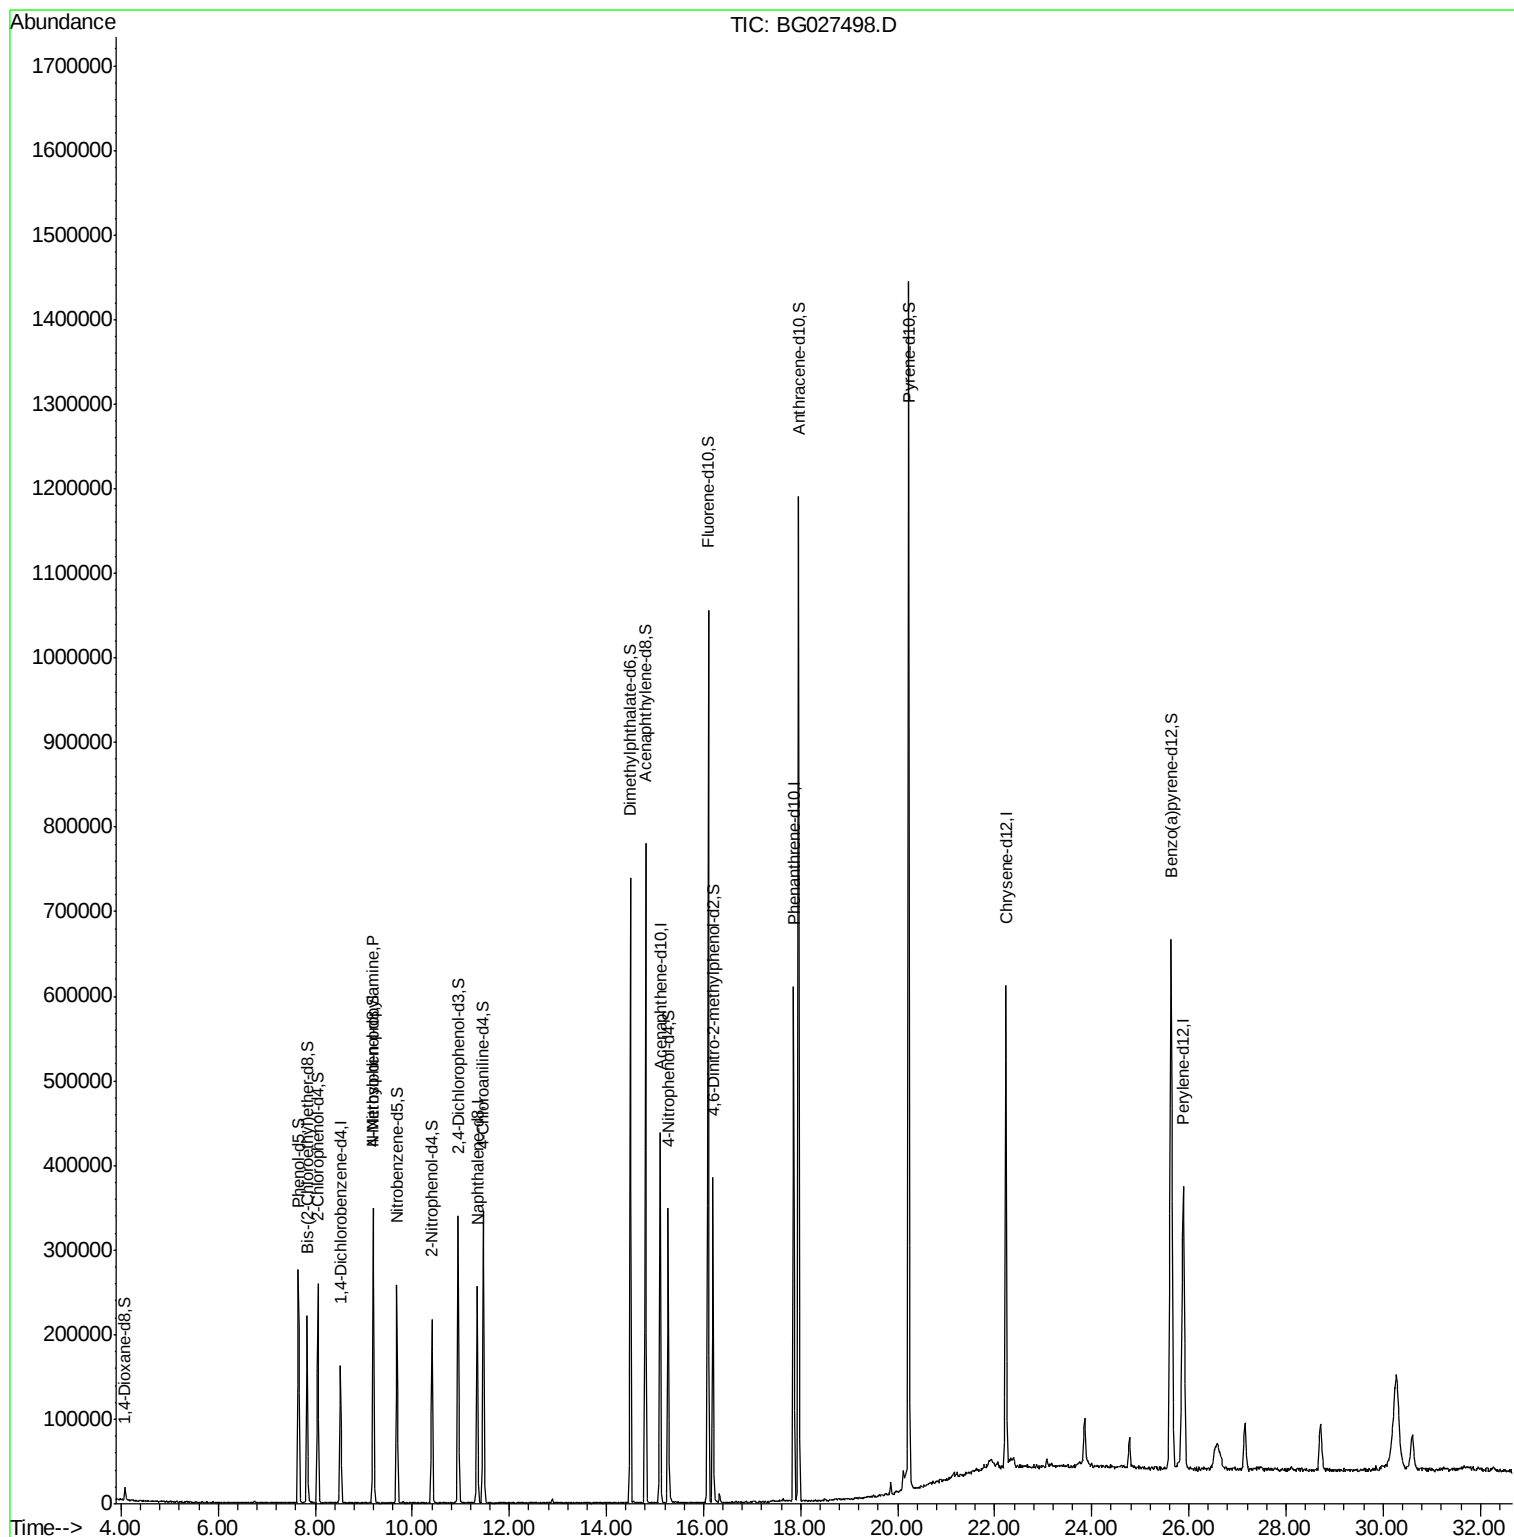

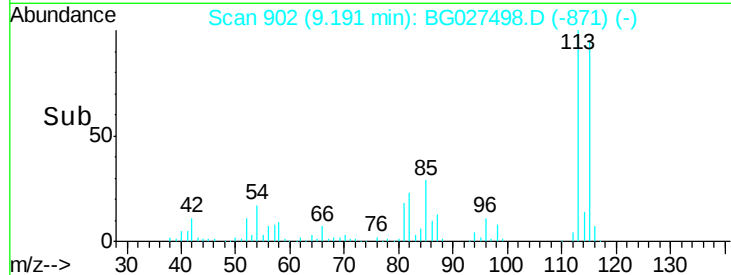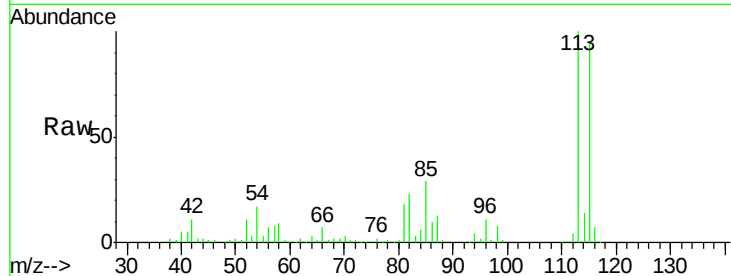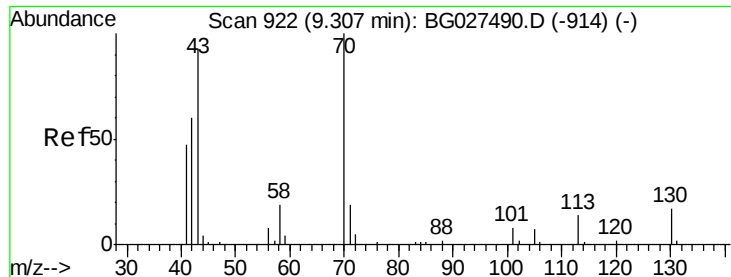

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.31 ng/ul
 RT: 9.19 min Scan# 902
 Delta R.T. -0.12 min
 Lab File: BG027498.D
 Acq: 17 Jun 2017 8:35

Instrument :
 BNA_G
 ClientSampleId :
 SBLK87

Tgt Ion:	70	Resp:	4156
Ion	Ratio	Lower	Upper
70	100		
42	369.4	59.0	88.6#
101	0.0	6.6	9.8#
130	0.0	15.6	23.4#

