

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
 Data File : BG027497.D
 Acq On : 17 Jun 2017 7:56
 Operator : SJ/MA
 Sample : I3600-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 F5A16

Quant Time: Jun 19 01:08:17 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 19 00:57:08 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.52	152	46936	20.00	ng/ul	0.00
18) Naphthalene-d8	11.34	136	236459	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.11	164	153790	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.86	188	359352	20.00	ng/ul	0.00
75) Chrysene-d12	22.23	240	375155	20.00	ng/ul	0.00
83) Perylene-d12	25.89	264	365200	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	4.08	96	5655	4.82	ng/uL	0.00
5) Phenol-d5	7.66	99	28648	5.63	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.83	67	90740	26.16	ng/ul	0.00
9) 2-Chlorophenol-d4	8.06	132	71325	21.21	ng/ul	0.00
13) 4-Methylphenol-d8	9.20	113	54631	13.73	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	45622	26.56	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	50921	27.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	87704	25.44	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	9322	2.14	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	350385	27.21	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	416885	28.11	ng/ul	0.00
51) 4-Nitrophenol-d4	15.28	143	10875	4.32	ng/ul	0.00
57) Fluorene-d10	16.09	176	313672	25.97	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.19	200	55354	24.80	ng/ul	0.00
70) Anthracene-d10	17.96	188	496294	29.62	ng/ul	0.00
76) Pyrene-d10	20.22	212	542935	29.64	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.64	264	477476	29.04	ng/ul	0.00
Target Compounds						
6) Phenol	7.69	94	16286	3.053	ng/ul#	83
44) Dimethylphthalate	14.54	163	237361	18.585	ng/ul	99
81) Bis(2-ethylhexyl)phthalate	22.06	149	252536	21.040	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
Data File : BG027497.D
Acq On : 17 Jun 2017 7:56
Operator : SJ/MA
Sample : I3600-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
F5A16

Quant Time: Jun 19 01:08:17 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 19 00:57:08 2017
Response via : Initial Calibration

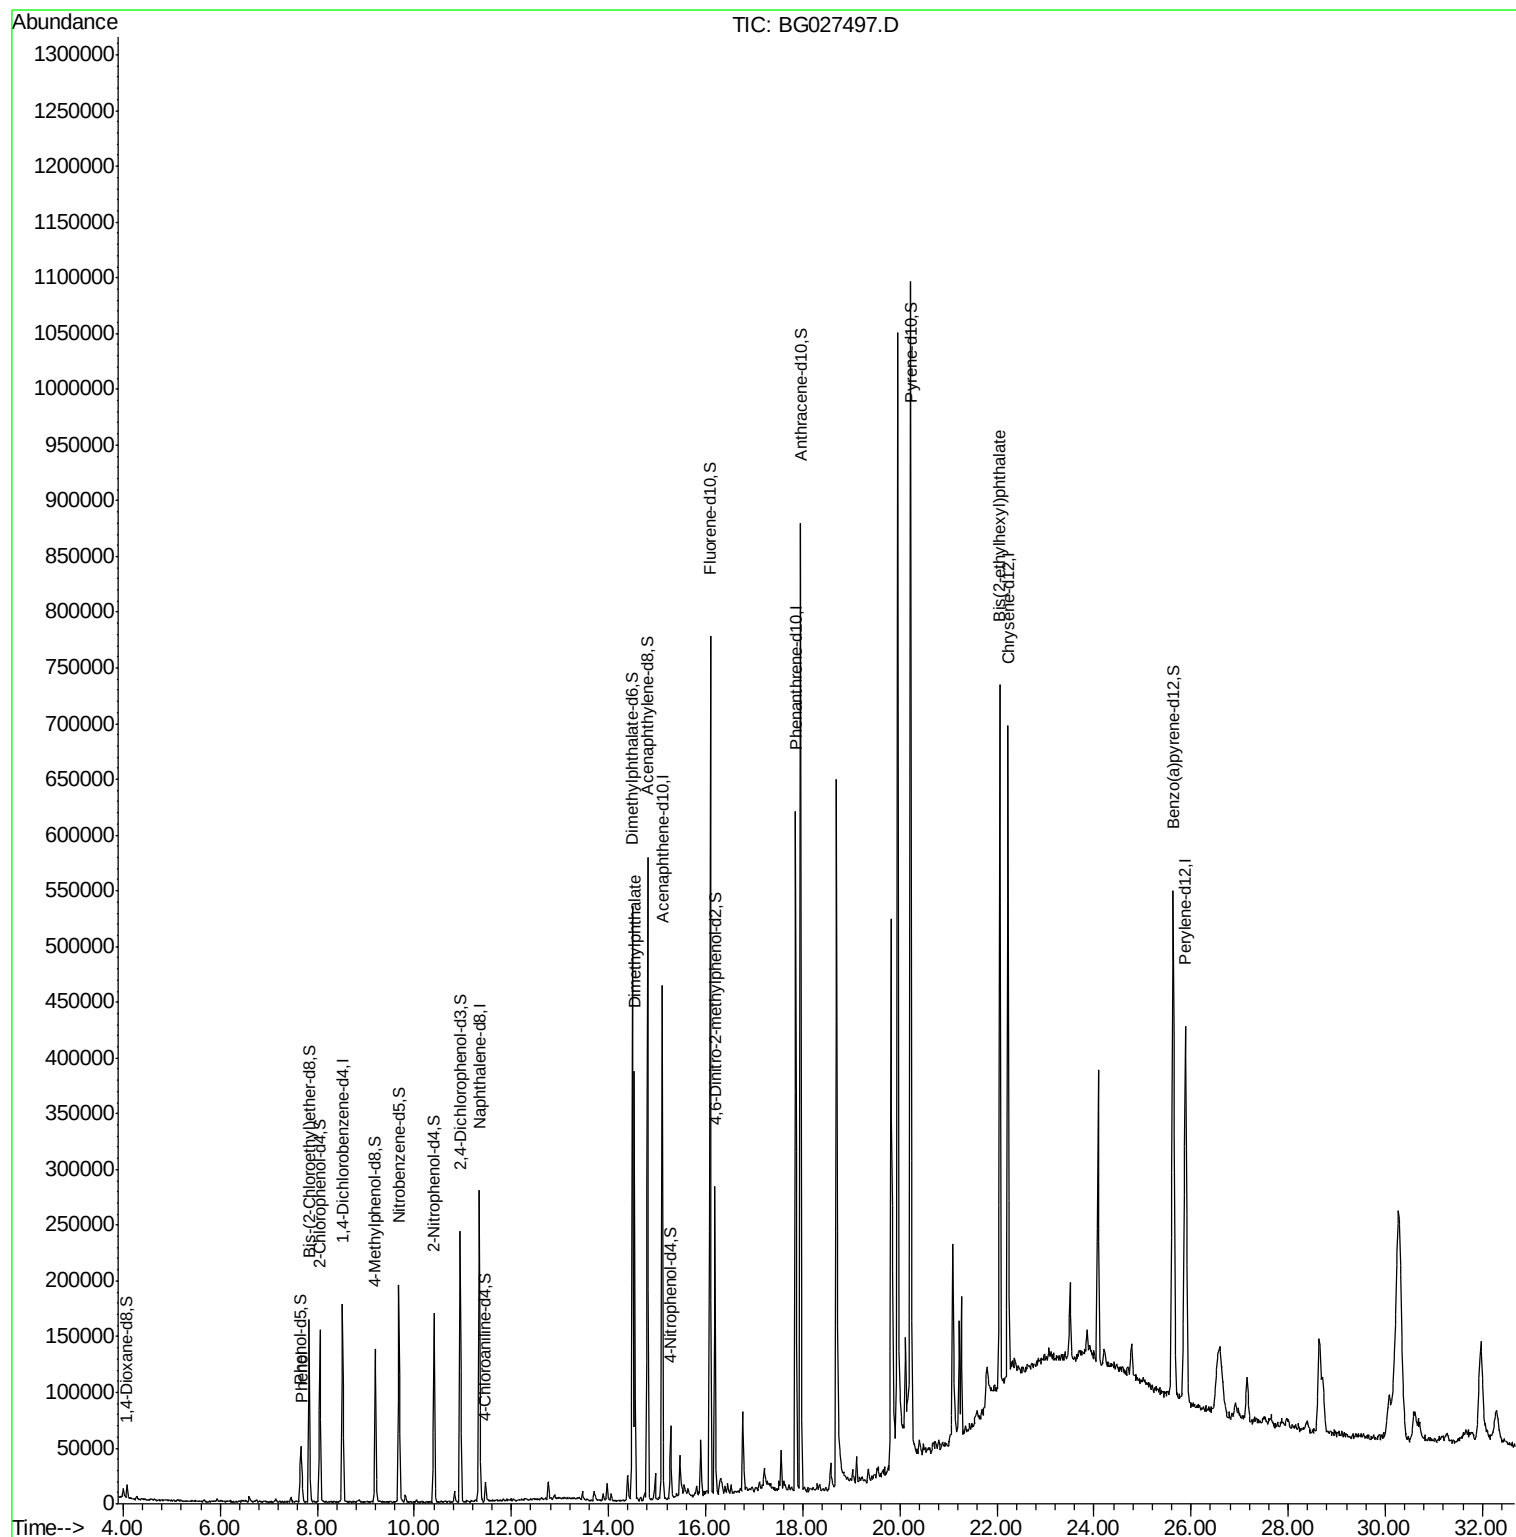

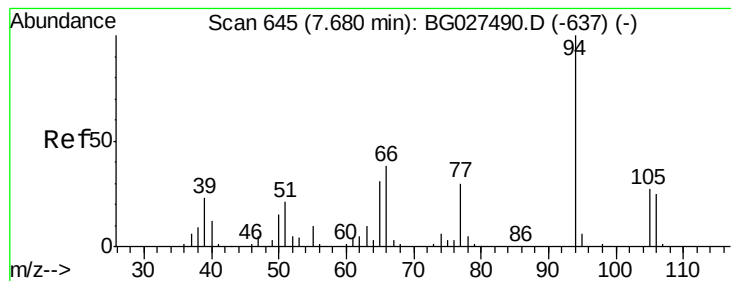

#6

Phenol

Concen: 3.053 ng/ul

RT: 7.69 min Scan# 646

Delta R.T. 0.01 min

Lab File: BG027497.D

Acq: 17 Jun 2017 7:56

Instrument :

BNA_G

ClientSampleId :

F5A16


Tgt Ion: 94 Resp: 16286

Ion Ratio Lower Upper




94 100

65 31.4 26.8 40.2

66 37.4 44.4 66.6#

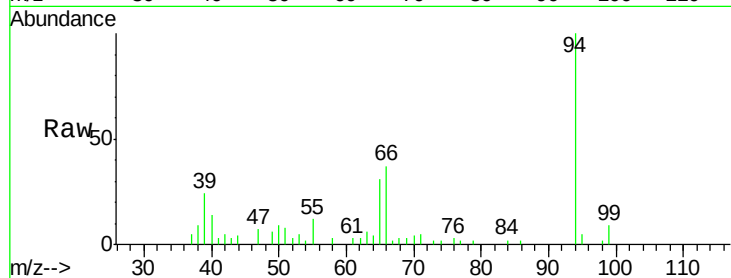

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

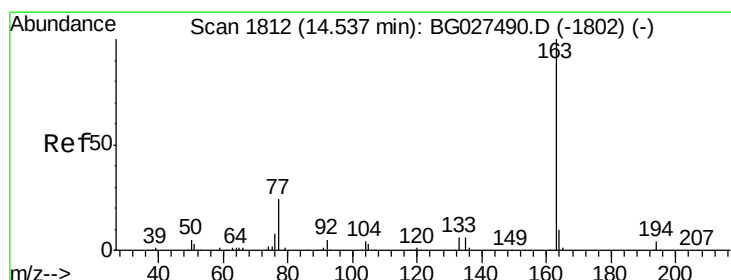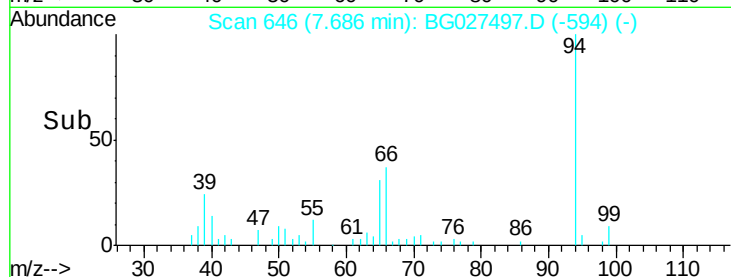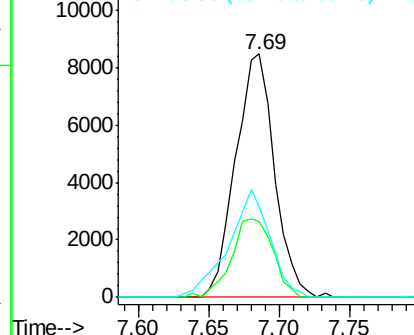

#44

Dimethylphthalate

Concen: 18.585 ng/ul

RT: 14.54 min Scan# 1812

Delta R.T. -0.00 min

Lab File: BG027497.D

Acq: 17 Jun 2017 7:56


Tgt Ion: 163 Resp: 237361

Ion Ratio Lower Upper



163 100


194 4.2 3.4 5.0

164 10.5 9.0 13.4

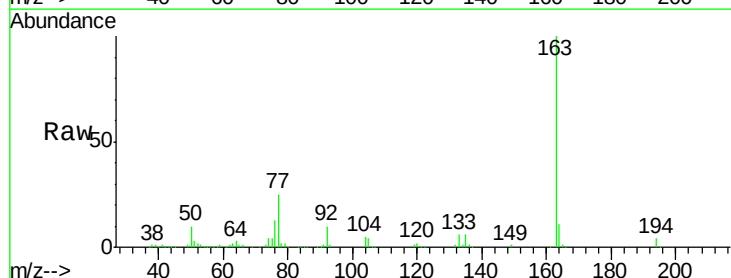

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

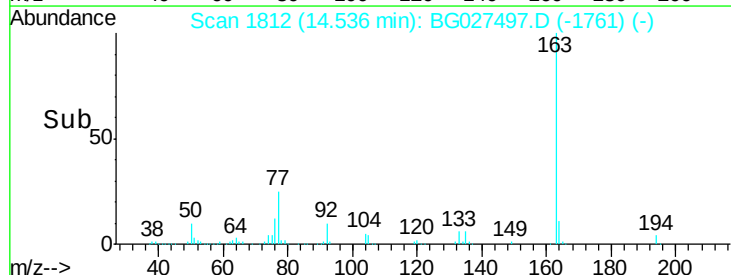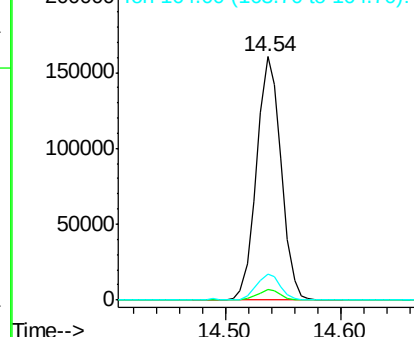

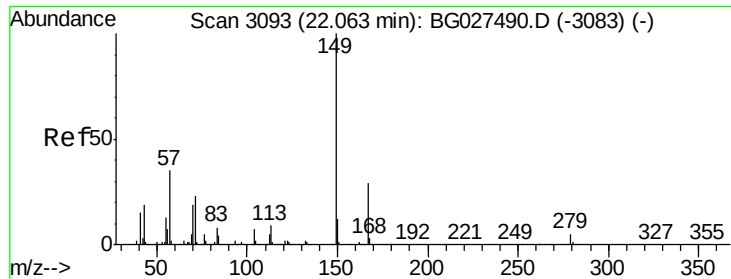

#81

Bis(2-ethylhexyl)phthalate

Concen: 21.040 ng/ul

RT: 22.06 min Scan# 3093

Delta R.T. -0.00 min

Lab File: BG027497.D

Acq: 17 Jun 2017 7:56

Instrument :

BNA_G

ClientSampleId :

F5A16


Tgt Ion:149 Resp: 252536

Ion Ratio Lower Upper

149 100

167 28.0 21.8 32.8

279 4.7 4.5 6.7

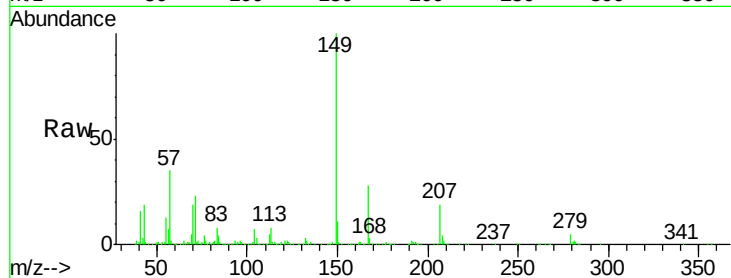

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

