

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
 Data File : BG027504.D
 Acq On : 17 Jun 2017 12:32
 Operator : SJ/MA
 Sample : I3599-17
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 F5C93

Quant Time: Jun 19 00:59:20 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 19 00:57:08 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.52	152	40621	20.00	ng/ul	0.00
18) Naphthalene-d8	11.33	136	206688	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.11	164	141762	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.86	188	344420	20.00	ng/ul	0.00
75) Chrysene-d12	22.23	240	361854	20.00	ng/ul	0.00
83) Perylene-d12	25.88	264	349388	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	4.07	96	4489	4.42	ng/uL	0.00
5) Phenol-d5	7.65	99	93202	21.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.83	67	70267	23.40	ng/ul	0.00
9) 2-Chlorophenol-d4	8.06	132	66051	22.69	ng/ul	0.00
13) 4-Methylphenol-d8	9.20	113	77165	22.40	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	33609	22.39	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	37573	23.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.94	165	66446	22.05	ng/ul	0.00
29) 4-Chloroaniline-d4	11.46	131	101517	26.61	ng/ul	0.00
43) Dimethylphthalate-d6	14.49	166	268036	22.58	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	309088	22.61	ng/ul	0.00
51) 4-Nitrophenol-d4	15.27	143	44142	19.01	ng/ul	0.00
57) Fluorene-d10	16.09	176	241091	21.65	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.19	200	41892	19.59	ng/ul	0.00
70) Anthracene-d10	17.96	188	390577	24.32	ng/ul	0.00
76) Pyrene-d10	20.22	212	442919	25.06	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.63	264	398752	25.35	ng/ul	0.00

Target Compounds


					Qvalue
6) Phenol	7.69	94	5897	1.277 ng/ul#	87
44) Dimethylphthalate	14.54	163	92040	7.818 ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
Data File : BG027504.D
Acq On : 17 Jun 2017 12:32
Operator : SJ/MA
Sample : I3599-17
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
F5C93

Quant Time: Jun 19 00:59:20 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 19 00:57:08 2017
Response via : Initial Calibration

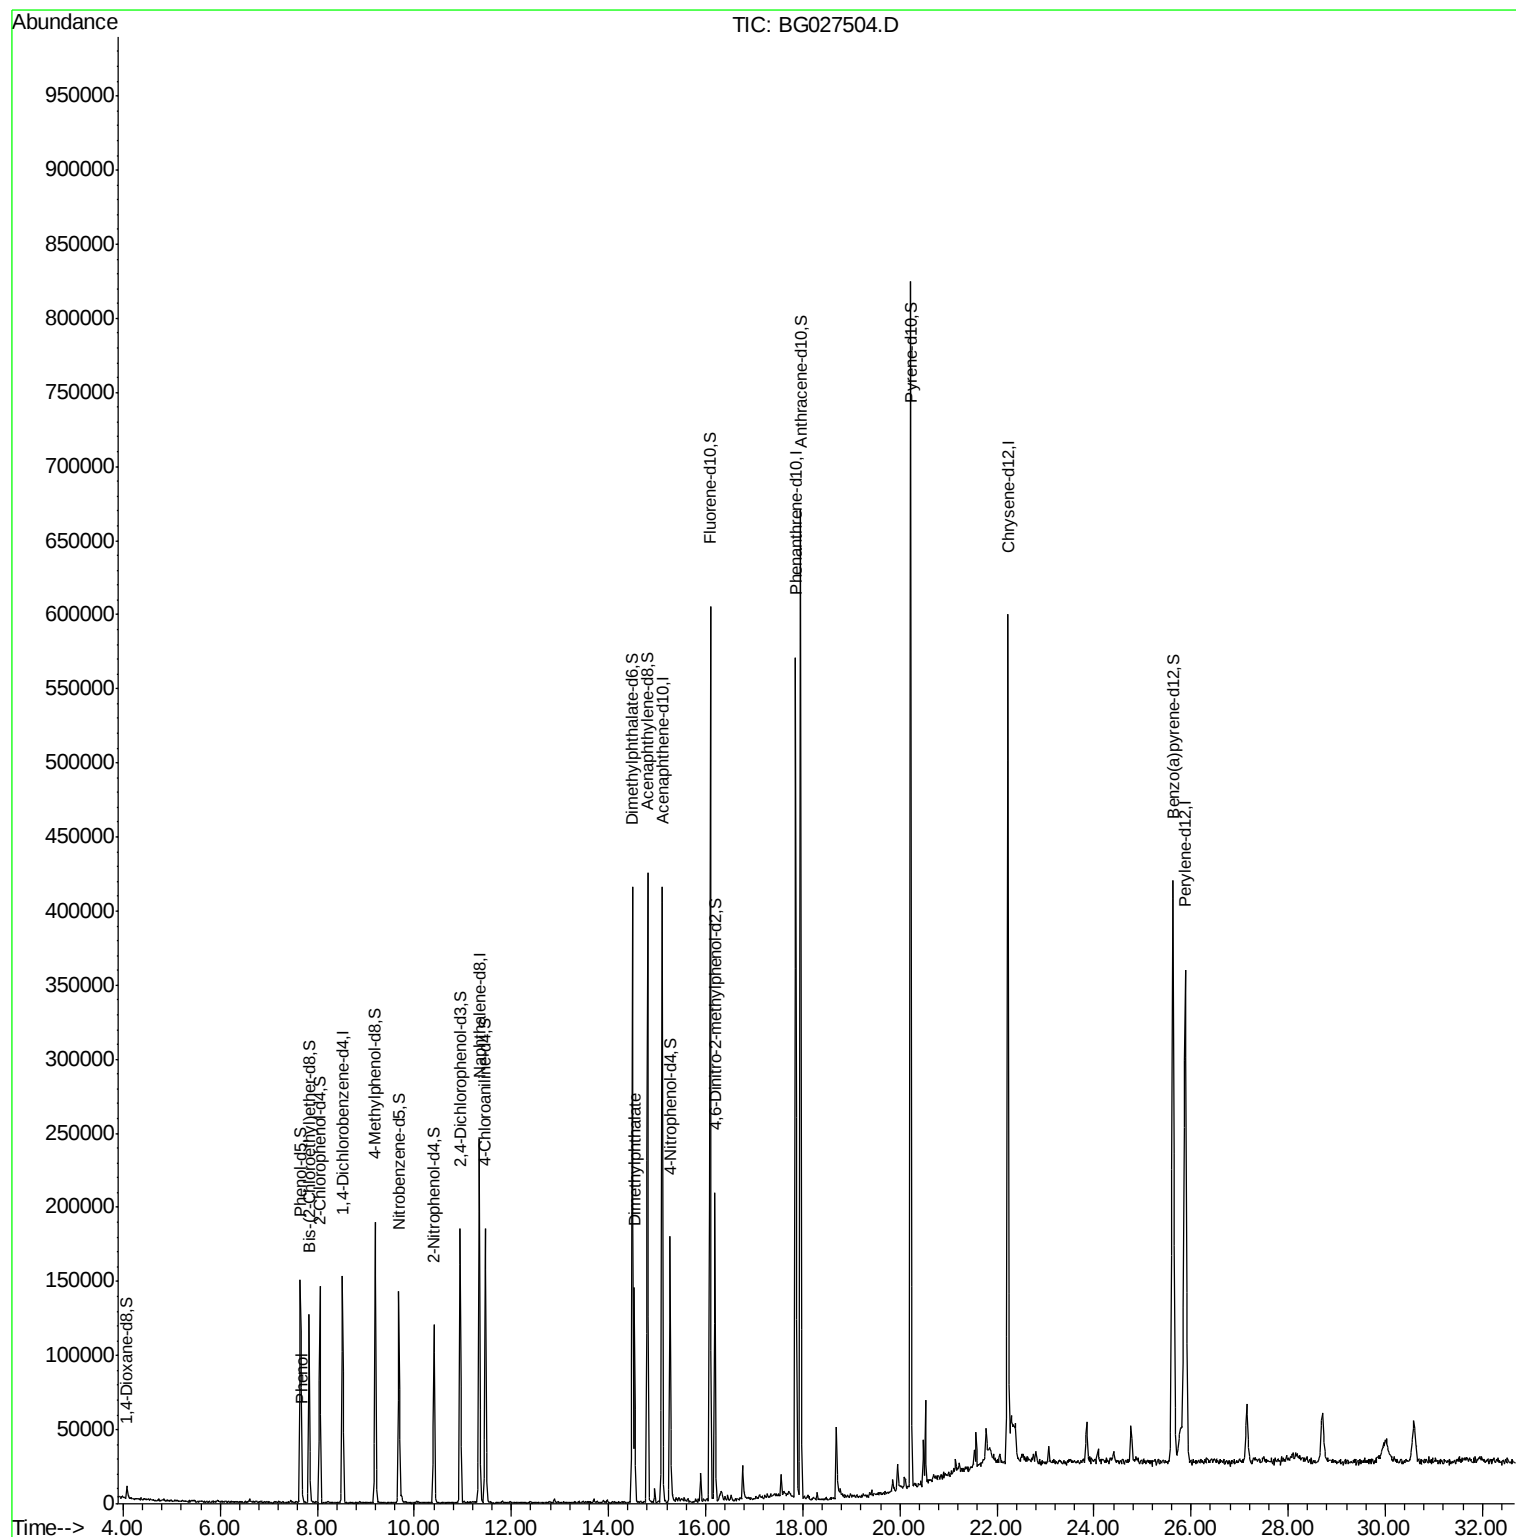

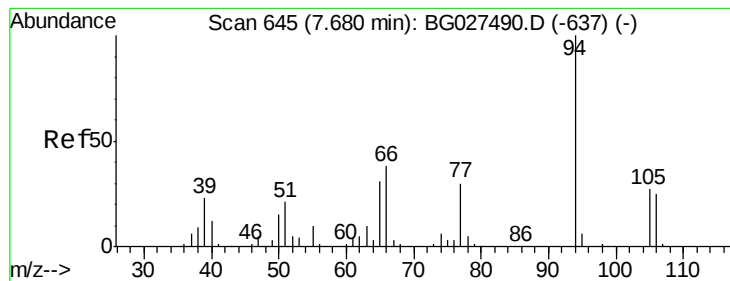

#6

Phenol

Concen: 1.277 ng/ul

RT: 7.69 min Scan# 646

Delta R.T. 0.01 min

Lab File: BG027504.D

Acq: 17 Jun 2017 12:32

Instrument :

BNA_G

ClientSampleId :

F5C93


Tgt Ion: 94 Resp: 5897

Ion Ratio Lower Upper




94 100

65 34.3 26.8 40.2

66 41.1 44.4 66.6#

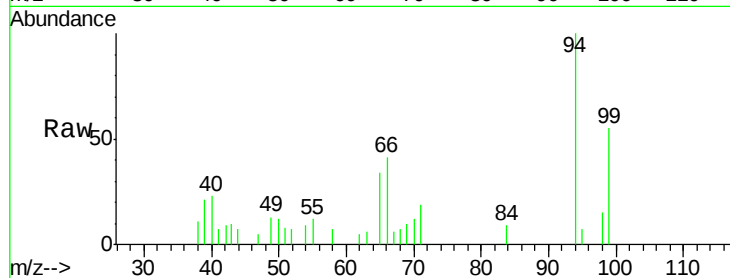

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

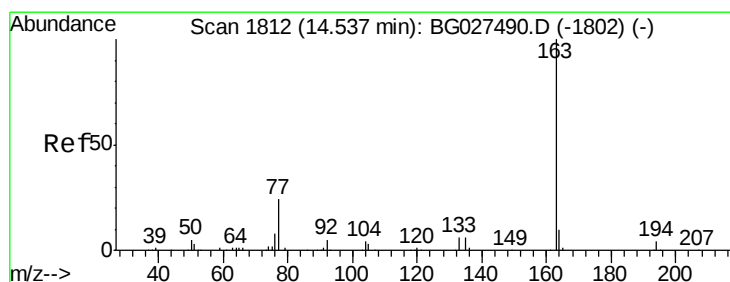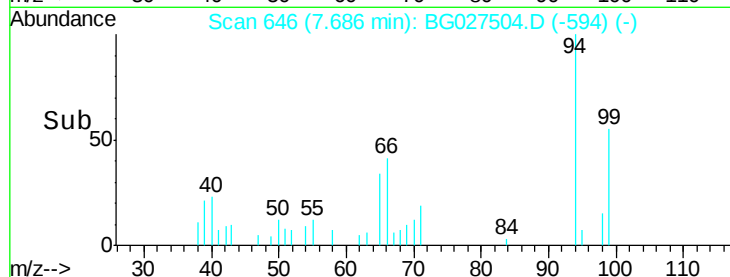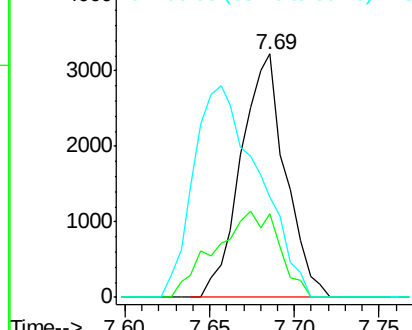

#44

Dimethylphthalate

Concen: 7.818 ng/ul

RT: 14.54 min Scan# 1812

Delta R.T. -0.00 min

Lab File: BG027504.D

Acq: 17 Jun 2017 12:32


Tgt Ion:163 Resp: 92040

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.0

164 9.9 9.0 13.4

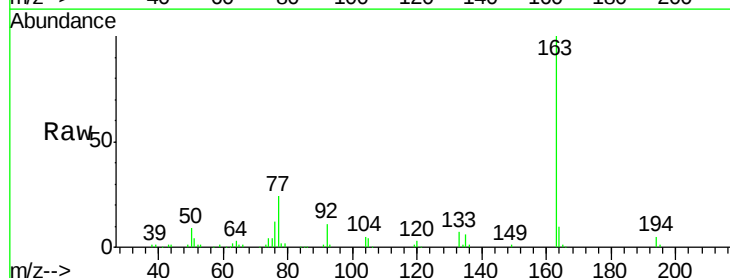

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

