

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
 Data File : BG027486.D
 Acq On : 17 Jun 2017 00:40
 Operator : SJ/MA
 Sample : I3493-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.055	22	28	34	rBV	335039	615283	33.12%	3.403%
2	4.108	34	37	57	rVV	318947	553583	29.80%	3.062%
3	4.237	57	59	66	rVB6	1471	2104	0.11%	0.012%
4	4.789	149	153	158	rBV2	3305	5672	0.31%	0.031%
5	4.836	158	161	164	rVB4	1672	2014	0.11%	0.011%
6	4.883	166	169	178	rVB	8546	14029	0.76%	0.078%
7	5.512	269	276	284	rBV3	2468	6396	0.34%	0.035%
8	5.653	296	300	303	rVB4	1382	2054	0.11%	0.011%
9	5.982	349	356	363	rVB2	13732	23669	1.27%	0.131%
10	6.740	479	485	489	rBV4	1734	2090	0.11%	0.012%
11	7.657	631	641	652	rVB	51925	99628	5.36%	0.551%
12	7.833	662	671	681	rBV	193177	337373	18.16%	1.866%
13	7.921	683	686	691	rVB4	1716	3331	0.18%	0.018%
14	8.050	699	708	719	rBV	178253	337780	18.18%	1.868%
15	8.520	780	788	801	rBV	150214	273344	14.71%	1.512%
16	9.196	895	903	912	rVV	154189	286599	15.43%	1.585%
17	9.284	912	918	925	rVB4	4156	7921	0.43%	0.044%
18	9.425	938	942	953	rBV6	2080	6393	0.34%	0.035%
19	9.684	977	986	1002	rVB	220294	440060	23.69%	2.434%
20	9.825	1006	1010	1015	rVB4	1422	2430	0.13%	0.013%
21	10.406	1100	1109	1118	rBV	191937	361845	19.48%	2.001%
22	10.941	1189	1200	1216	rBV	279358	530449	28.55%	2.934%
23	11.340	1258	1268	1277	rVB	237662	458568	24.69%	2.536%
24	11.470	1285	1290	1302	rVB5	1931	4601	0.25%	0.025%
25	12.069	1385	1392	1401	rBV6	1572	3913	0.21%	0.022%
26	12.886	1526	1531	1540	rBV3	4388	7332	0.39%	0.041%
27	13.144	1573	1575	1585	rVB2	1047	2274	0.12%	0.013%
28	13.461	1622	1629	1636	rVB6	2974	5604	0.30%	0.031%
29	13.520	1636	1639	1643	rBV4	1398	2442	0.13%	0.014%
30	13.697	1664	1669	1673	rBV5	3304	5478	0.29%	0.030%
31	13.732	1673	1675	1683	rVB4	2345	3259	0.18%	0.018%
32	13.908	1704	1705	1712	rBV5	1350	2356	0.13%	0.013%
33	14.073	1730	1733	1739	rVB3	2096	2360	0.13%	0.013%
34	14.372	1777	1784	1788	rBV5	1068	2007	0.11%	0.011%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
 Data File : BG027486.D
 Acq On : 17 Jun 2017 00:40
 Operator : SJ/MA
 Sample : I3493-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

35	14.490	1796	1804	1812	rBV	626763	966670	52.04%	5.346%
36	14.801	1846	1857	1866	rBV	645430	1074857	57.86%	5.945%
37	15.107	1901	1909	1918	rVB2	417312	689165	37.10%	3.811%
38	15.271	1930	1937	1953	rBV	52703	109013	5.87%	0.603%
39	15.577	1985	1989	1995	rBV3	3741	5078	0.27%	0.028%
40	15.776	2022	2023	2030	rVB3	1500	1919	0.10%	0.011%
41	15.865	2030	2038	2048	rBV5	3218	8967	0.48%	0.050%
42	16.041	2060	2068	2070	rBV2	5894	8185	0.44%	0.045%
43	16.094	2070	2077	2085	rVB	906377	1449731	78.04%	8.018%
44	16.194	2085	2094	2106	rVB	324262	512855	27.61%	2.836%
45	16.335	2112	2118	2124	rVB2	8841	13666	0.74%	0.076%
46	16.570	2156	2158	2163	rVB3	1476	2369	0.13%	0.013%
47	16.775	2187	2193	2203	rBV	20413	35397	1.91%	0.196%
48	16.957	2219	2224	2228	rVV5	1761	2648	0.14%	0.015%
49	17.051	2234	2240	2242	rBV3	1736	2849	0.15%	0.016%
50	17.204	2259	2266	2272	rVB5	2626	6007	0.32%	0.033%
51	17.398	2295	2299	2302	rBV6	2001	2497	0.13%	0.014%
52	17.563	2323	2327	2331	rVB5	1748	1999	0.11%	0.011%
53	17.645	2335	2341	2345	rVB3	3001	4045	0.22%	0.022%
54	17.721	2349	2354	2359	rBV8	2877	5728	0.31%	0.032%
55	17.856	2367	2377	2386	rBV	569206	905462	48.74%	5.008%
56	17.956	2386	2394	2407	rVB	1040415	1643823	88.49%	9.091%
57	18.221	2436	2439	2441	rBV3	1451	2053	0.11%	0.011%
58	18.320	2450	2456	2458	rVB4	1953	2715	0.15%	0.015%
59	18.432	2472	2475	2478	rVB3	2151	1937	0.10%	0.011%
60	18.491	2478	2485	2491	rBV6	4672	8688	0.47%	0.048%
61	18.661	2509	2514	2515	rVB4	1841	2790	0.15%	0.015%
62	18.697	2515	2520	2529	rBV5	9730	22543	1.21%	0.125%
63	18.779	2530	2534	2539	rVB4	3339	5346	0.29%	0.030%
64	18.843	2543	2545	2548	rBV4	1646	2054	0.11%	0.011%
65	19.067	2578	2583	2588	rBV5	3627	7078	0.38%	0.039%
66	19.155	2595	2598	2600	rBV4	1833	2642	0.14%	0.015%
67	19.601	2670	2674	2677	rBV6	2233	3215	0.17%	0.018%
68	19.766	2693	2702	2706	rBV8	3918	10763	0.58%	0.060%
69	19.860	2711	2718	2720	rBV2	12127	20210	1.09%	0.112%
70	19.889	2721	2723	2729	rVB2	10806	12548	0.68%	0.069%
71	19.954	2730	2734	2741	rBV7	13533	27124	1.46%	0.150%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
 Data File : BG027486.D
 Acq On : 17 Jun 2017 00:40
 Operator : SJ/MA
 Sample : I3493-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDC60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION

72	20.113	2756	2761	2765	rBV2	11317	16923	0.91%	0.094%
73	20.224	2769	2780	2792	rBV	1227382	1857660	100.00%	10.274%
74	20.424	2810	2814	2817	rBV6	4244	8137	0.44%	0.045%
75	20.536	2832	2833	2837	rBV4	2190	2644	0.14%	0.015%
76	20.577	2837	2840	2842	rVV4	4018	3745	0.20%	0.021%
77	20.735	2865	2867	2872	rBV6	4274	5086	0.27%	0.028%
78	20.841	2881	2885	2891	rVB9	4547	7204	0.39%	0.040%
79	20.894	2893	2894	2899	rBV5	3768	6288	0.34%	0.035%
80	22.228	3112	3121	3130	rBV	518534	1018464	54.83%	5.633%
81	23.074	3261	3265	3271	rVB9	9112	14835	0.80%	0.082%
82	23.861	3393	3399	3406	rVB8	14415	33158	1.78%	0.183%
83	24.784	3547	3556	3561	rBV6	17951	48316	2.60%	0.267%
84	25.635	3688	3701	3717	rVB2	538186	1728412	93.04%	9.559%
85	25.882	3732	3743	3760	rVB2	311124	1072556	57.74%	5.932%
86	27.157	3952	3960	3975	rVB4	26871	89758	4.83%	0.496%
87	28.039	4108	4110	4112	rBV3	3828	3627	0.20%	0.020%
88	28.714	4215	4225	4239	rVB7	25694	103667	5.58%	0.573%
89	30.612	4539	4548	4558	rVB10	15993	57615	3.10%	0.319%
90	32.569	4878	4881	4884	rBV5	3266	4394	0.24%	0.024%


Sum of corrected areas: 18081366

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
Data File : BG027486.D
Acq On : 17 Jun 2017 00:40
Operator : SJ/MA
Sample : I3493-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC60

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

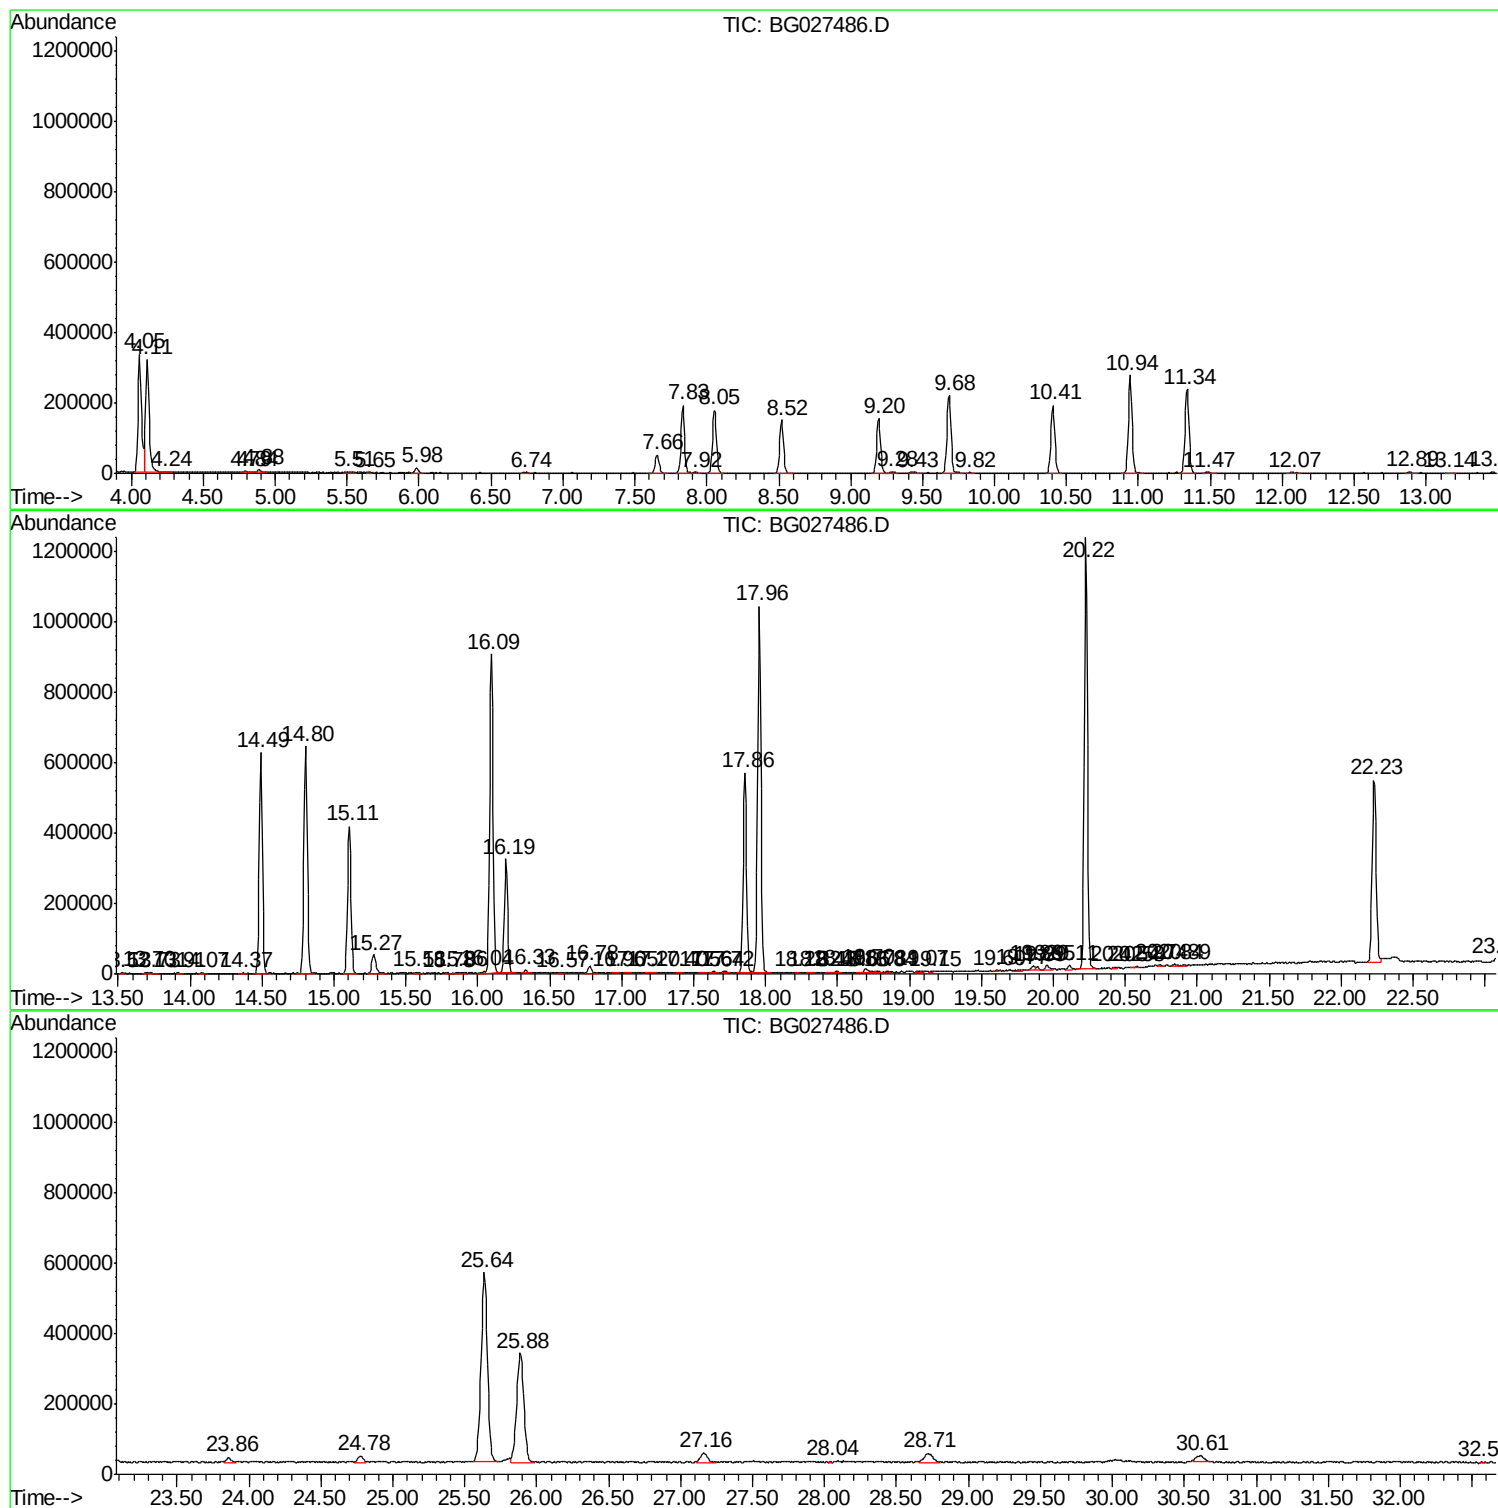

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
Data File : BG027486.D
Acq On : 17 Jun 2017 00:40
Operator : SJ/MA
Sample : I3493-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC60

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
Data File : BG027486.D
Acq On : 17 Jun 2017 00:40
Operator : SJ/MA
Sample : I3493-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDC60

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc