


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061617\
 Data File : BG027466.D
 Acq On : 16 Jun 2017 10:32
 Operator : SJ/MA
 Sample : DFTPP72
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP72

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG061617.M
 Title : SVOA CALIBRATION
 Last Update : Mon Jun 19 01:52:26 2017

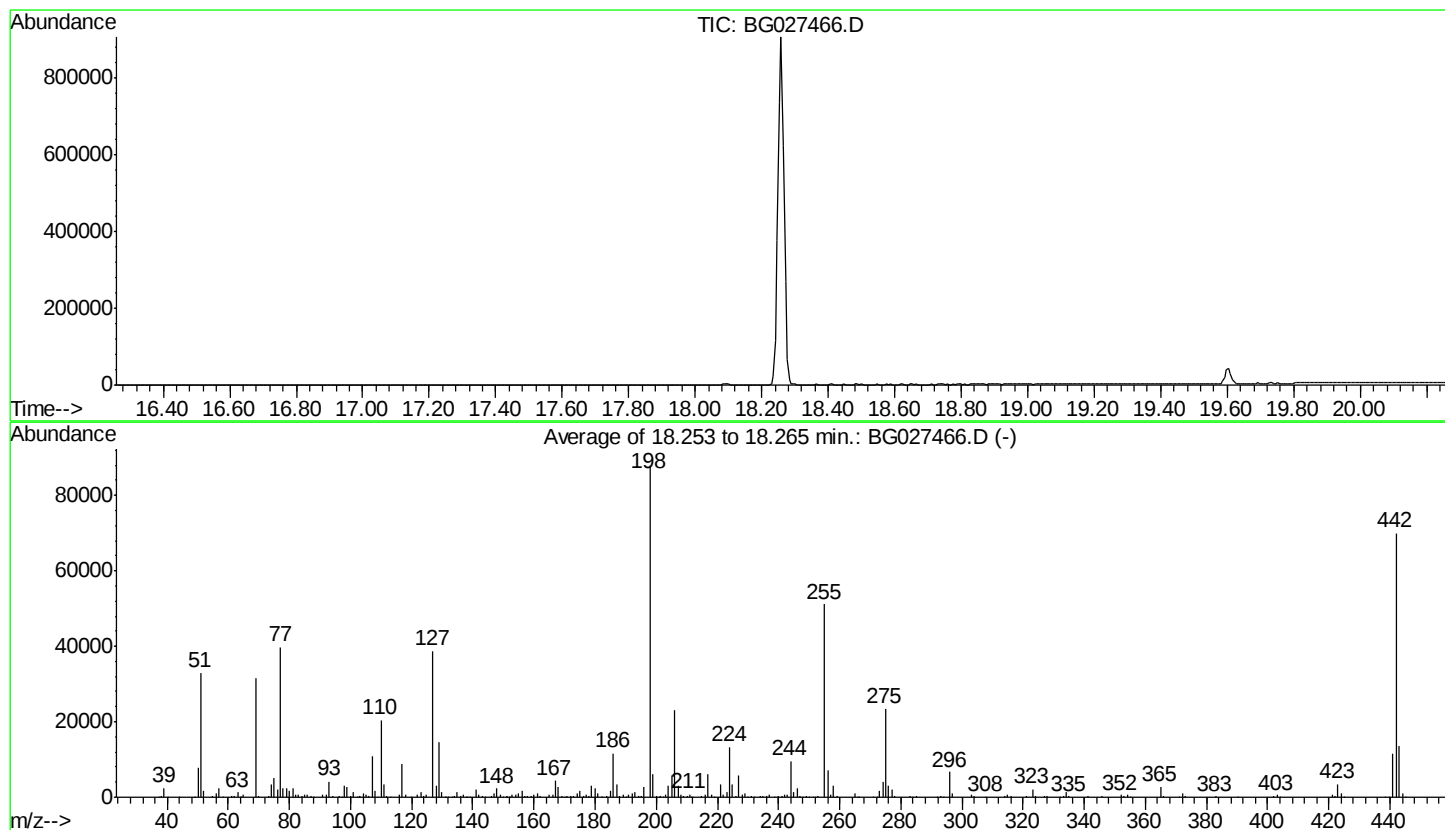

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	32965	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.7	31394	PASS
70	69	0.00	2	0.6	187	PASS
127	198	10	80	44.1	38720	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87869	PASS
199	198	5	9	7.0	6109	PASS
275	198	10	60	26.8	23544	PASS
365	198	1	100	3.3	2868	PASS
441	442	0.01	100	16.7	11654	PASS
442	198	50	100	79.6	69973	PASS
443	442	15	24	19.6	13738	PASS

m/z	Abundance
38.00	610.0
39.00	2757.0
39.90	223.0
44.00	557.0
50.00	9291.0
51.00	37720.0
52.00	2149.0
54.90	195.0
56.00	1054.0
57.00	2618.0
58.10	198.0
61.00	591.0
61.90	567.0
63.00	1610.0
63.80	204.0
65.00	748.0
68.90	35040.0
69.90	329.0
73.00	393.0
74.00	3695.0
75.00	6215.0
76.10	2349.0
77.00	44728.0
78.00	2511.0
79.00	2803.0
80.00	2161.0
81.00	2696.0
82.00	733.0
83.00	776.0
83.90	186.0
84.90	493.0
86.00	760.0
87.00	290.0
90.90	668.0
91.90	813.0
93.00	4508.0
94.00	363.0
96.00	202.0
97.90	3425.0
98.90	3059.0
100.00	382.0
100.90	1459.0
102.00	166.0
102.80	507.0
104.00	1081.0
104.90	830.0
106.00	341.0
107.00	10603.0
108.00	1725.0
110.00	21976.0
111.00	3741.0
111.90	449.0
116.10	753.0
116.90	9182.0
118.00	841.0
121.90	781.0
123.00	1249.0
123.90	634.0
124.90	558.0
127.00	40600.0
128.00	3401.0
129.00	15188.0
129.90	1305.0
130.80	280.0
134.00	469.0
134.90	1408.0
136.00	562.0
137.00	763.0
140.90	2257.0
141.90	482.0
143.00	448.0
143.90	159.0
146.00	408.0
146.90	1389.0
147.90	2408.0
149.00	550.0
149.90	198.0
150.90	217.0
152.90	731.0
153.90	539.0
155.00	1035.0
156.00	1835.0
157.00	374.0
158.00	350.0
158.90	339.0
159.80	484.0
161.00	1044.0
161.90	288.0
164.90	1041.0
166.00	644.0
167.00	4582.0

Instrument :
BNA_G
ClientSampleId :
DFTPP72

167.90	2849.0
168.90	410.0
171.00	180.0
171.90	476.0
172.90	381.0
174.00	721.0
175.00	1808.0
176.10	360.0
177.00	1000.0
178.00	320.0
178.90	3076.0
180.00	2311.0
180.90	861.0
182.00	156.0
183.90	504.0
185.00	1811.0
186.00	11628.0
187.00	3413.0
188.00	489.0
189.00	1012.0
190.90	591.0
192.00	853.0
192.90	1109.0
194.00	266.0
195.00	197.0
196.00	2122.0
197.90	84632.0
198.90	5883.0
200.00	482.0
200.90	165.0
201.50	243.0
202.10	213.0
202.90	671.0
204.00	3032.0
205.00	5858.0
206.00	21992.0
207.00	3622.0
207.90	790.0
208.90	448.0
210.10	359.0
211.00	697.0
211.90	185.0
214.90	226.0
216.00	644.0
216.90	6096.0
218.00	873.0
219.00	173.0
221.00	3510.0
221.90	1108.0
223.00	1619.0
224.00	12745.0
225.00	2970.0
226.00	354.0
226.90	5503.0
228.00	794.0
228.90	901.0
230.00	163.0
231.00	399.0
233.90	369.0
234.90	326.0
236.00	215.0
236.90	672.0
238.90	206.0
240.00	329.0
241.00	305.0
242.00	562.0
243.10	826.0
244.00	8660.0
245.00	978.0
245.90	2035.0
246.90	417.0
248.00	160.0
249.00	333.0
251.90	152.0
252.90	295.0
255.00	46360.0
256.00	6815.0
257.00	727.0
258.00	3032.0
258.90	460.0
265.00	1347.0
266.00	221.0
271.90	181.0
272.90	1215.0
274.00	3611.0
275.00	21888.0
276.00	2929.0
277.00	1866.0
278.00	407.0
283.10	204.0
283.90	158.0
285.00	531.0
293.00	495.0
293.90	210.0
296.00	6049.0

Instrument :
BNA_G
ClientSampleId :
DFTPP72

297.00	900.0
303.00	585.0
303.90	167.0
314.00	278.0
314.90	569.0
316.00	418.0
320.90	278.0
323.00	1761.0
324.10	205.0
326.90	505.0
327.90	203.0
333.20	176.0
334.00	1059.0
334.90	262.0
341.00	230.0
345.90	374.0
352.00	673.0
352.90	442.0
354.00	515.0
364.90	2296.0
365.90	225.0
370.90	154.0
372.00	774.0
373.00	300.0
383.00	167.0
401.90	340.0
403.00	497.0
421.00	608.0
422.00	359.0
423.00	2912.0
424.00	907.0
439.40	164.0
441.00	8820.0
442.00	52576.0
443.00	9758.0
444.00	1048.0

Instrument :
BNA_G
ClientSampleId :
DFTPP72

m/z	Abundance
37.00	200.0
38.00	305.0
39.00	2694.0
40.00	239.0
44.00	524.0
49.00	484.0
50.00	9095.0
51.00	38248.0
52.00	1907.0
55.00	226.0
56.00	1105.0
57.00	2608.0
58.00	186.0
60.90	636.0
62.00	688.0
63.00	1528.0
64.00	289.0
65.00	914.0
69.00	36768.0
73.10	347.0
74.00	3953.0
75.00	6095.0
76.00	2052.0
77.00	45448.0
78.00	3042.0
79.00	2721.0
80.00	2017.0
81.00	2939.0
81.90	752.0
83.00	811.0
84.00	287.0
85.00	944.0
85.90	1036.0
87.00	519.0
87.90	261.0
91.00	771.0
92.00	717.0
93.00	4957.0
94.00	315.0
96.10	194.0
97.00	184.0
98.00	3739.0
99.00	3411.0
99.90	236.0
100.90	1787.0
101.90	151.0
103.00	764.0
104.00	790.0
104.90	1094.0
107.00	13899.0
108.00	1863.0
110.00	23376.0
111.00	4180.0
111.80	444.0
112.90	257.0
116.10	821.0
117.00	10834.0
117.90	783.0
119.80	164.0
121.90	936.0
123.00	1418.0
123.90	575.0
124.90	806.0
127.00	45680.0
128.00	3520.0
128.90	17616.0
130.00	1498.0
131.00	312.0
132.90	215.0
133.90	458.0
135.00	1534.0
136.00	532.0
137.00	947.0
138.10	163.0
138.90	152.0
141.00	2300.0
142.00	849.0
143.00	599.0
144.00	167.0
146.00	588.0
146.90	1333.0
147.90	2719.0
149.00	791.0
151.00	448.0
151.80	283.0
152.90	916.0
153.90	766.0
155.00	1425.0
156.00	1934.0
156.90	373.0
157.90	654.0

Instrument :
BNA_G
ClientSampleId :
DFTPP72

158.90	402.0
159.90	811.0
161.00	1222.0
162.00	312.0
165.00	794.0
166.00	946.0
167.00	5365.0
168.00	2933.0
168.90	423.0
170.90	383.0
171.90	333.0
172.90	597.0
174.00	1252.0
175.00	2007.0
176.00	414.0
177.00	863.0
178.00	204.0
178.90	4028.0
180.00	2696.0
180.90	1164.0
182.20	256.0
183.90	451.0
185.00	2028.0
186.00	14481.0
187.00	4531.0
188.00	487.0
189.00	991.0
190.00	171.0
190.90	746.0
192.00	1313.0
193.00	1527.0
194.10	286.0
194.90	168.0
196.00	3371.0
197.90	107784.0
198.90	7759.0
200.00	583.0
201.50	629.0
202.10	194.0
202.90	773.0
204.00	3334.0
205.00	6780.0
206.00	27944.0
207.00	4676.0
208.00	910.0
208.90	397.0
210.00	664.0
211.00	1007.0
211.60	328.0
214.90	253.0
216.10	747.0
216.90	7302.0
218.00	977.0
221.00	3883.0
222.00	947.0
223.00	1843.0
224.00	15935.0
225.00	4030.0
226.10	649.0
226.90	7244.0
227.90	1000.0
228.90	1312.0
231.00	583.0
233.90	298.0
234.90	476.0
235.90	251.0
237.00	733.0
238.70	203.0
240.00	197.0
241.00	363.0
241.90	769.0
243.00	904.0
244.00	11934.0
245.00	1902.0
246.00	2845.0
246.90	380.0
248.90	443.0
249.80	154.0
251.00	203.0
251.80	157.0
252.90	346.0
255.00	62632.0
256.00	8873.0
256.90	759.0
258.00	3875.0
259.00	661.0
264.90	1265.0
266.00	187.0
272.00	238.0
273.00	2158.0
274.00	5003.0
275.00	28096.0
276.00	3242.0
277.00	2479.0
278.00	410.0

Instrument :
BNA_G
ClientSampleId :
DFTPP72

282.90	298.0
284.00	312.0
285.00	581.0
291.90	150.0
292.90	546.0
296.00	8059.0
297.00	1053.0
303.00	1010.0
304.00	288.0
307.90	152.0
313.90	373.0
315.00	752.0
315.90	488.0
321.00	276.0
323.00	2399.0
324.10	378.0
326.90	392.0
327.90	239.0
332.00	325.0
333.00	283.0
334.00	1847.0
335.00	438.0
341.00	314.0
345.80	577.0
352.00	677.0
352.90	342.0
354.00	706.0
355.00	319.0
365.00	3584.0
366.00	448.0
372.00	1475.0
372.90	172.0
382.90	279.0
402.00	493.0
403.00	833.0
404.00	292.0
421.00	657.0
422.00	725.0
423.00	4271.0
424.10	1014.0
424.80	225.0
438.20	152.0
439.50	172.0
441.00	13788.0
442.00	84272.0
443.00	17160.0
444.00	1294.0
444.90	150.0

Instrument :
BNA_G
ClientSampleId :
DFTPP72

m/z	Abundance
38.00	308.0
39.00	1921.0
44.00	639.0
49.00	412.0
50.00	5560.0
51.00	22928.0
52.00	1118.0
55.00	198.0
55.90	719.0
57.00	1536.0
60.80	330.0
61.90	238.0
63.00	876.0
65.10	437.0
69.00	22376.0
69.90	234.0
73.00	346.0
74.00	2434.0
75.00	3336.0
76.00	1505.0
77.00	29256.0
78.00	1972.0
79.00	1961.0
79.90	1123.0
81.00	1945.0
81.90	655.0
83.00	472.0
83.80	151.0
85.00	621.0
85.90	555.0
87.00	337.0
91.00	608.0
92.00	457.0
92.90	2884.0
93.90	288.0
96.00	376.0
97.90	2314.0
99.00	1719.0
100.10	186.0
101.00	1017.0
103.00	310.0
104.00	750.0
104.90	625.0
105.90	231.0
107.00	8074.0
108.00	1384.0
109.00	329.0
110.00	16099.0
111.00	2048.0
111.90	209.0
116.00	667.0
117.00	6414.0
117.90	482.0
122.00	720.0
123.00	947.0
123.90	265.0
125.00	367.0
127.00	29880.0
127.90	2391.0
129.00	11311.0
129.90	936.0
131.00	186.0
131.90	184.0
133.90	312.0
134.90	1133.0
135.90	361.0
137.00	464.0
137.60	211.0
140.90	1702.0
141.90	584.0
142.90	402.0
143.90	165.0
146.00	368.0
147.00	872.0
147.90	1675.0
148.90	647.0
151.00	179.0
151.30	164.0
152.00	214.0
152.90	543.0
153.90	325.0
155.00	904.0
156.00	1466.0
157.00	367.0
157.90	382.0
158.90	251.0
160.00	486.0
160.90	690.0
162.00	165.0
164.90	637.0
166.00	383.0

Instrument :
BNA_G
ClientSampleId :
DFTPP72

167.00	3138.0
168.00	2103.0
168.90	300.0
170.00	170.0
171.90	307.0
172.90	421.0
174.00	645.0
175.00	1082.0
176.00	335.0
177.00	658.0
177.90	280.0
178.90	2567.0
180.00	1809.0
181.00	730.0
183.90	281.0
185.00	1163.0
186.00	9035.0
187.00	2556.0
187.90	358.0
189.00	572.0
191.00	353.0
192.00	915.0
193.00	1207.0
194.00	304.0
194.90	210.0
196.00	2464.0
197.90	71192.0
198.90	4687.0
199.90	456.0
201.40	345.0
202.90	525.0
204.00	2504.0
205.00	4877.0
206.00	19512.0
207.00	2770.0
208.00	736.0
209.00	293.0
209.90	372.0
210.90	745.0
214.90	293.0
215.90	423.0
216.90	5362.0
218.00	717.0
221.00	2727.0
222.90	1109.0
224.00	11060.0
225.00	2910.0
225.90	397.0
227.00	4995.0
228.00	684.0
228.80	1063.0
231.00	344.0
231.90	172.0
233.90	347.0
234.90	318.0
235.90	328.0
237.00	507.0
240.00	234.0
241.00	227.0
242.00	631.0
242.90	576.0
244.00	8042.0
245.00	1081.0
245.90	1866.0
247.00	355.0
248.90	318.0
251.00	186.0
252.80	267.0
255.00	44416.0
256.00	6039.0
257.00	538.0
258.00	2738.0
258.90	385.0
265.00	925.0
266.20	235.0
270.90	167.0
273.00	1419.0
274.00	3946.0
275.00	20648.0
276.00	3205.0
277.00	1918.0
278.00	230.0
283.00	207.0
285.10	214.0
291.90	156.0
293.00	312.0
296.00	6169.0
296.90	1001.0
303.00	646.0
304.00	154.0
314.00	414.0
315.00	510.0
315.80	386.0
320.90	228.0
323.00	2168.0

Instrument :
BNA_G
ClientSampleId :
DFTPP72

324.00	245.0
326.90	421.0
327.90	156.0
332.90	196.0
334.00	1422.0
335.00	277.0
341.00	252.0
346.00	418.0
351.90	483.0
352.90	380.0
354.00	571.0
365.00	2725.0
366.00	340.0
372.00	1180.0
373.00	247.0
382.90	242.0
390.00	172.0
401.90	512.0
403.00	663.0
421.00	525.0
422.00	475.0
423.00	3336.0
424.00	1003.0
424.90	158.0
439.40	158.0
441.00	12355.0
442.00	73072.0
443.00	14296.0
444.00	1219.0

Instrument :
BNA_G
ClientSampleId :
DFTPP72

Scan 2472 (18.212 min): BG027466.D
DFTPP72

m/z	Abundance
43.90	412.0
48.80	157.0
85.90	196.0
207.00	536.0
207.90	154.0

Instrument :
BNA_G
ClientSampleId :
DFTPP72