
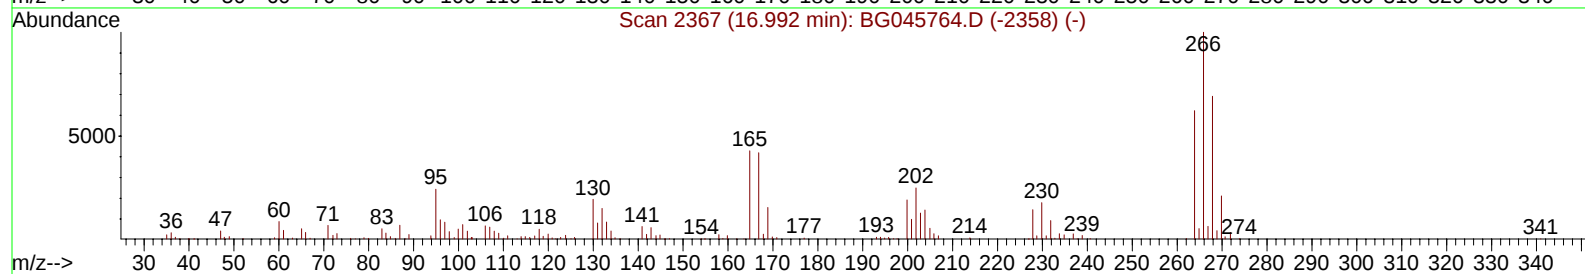
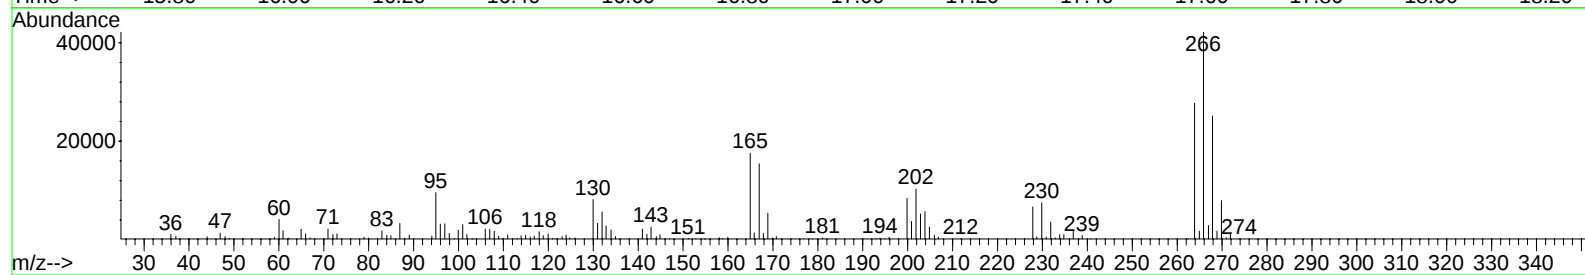


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061620\
 Data File : BG045770.D
 Acq On : 16 Jun 2020 9:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 17:37:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 18:34:19 2020
 Response via : Initial Calibration

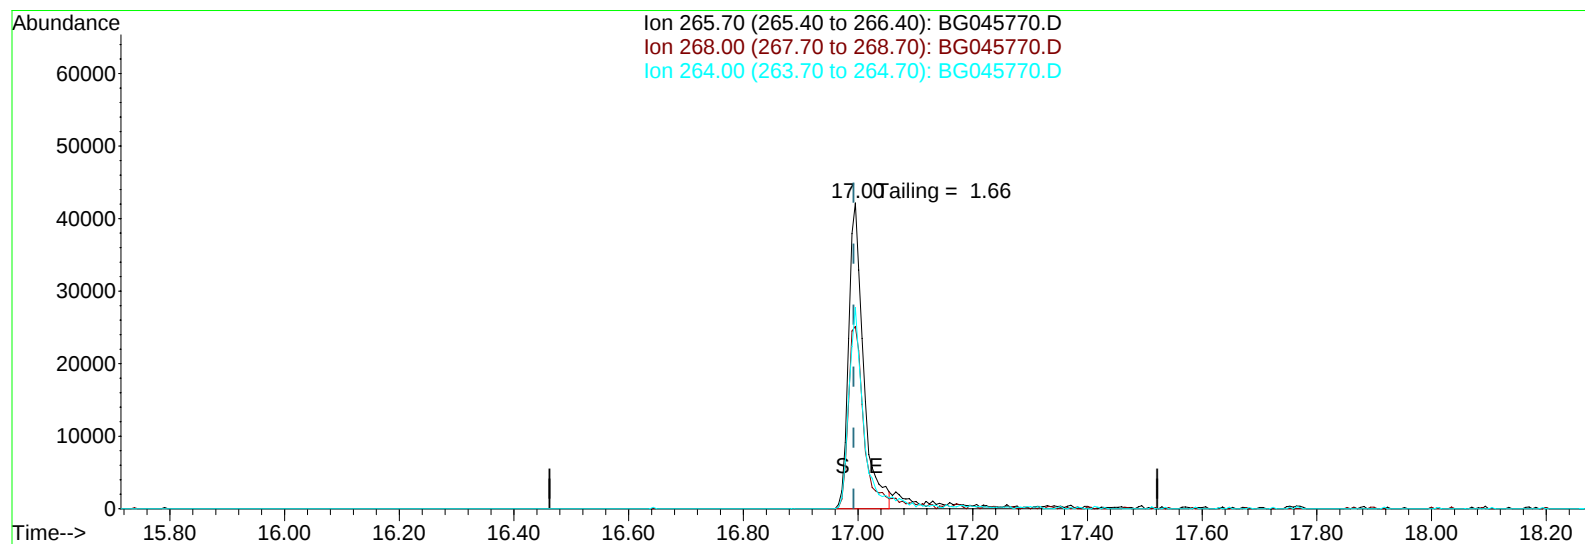

TIC: BG045770.D

(70) Pentachlorophenol (C)




16.995min (+0.003) 164319.72ng

response 80869

Ion	Exp%	Act%
265.70	100	100
268.00	69.20	59.65
264.00	62.20	65.76
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061620\
 Data File : BG045770.D
 Acq On : 16 Jun 2020 9:57
 Operator : CG/JU
 Sample : DF TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 17:37:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 18:34:19 2020
 Response via : Initial Calibration

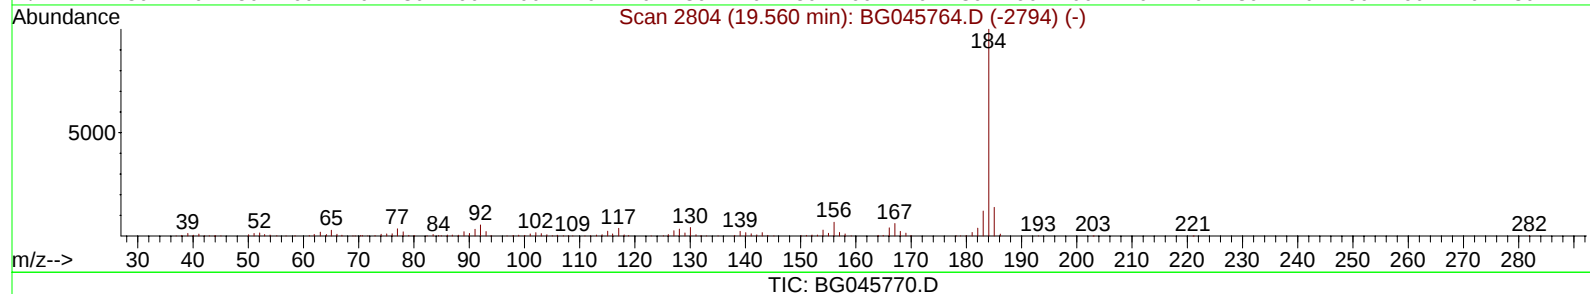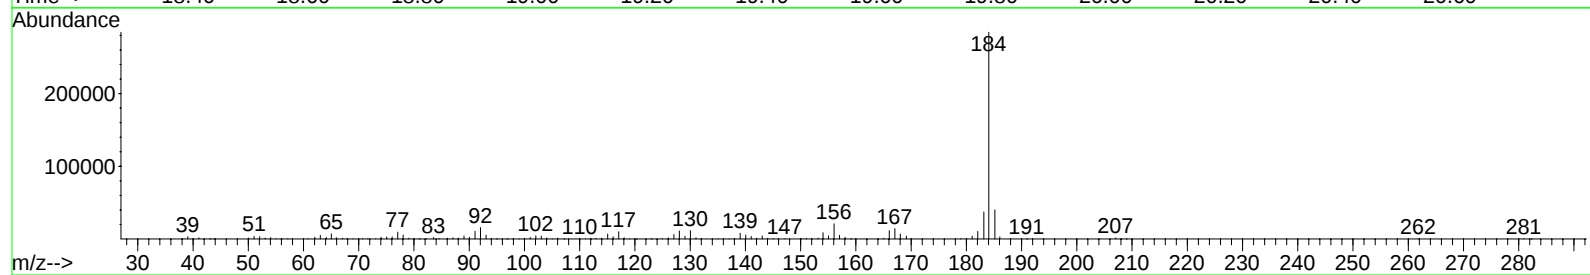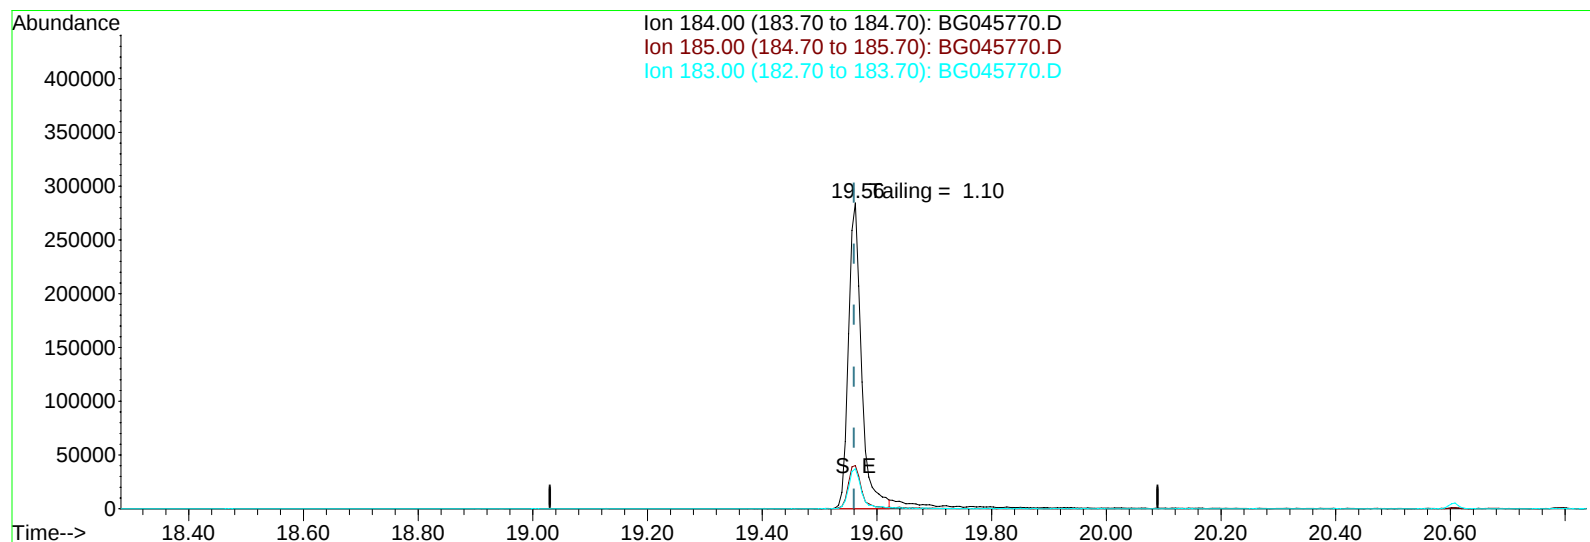

(77) Benzidine

19.562min (+0.003) 78237.78ng

response 473910

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.15
183.00	12.10	13.10
0.00	0.00	0.00