
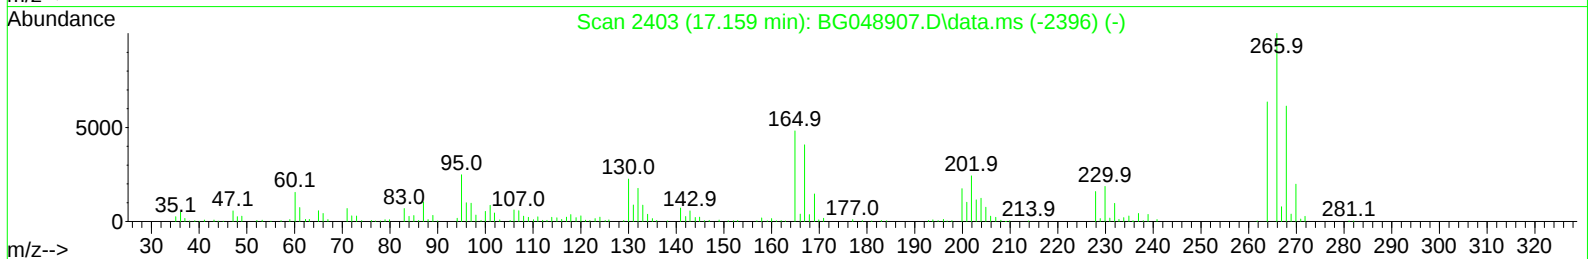
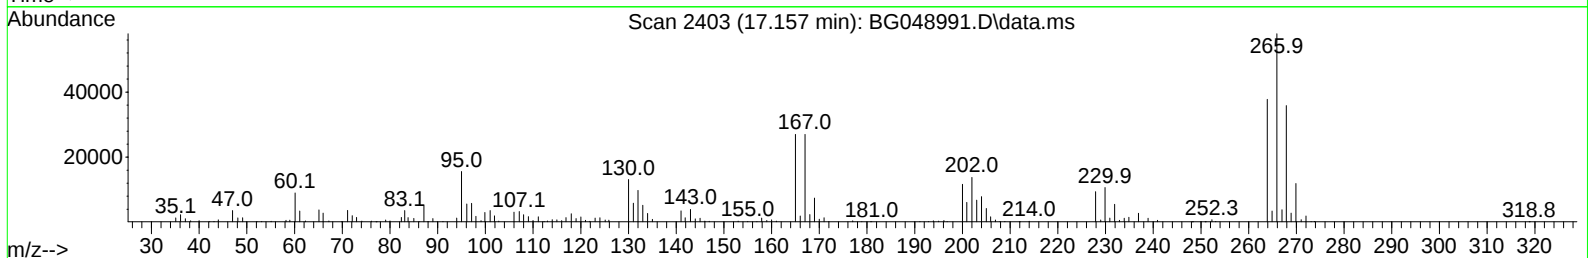


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061621\
Data File : BG048991.D
Acq On : 16 Jun 2021 9:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 12:01:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

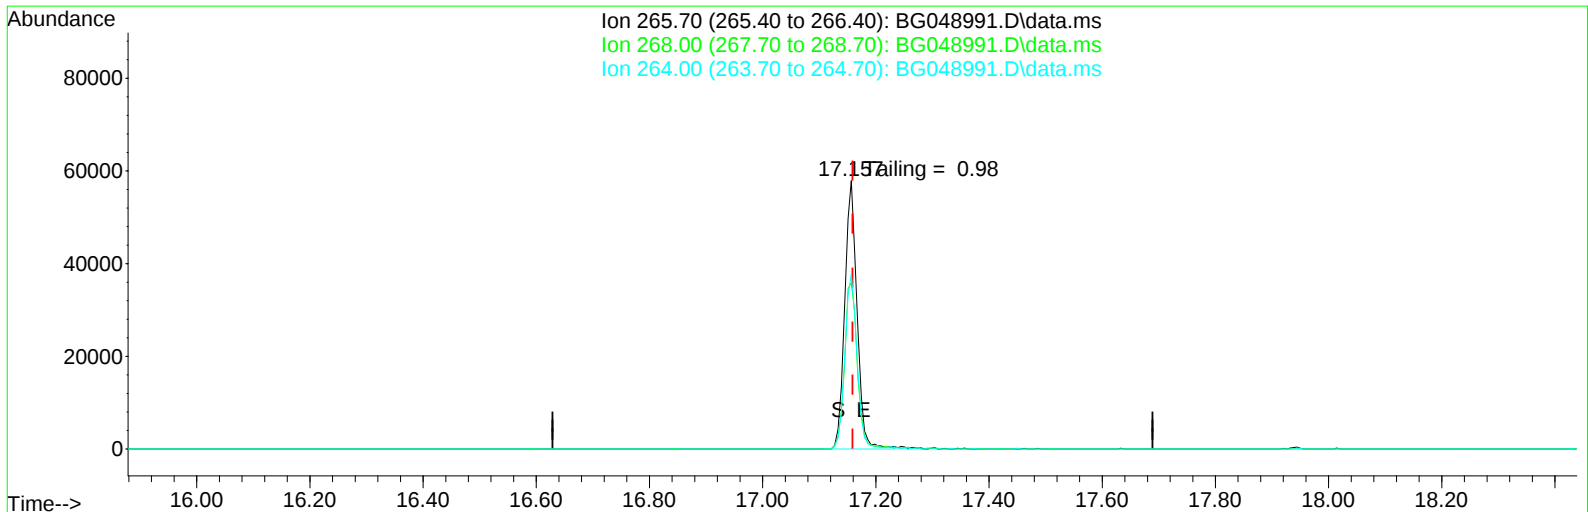

TIC: BG048991.D\data.ms

(70) Pentachlorophenol (C)




17.157min (-0.002) 177584.10 ng

response 86659

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.89
264.00	61.30	65.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061621\
Data File : BG048991.D
Acq On : 16 Jun 2021 9:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 12:01:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

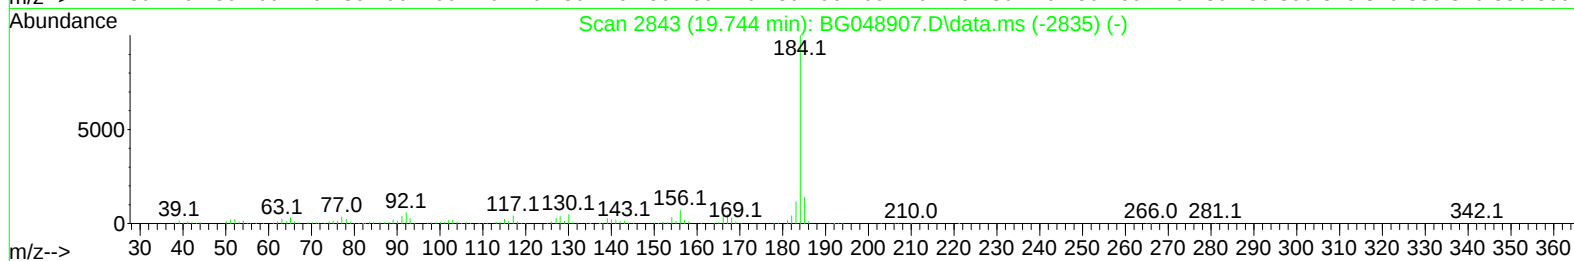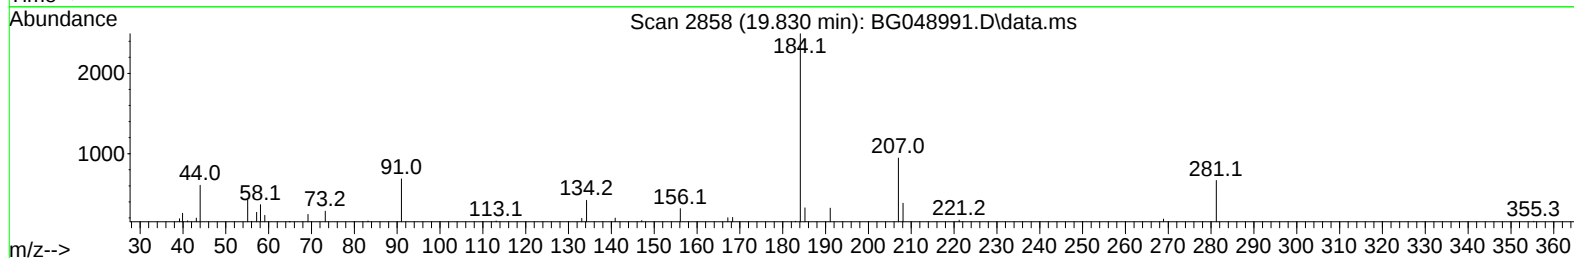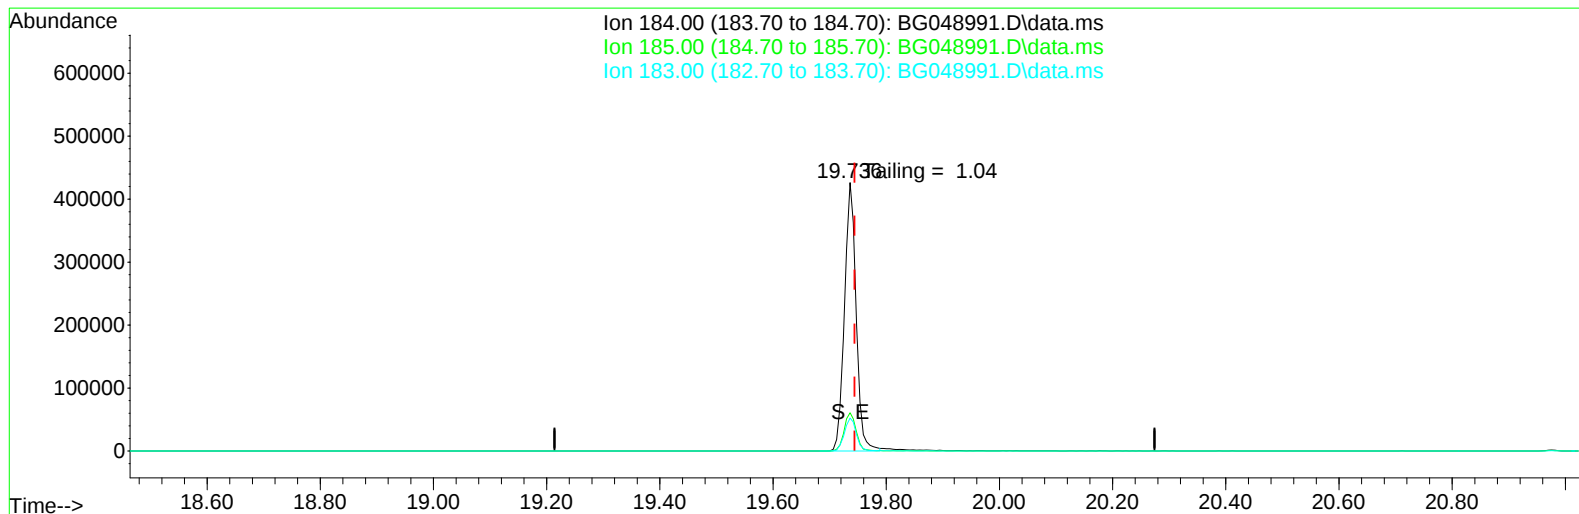

TIC: BG048991.D\data.ms

(77) Benzidine

19.736min (-0.008) 471572.23 ng

response 617487

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.25
183.00	11.70	12.32
0.00	0.00	0.00