
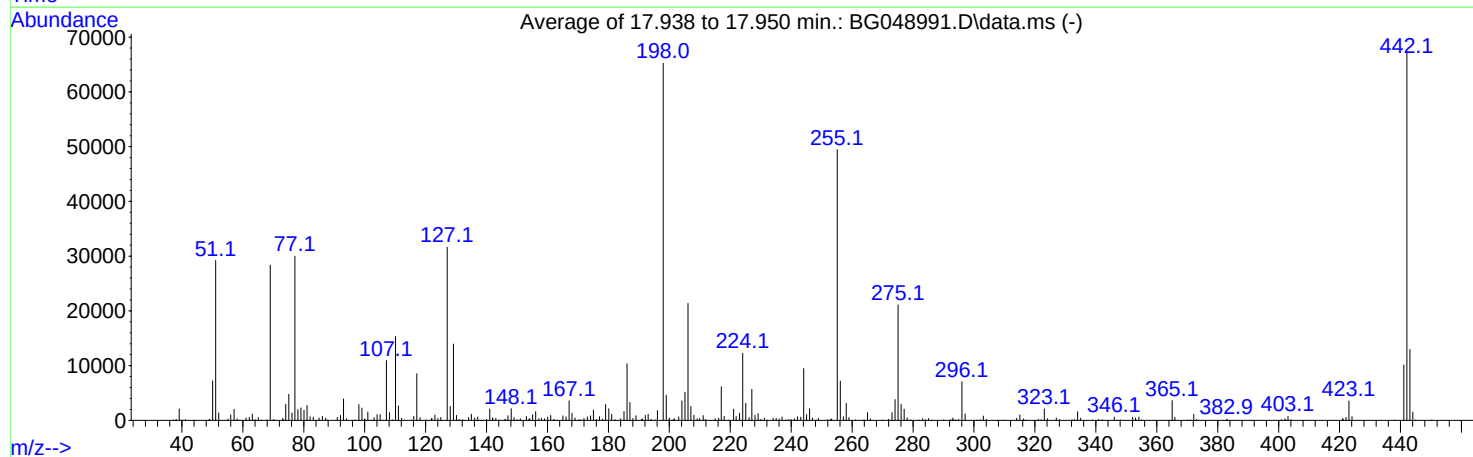


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061621\
 Data File : BG048991.D
 Acq On : 16 Jun 2021 9:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 16 12:04:50 2021

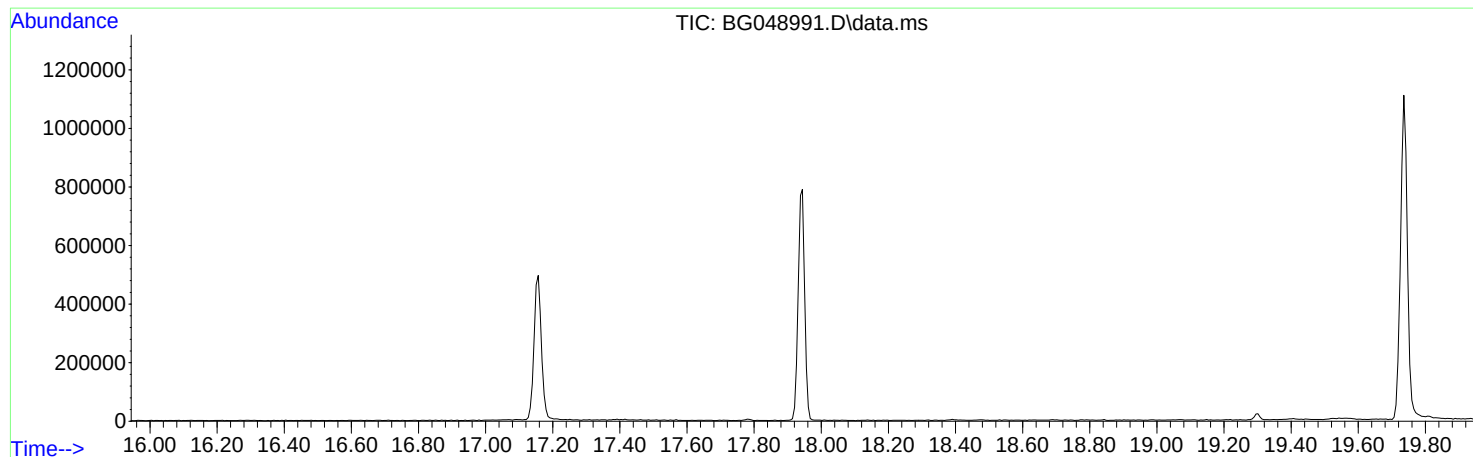




AutoFind: Scans 2536, 2537, 2538; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.8	29205	PASS
68	69	0.00	2	0.4	115	PASS
69	198	0.00	100	43.4	28345	PASS
70	69	0.00	2	0.4	125	PASS
127	198	10	80	48.5	31643	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65245	PASS
199	198	5	9	7.0	4595	PASS
275	198	10	60	32.3	21105	PASS
365	198	1	100	5.6	3633	PASS
441	198	0.01	100	15.5	10123	PASS
442	442	100	100	100.0	67197	PASS
443	442	15	24	19.3	12938	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061621\
Data File : BG048991.D
Acq On : 16 Jun 2021 9:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 16 12:01:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

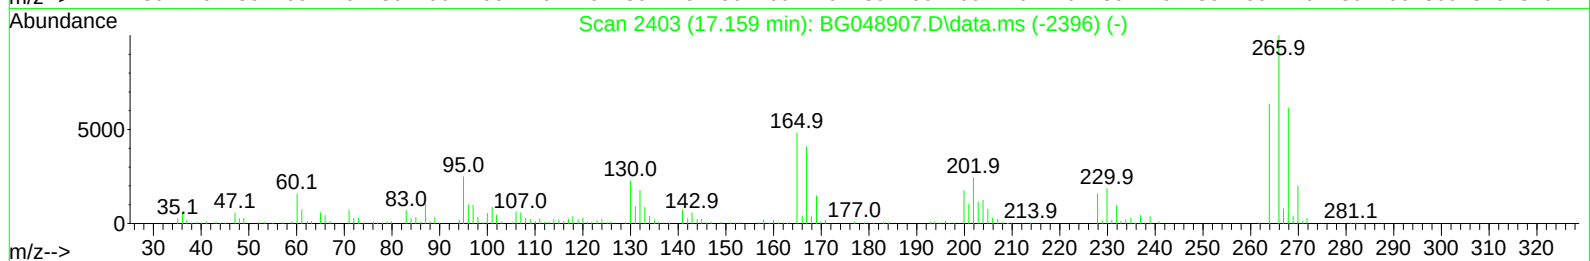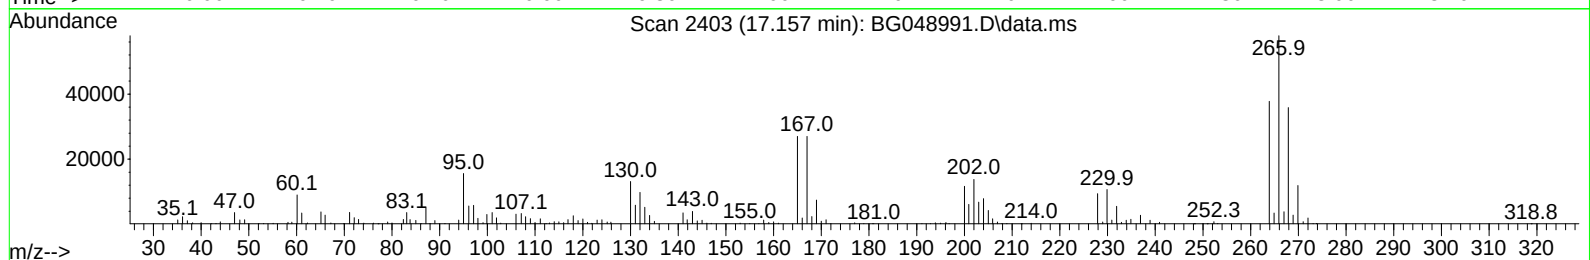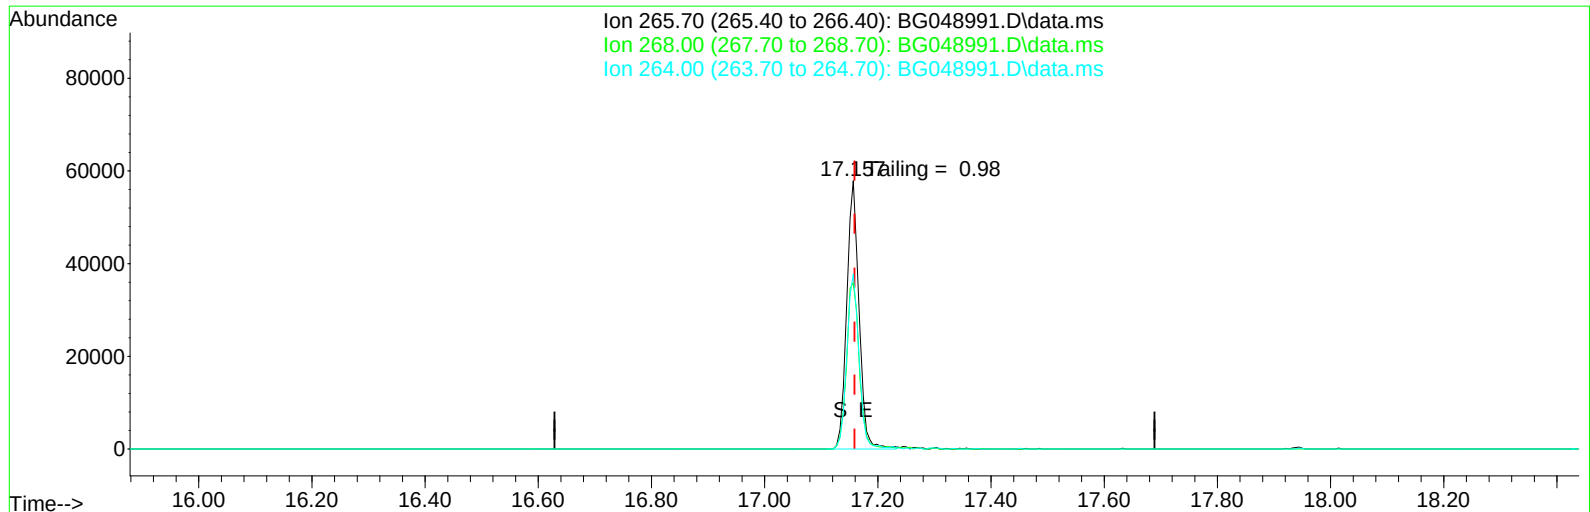

TIC: BG048991.D\data.ms

(70) Pentachlorophenol (C)

17.157min (-0.002) 177584.10 ng




response 86659

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.89
264.00	61.30	65.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061621\
Data File : BG048991.D
Acq On : 16 Jun 2021 9:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 16 12:01:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 11 16:03:10 2021
Response via : Initial Calibration

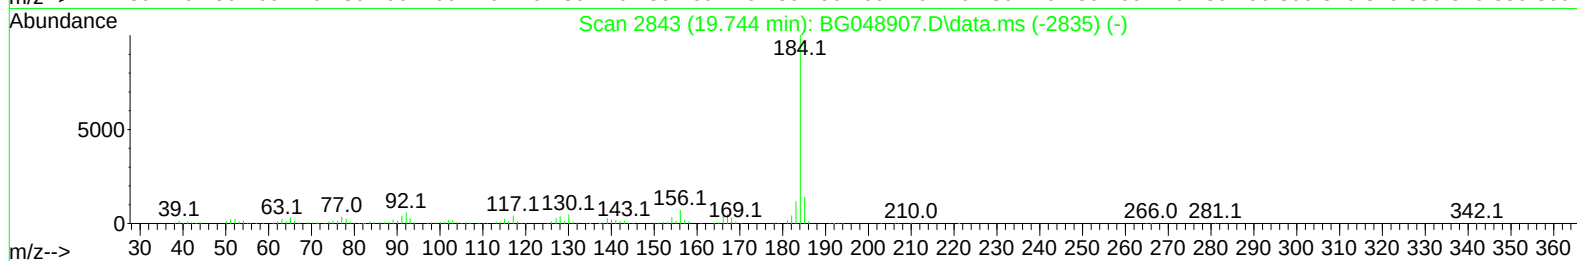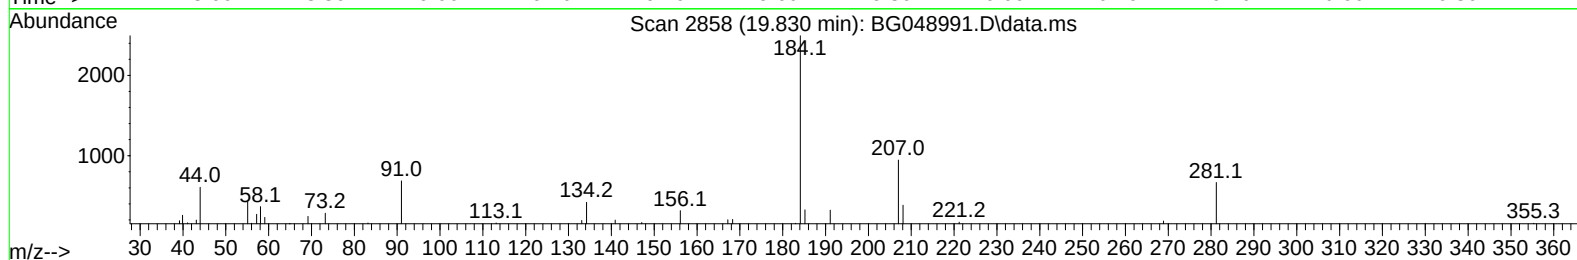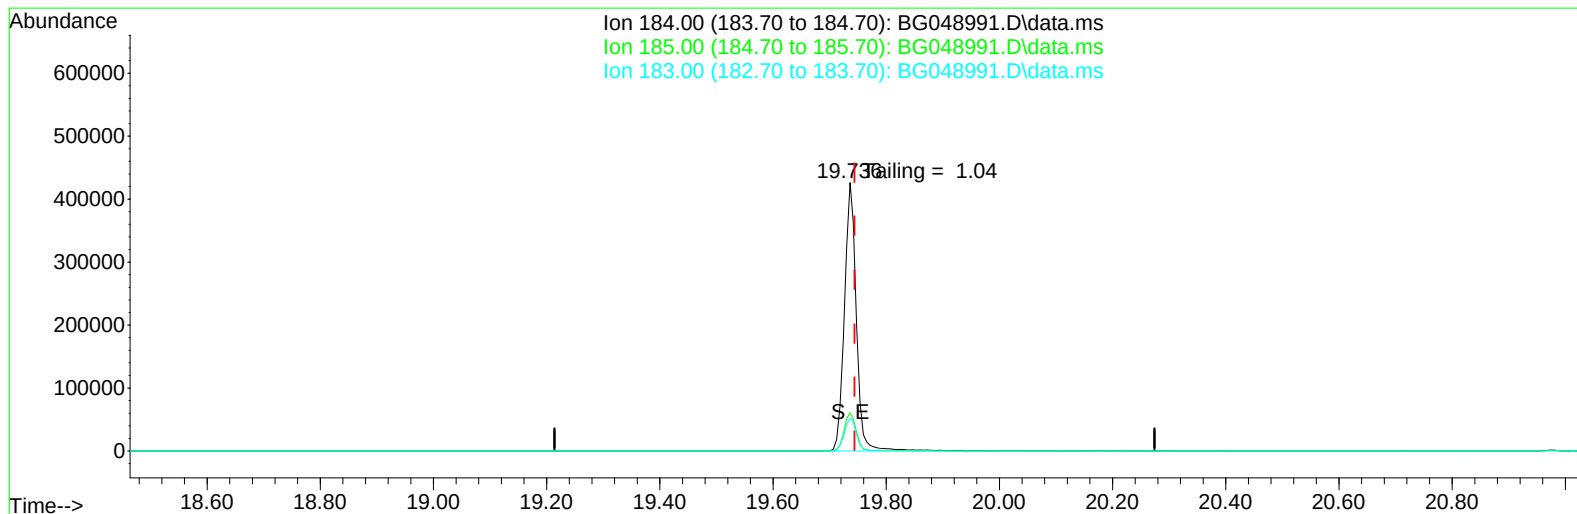

TIC: BG048991.D\data.ms

(77) Benzidine

19.736min (-0.008) 471572.23 ng

response 617487

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.25
183.00	11.70	12.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/16/2021	BNA_G	BG048991.D
Compound Name	Response	Retention Time
DDT	305826	20.97
DDD	996	20.52
DDE	337	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1333	307159	0.43