
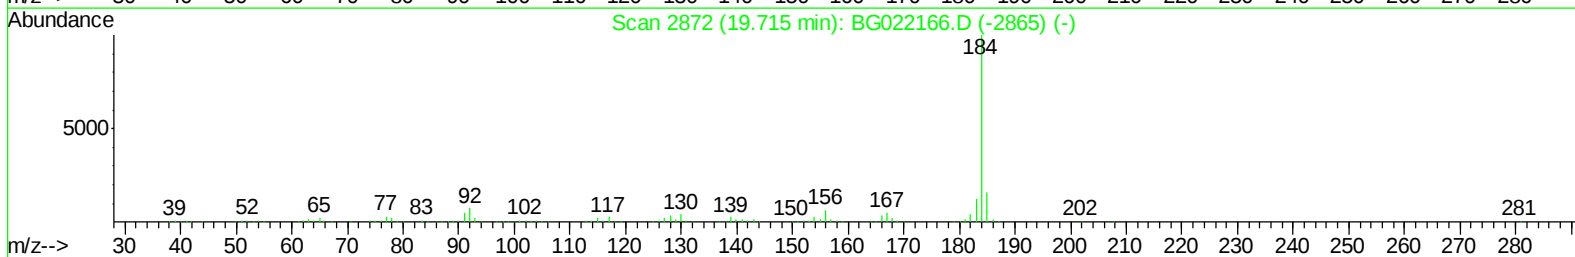
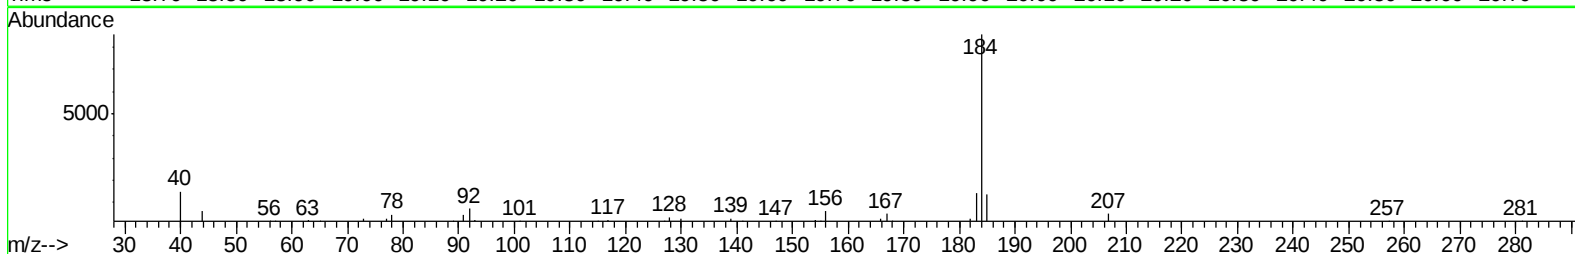


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061716\
Data File : BG022430.D
Acq On : 18 Jun 2016 19:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 09:01:31 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

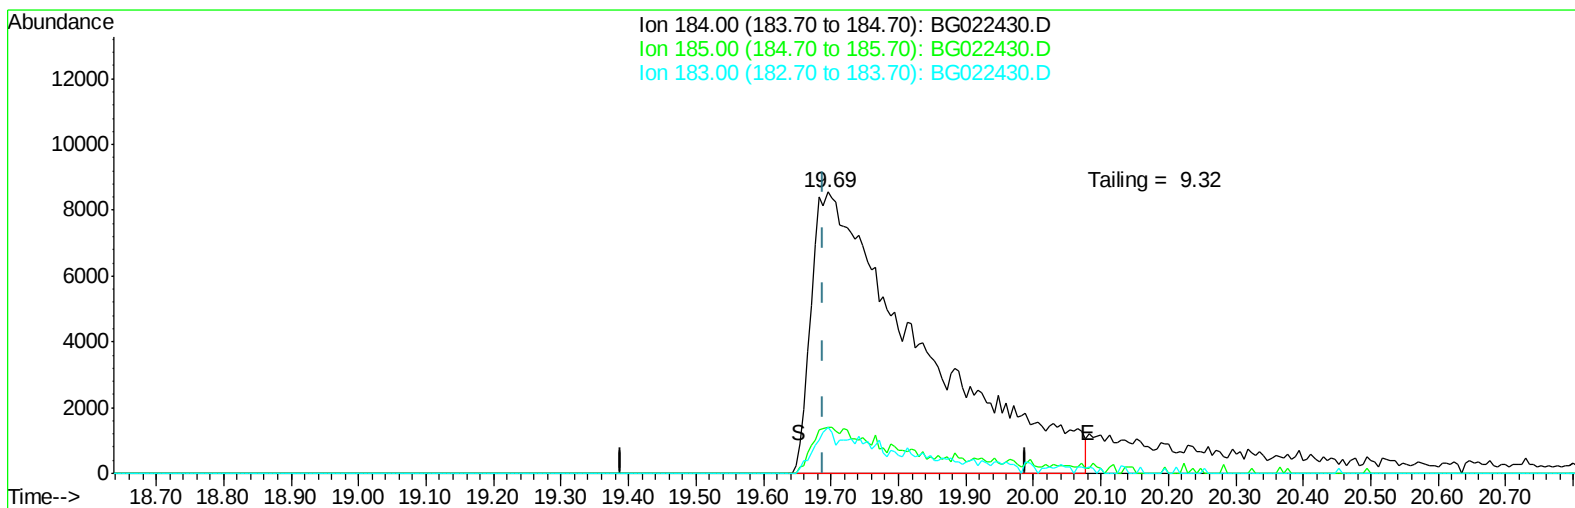

TIC: BG022430.D

(76) Benzidine




19.695min (+0.006) 0.00ng

response 57887

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	16.15
183.00	12.80	16.33#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG061716\
Data File : BG022430.D
Acq On : 18 Jun 2016 19:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 20 09:01:31 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 13 17:40:23 2016
Response via : Initial Calibration

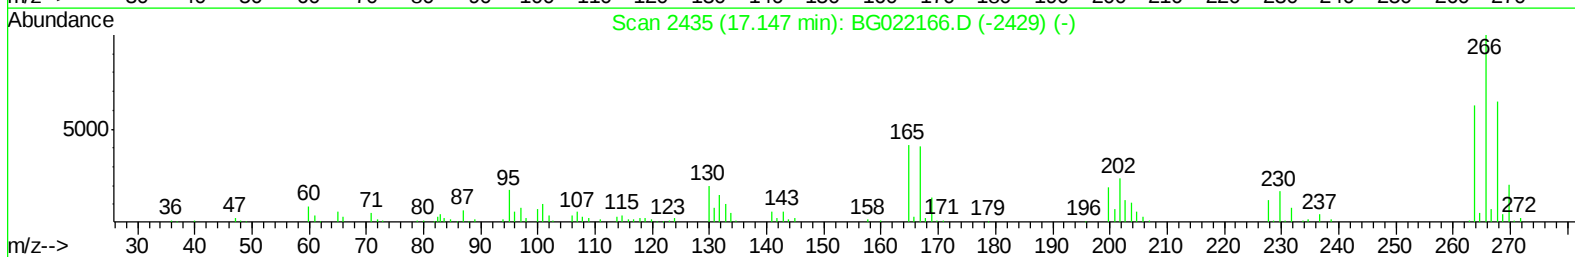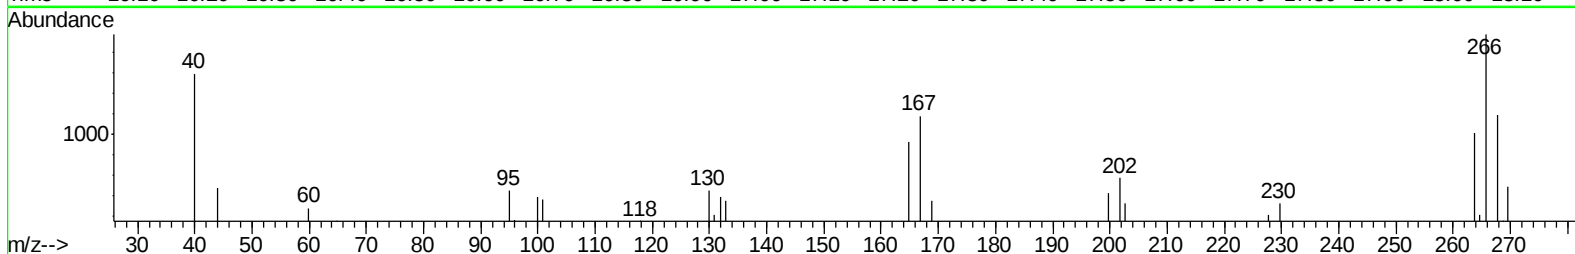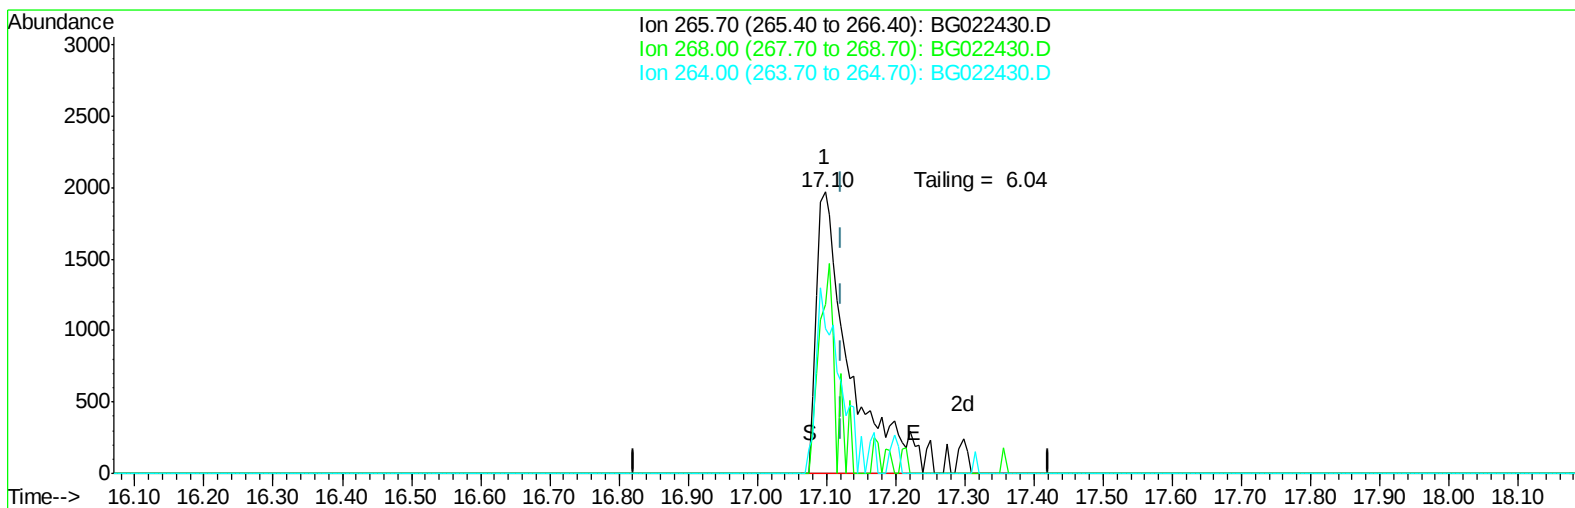

TIC: BG022430.D

(69) Pentachlorophenol (C)

17.098min (-0.023) 0.00ng m

response 6897

Ion	Exp%	Act%
265.70	100	100
268.00	68.10	60.15
264.00	67.20	51.22#
0.00	0.00	0.00