

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061716\
 Data File : BG022425.D
 Acq On : 18 Jun 2016 15:59
 Operator : UM/SJ
 Sample : H3607-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PE-003

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.600	464	470	482	rBV	123502	242776	14.03%	3.208%
2	7.227	741	747	760	rBV	74042	164828	9.52%	2.178%
3	7.580	800	807	824	rBV	281994	556854	32.18%	7.358%
4	8.044	879	886	895	rVB	61232	118679	6.86%	1.568%
5	8.367	931	941	952	rBV	268158	539908	31.20%	7.134%
6	9.219	1078	1086	1101	rBV	173842	381100	22.02%	5.036%
7	10.864	1359	1366	1380	rBV	89904	196889	11.38%	2.602%
8	13.302	1773	1781	1797	rBV	751719	1294158	74.78%	17.101%
9	14.683	2009	2016	2029	rBV2	192390	346681	20.03%	4.581%
10	16.176	2262	2270	2287	rBV	476772	835142	48.26%	11.036%
11	17.427	2476	2483	2497	rBV2	223268	405873	23.45%	5.363%
12	20.024	2918	2925	2939	rBV	1177075	1730512	100.00%	22.867%
13	21.258	3131	3135	3139	rBV	13047	20057	1.16%	0.265%
14	21.687	3202	3208	3219	rBV	192213	390463	22.56%	5.160%
15	24.930	3749	3760	3773	rBV3	103876	343651	19.86%	4.541%


Sum of corrected areas: 7567571

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061716\
Data File : BG022425.D
Acq On : 18 Jun 2016 15:59
Operator : UM/SJ
Sample : H3607-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-003

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

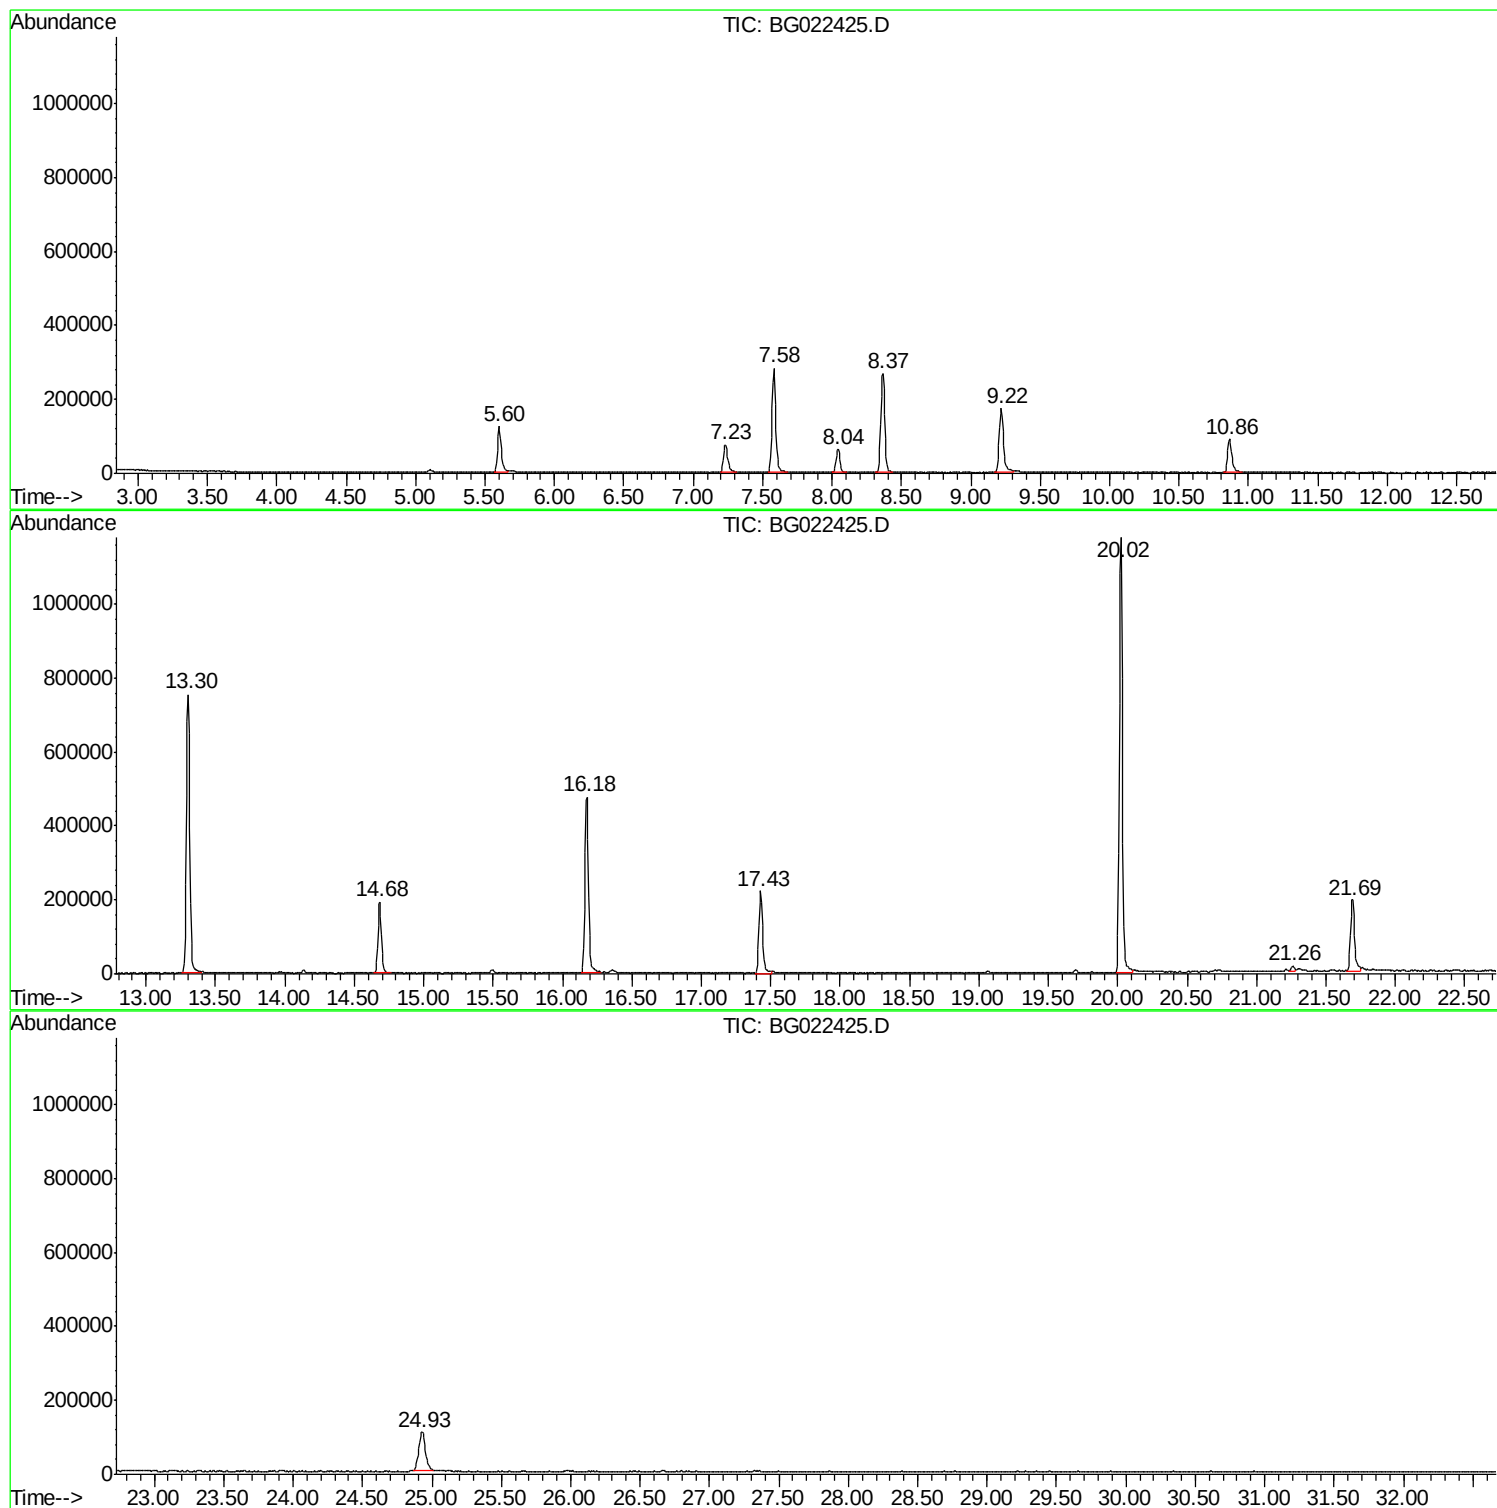

Data Path : Z:\HPCHEM1\BNA G\DATA\BG061716\
Data File : BG022425.D
Acq On : 18 Jun 2016 15:59
Operator : UM/SJ
Sample : H3607-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-003










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.58 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.58	93.84 ng	556854	1,4-Dichlorobenzene-d4	8.04

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

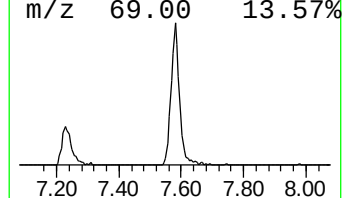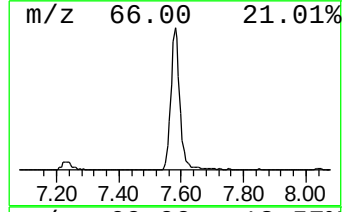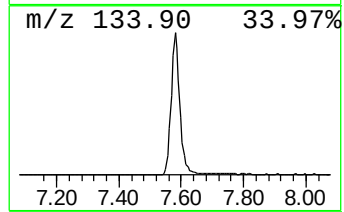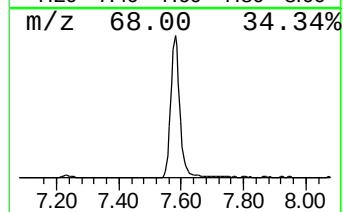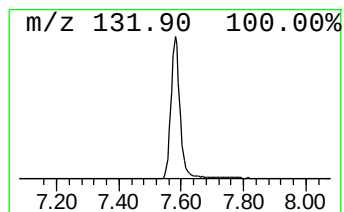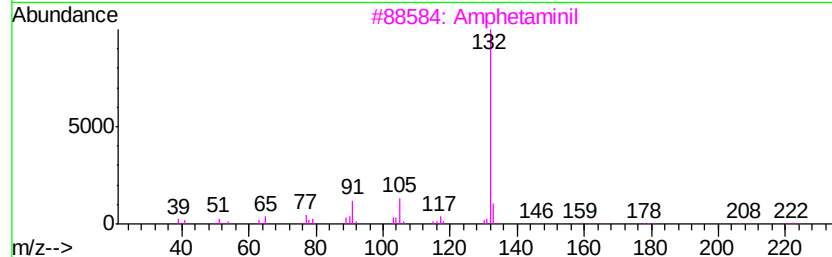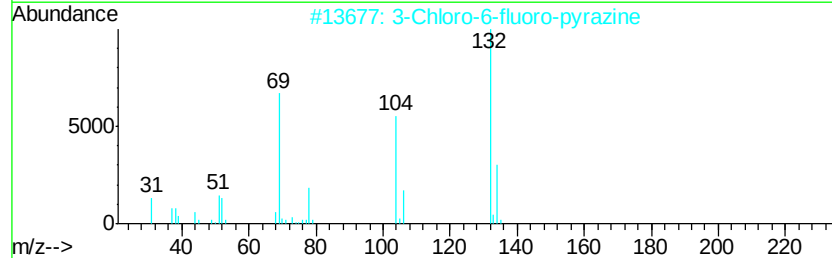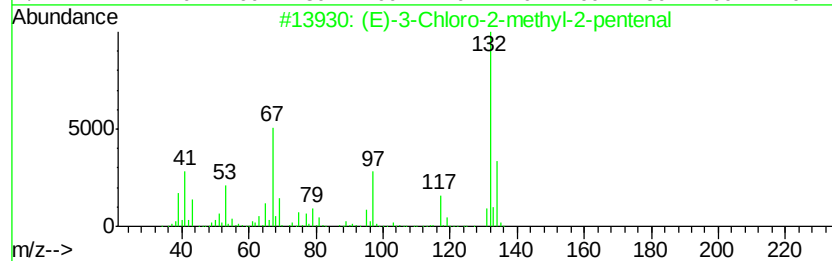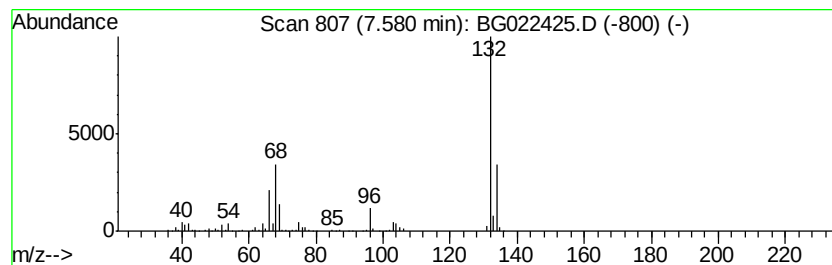

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061716\
Data File : BG022425.D
Acq On : 18 Jun 2016 15:59
Operator : UM/SJ
Sample : H3607-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PE-003

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.58	7.58	93.8	ng	556854	1	8.04	118679	20.0