


Data Path : Z:\HPCHEM1\BNA G\DATA\BG061716\
 Data File : BG022414.D
 Acq On : 18 Jun 2016 8:35
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 17:40:23 2016

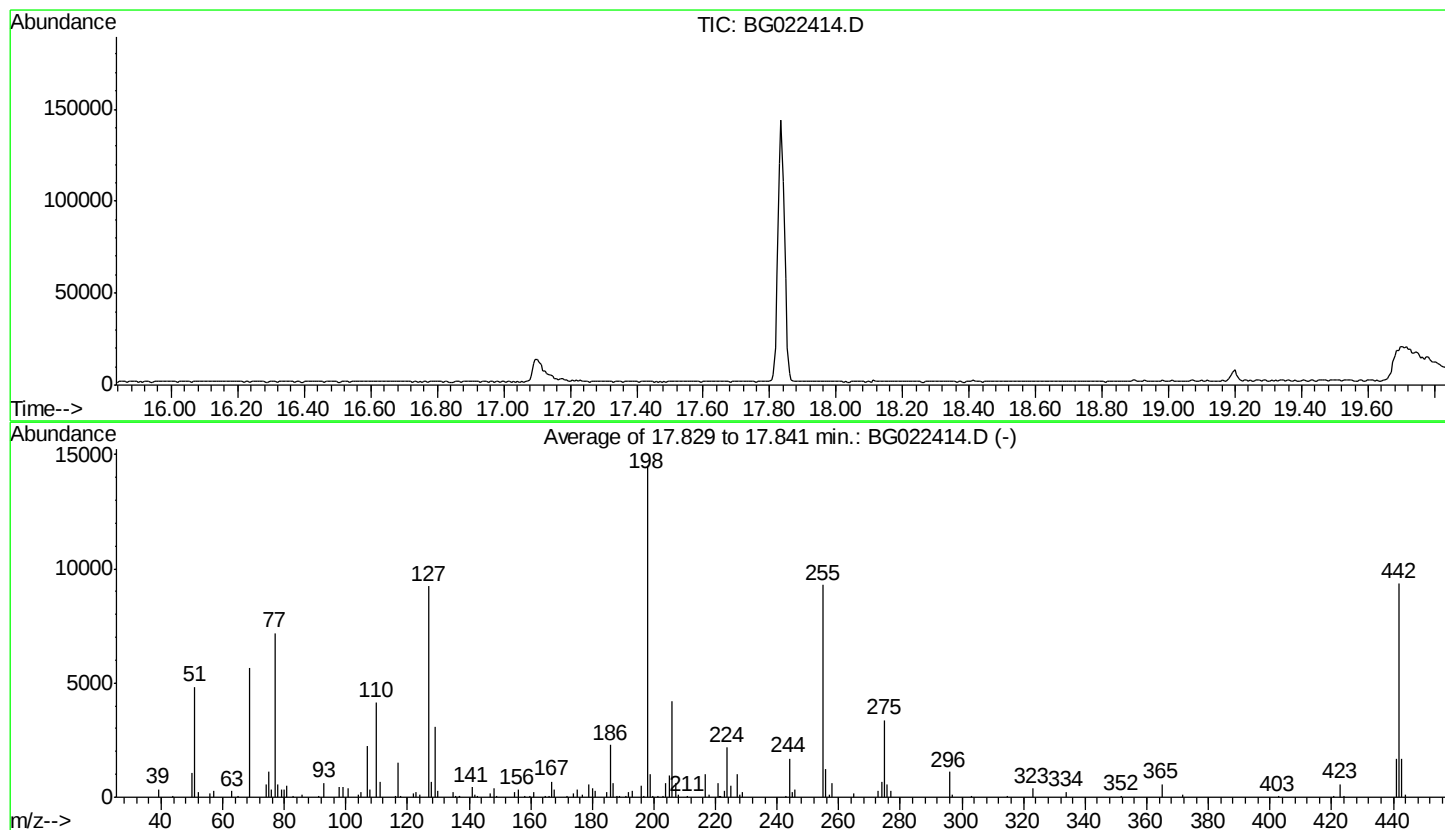

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2545

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	4819	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.9	5648	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	63.7	9238	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14510	PASS
199	198	5	9	7.1	1031	PASS
275	198	10	60	23.2	3371	PASS
365	198	1	100	3.9	561	PASS
441	442	0.01	24	18.0	1681	PASS
442	198	50	100	64.4	9343	PASS
443	442	15	24	18.3	1710	PASS