


Data Path : Z:\HPCHEM1\BNA G\DATA\BG061716\
 Data File : BG022430.D
 Acq On : 18 Jun 2016 19:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG060616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 13 17:40:23 2016

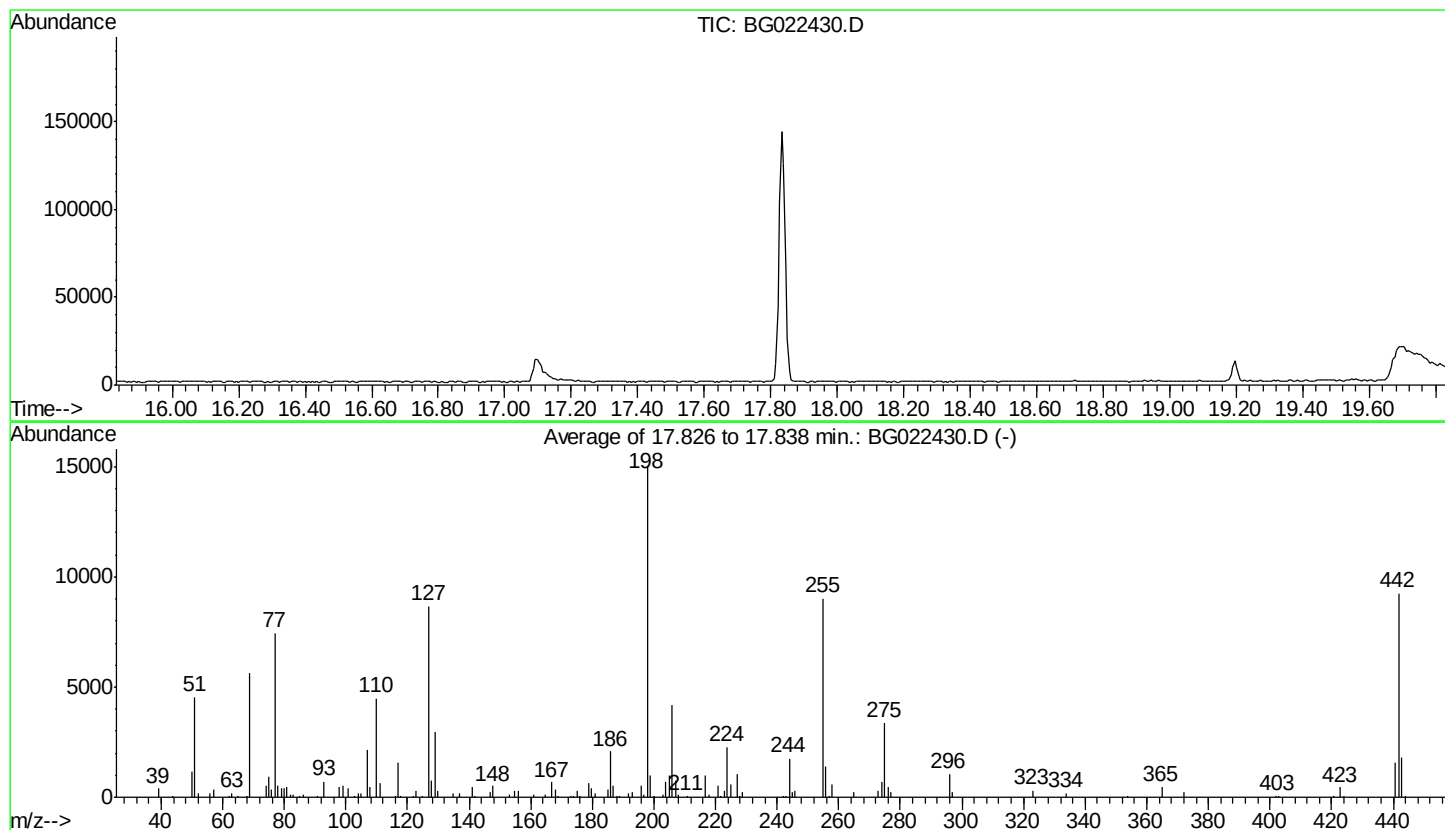

AutoFind: Scans 2551, 2552, 2553; Background Corrected with Scan 2545

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	4538	PASS
68	69	0.00	2	1.1	61	PASS
69	198	0.00	100	37.3	5618	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.6	8667	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	15045	PASS
199	198	5	9	6.6	987	PASS
275	198	10	60	22.6	3398	PASS
365	198	1	100	3.2	474	PASS
441	442	0.01	24	16.9	1564	PASS
442	198	50	100	61.4	9238	PASS
443	442	15	24	19.3	1785	PASS