
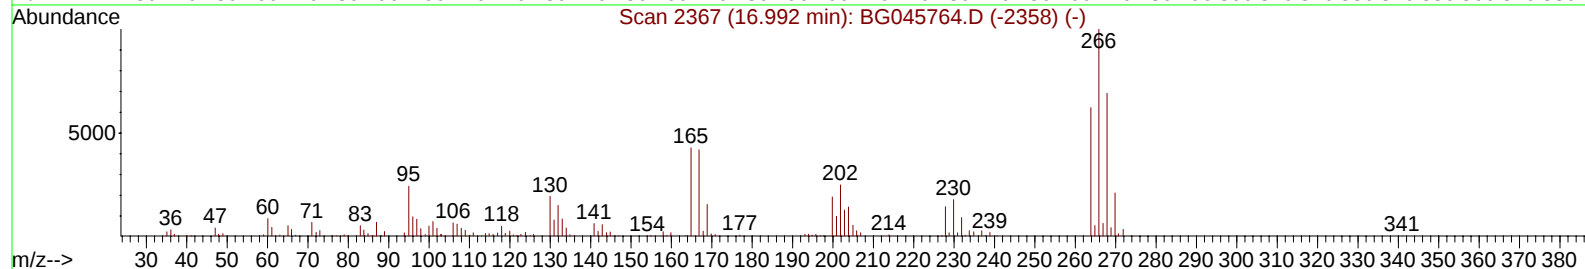
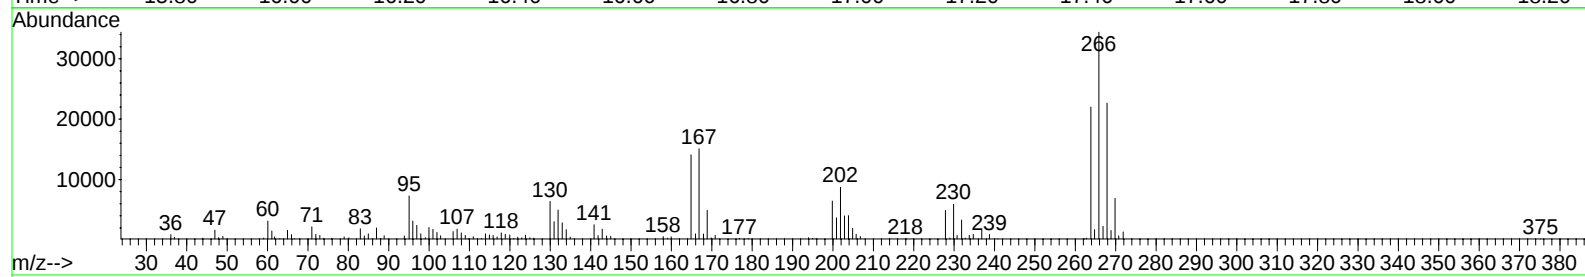


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061720\
Data File : BG045783.D
Acq On : 17 Jun 2020 9:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 18:18:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 18:34:19 2020
Response via : Initial Calibration

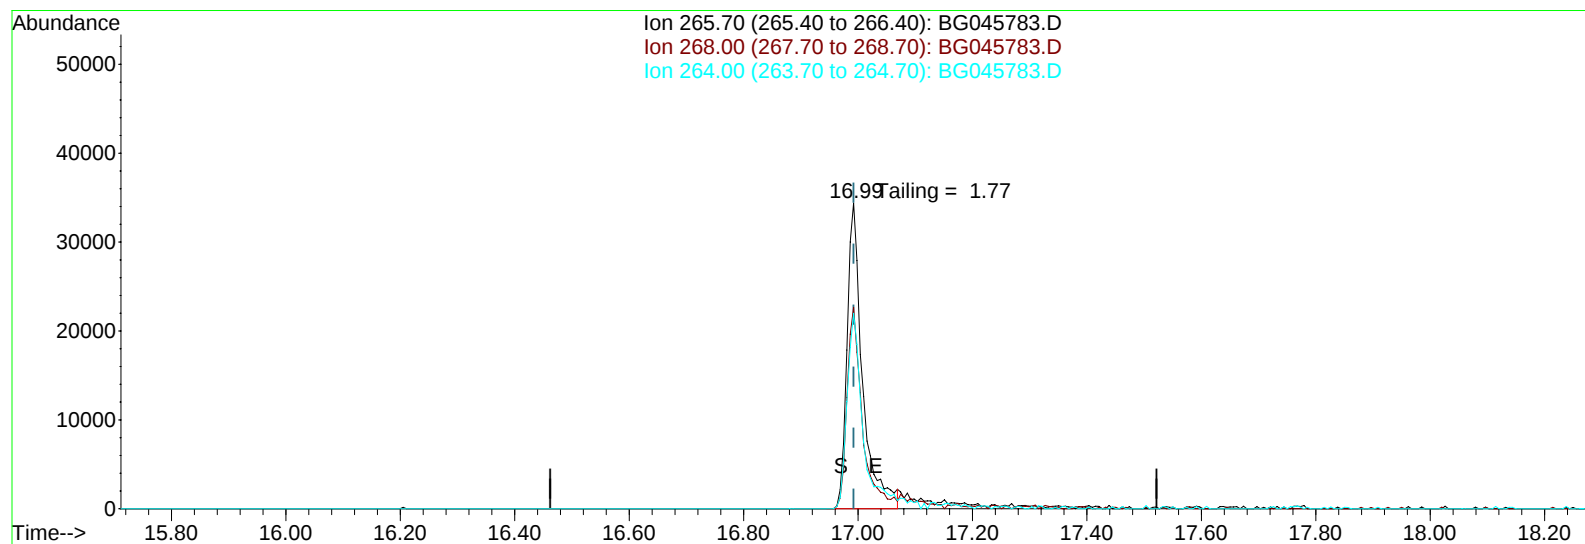

TIC: BG045783.D

(70) Pentachlorophenol (C)




16.992min (+0.000) 167685.91ng

response 67745

Ion	Exp%	Act%
265.70	100	100
268.00	69.20	65.88
264.00	62.20	63.95
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061720\
Data File : BG045783.D
Acq On : 17 Jun 2020 9:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 18:18:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 18:34:19 2020
Response via : Initial Calibration

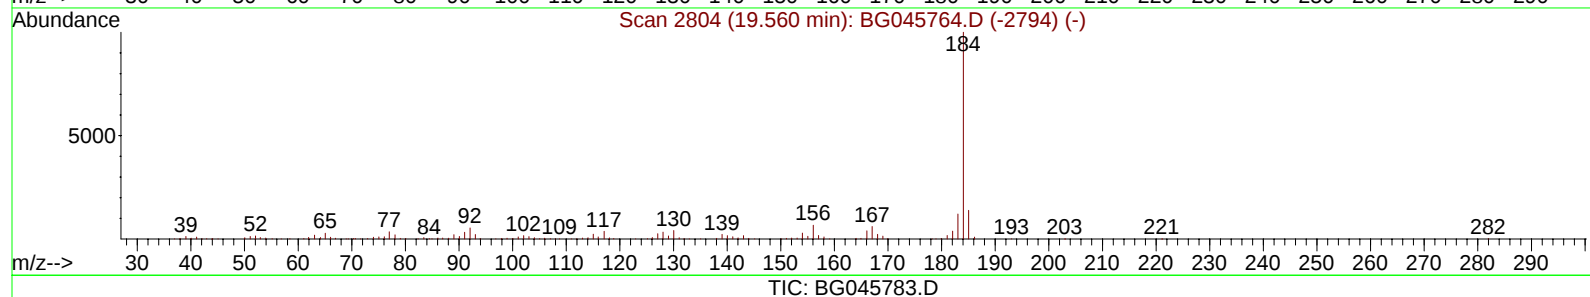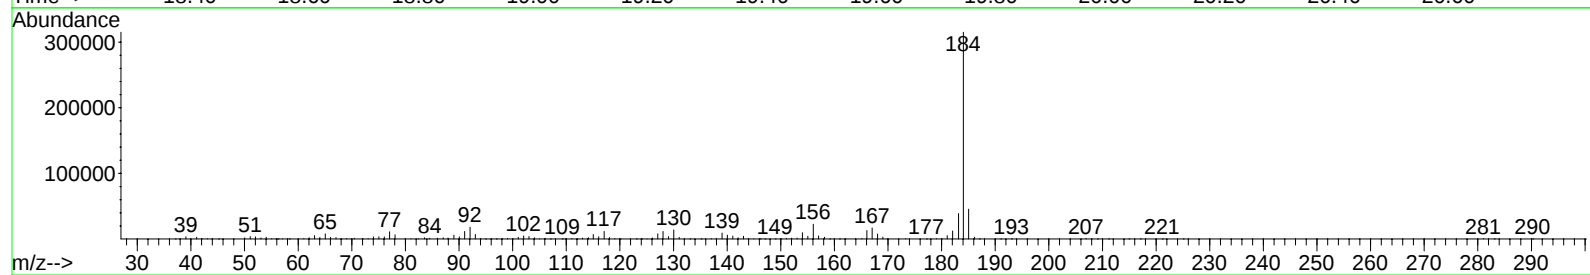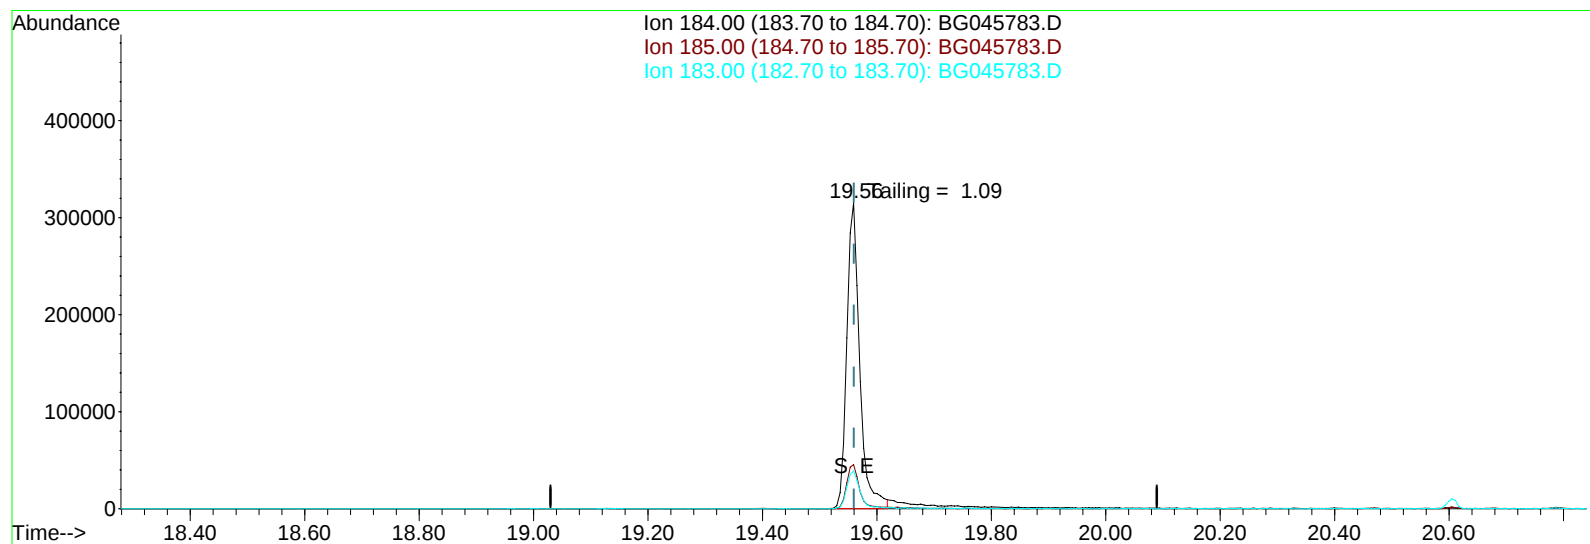

(77) Benzidine

19.559min (-0.000) 336120.68ng

response 524288

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.47
183.00	12.10	12.35
0.00	0.00	0.00