

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061720\
 Data File : BG045789.D
 Acq On : 17 Jun 2020 14:03
 Operator : CG/JU
 Sample : L3017-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SG1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.531	409	416	432	rBV	615624	1079034	36.95%	6.354%
2	7.159	684	693	708	rBV	707301	1313570	44.98%	7.735%
3	7.916	815	822	829	rBV	228713	397722	13.62%	2.342%
4	8.240	870	877	888	rBV	623584	1127663	38.61%	6.640%
5	9.080	1012	1020	1032	rBV	480329	916892	31.39%	5.399%
6	10.724	1292	1300	1312	rBV	297668	556381	19.05%	3.276%
7	13.186	1712	1719	1734	rBV	1385793	2258719	77.34%	13.300%
8	13.474	1760	1768	1779	rBV	180118	293115	10.04%	1.726%
9	14.020	1855	1861	1867	rBV	105467	159164	5.45%	0.937%
10	14.566	1947	1954	1962	rBV	493722	777567	26.62%	4.579%
11	15.700	2141	2147	2157	rBV2	137713	227043	7.77%	1.337%
12	16.070	2202	2210	2224	rBV	1069740	1710764	58.58%	10.074%
13	17.316	2416	2422	2432	rBV	556305	878716	30.09%	5.174%
14	17.703	2485	2488	2495	rVB5	22074	37675	1.29%	0.222%
15	18.226	2572	2577	2582	rBV4	31937	55264	1.89%	0.325%
16	19.072	2717	2721	2730	rBV	142956	243607	8.34%	1.434%
17	19.389	2771	2775	2779	rBV2	50216	68475	2.34%	0.403%
18	19.935	2862	2868	2875	rBV	2178546	2920507	100.00%	17.197%
19	20.576	2974	2977	2981	rVB	38818	44153	1.51%	0.260%
20	21.234	3085	3089	3099	rVB2	113928	201704	6.91%	1.188%
21	21.574	3142	3147	3155	rBV	504592	802548	27.48%	4.726%
22	24.706	3671	3680	3692	rBV	319155	911984	31.23%	5.370%


Sum of corrected areas: 16982267

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG061720\
Data File : BG045789.D
Acq On : 17 Jun 2020 14:03
Operator : CG/JU
Sample : L3017-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SG1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

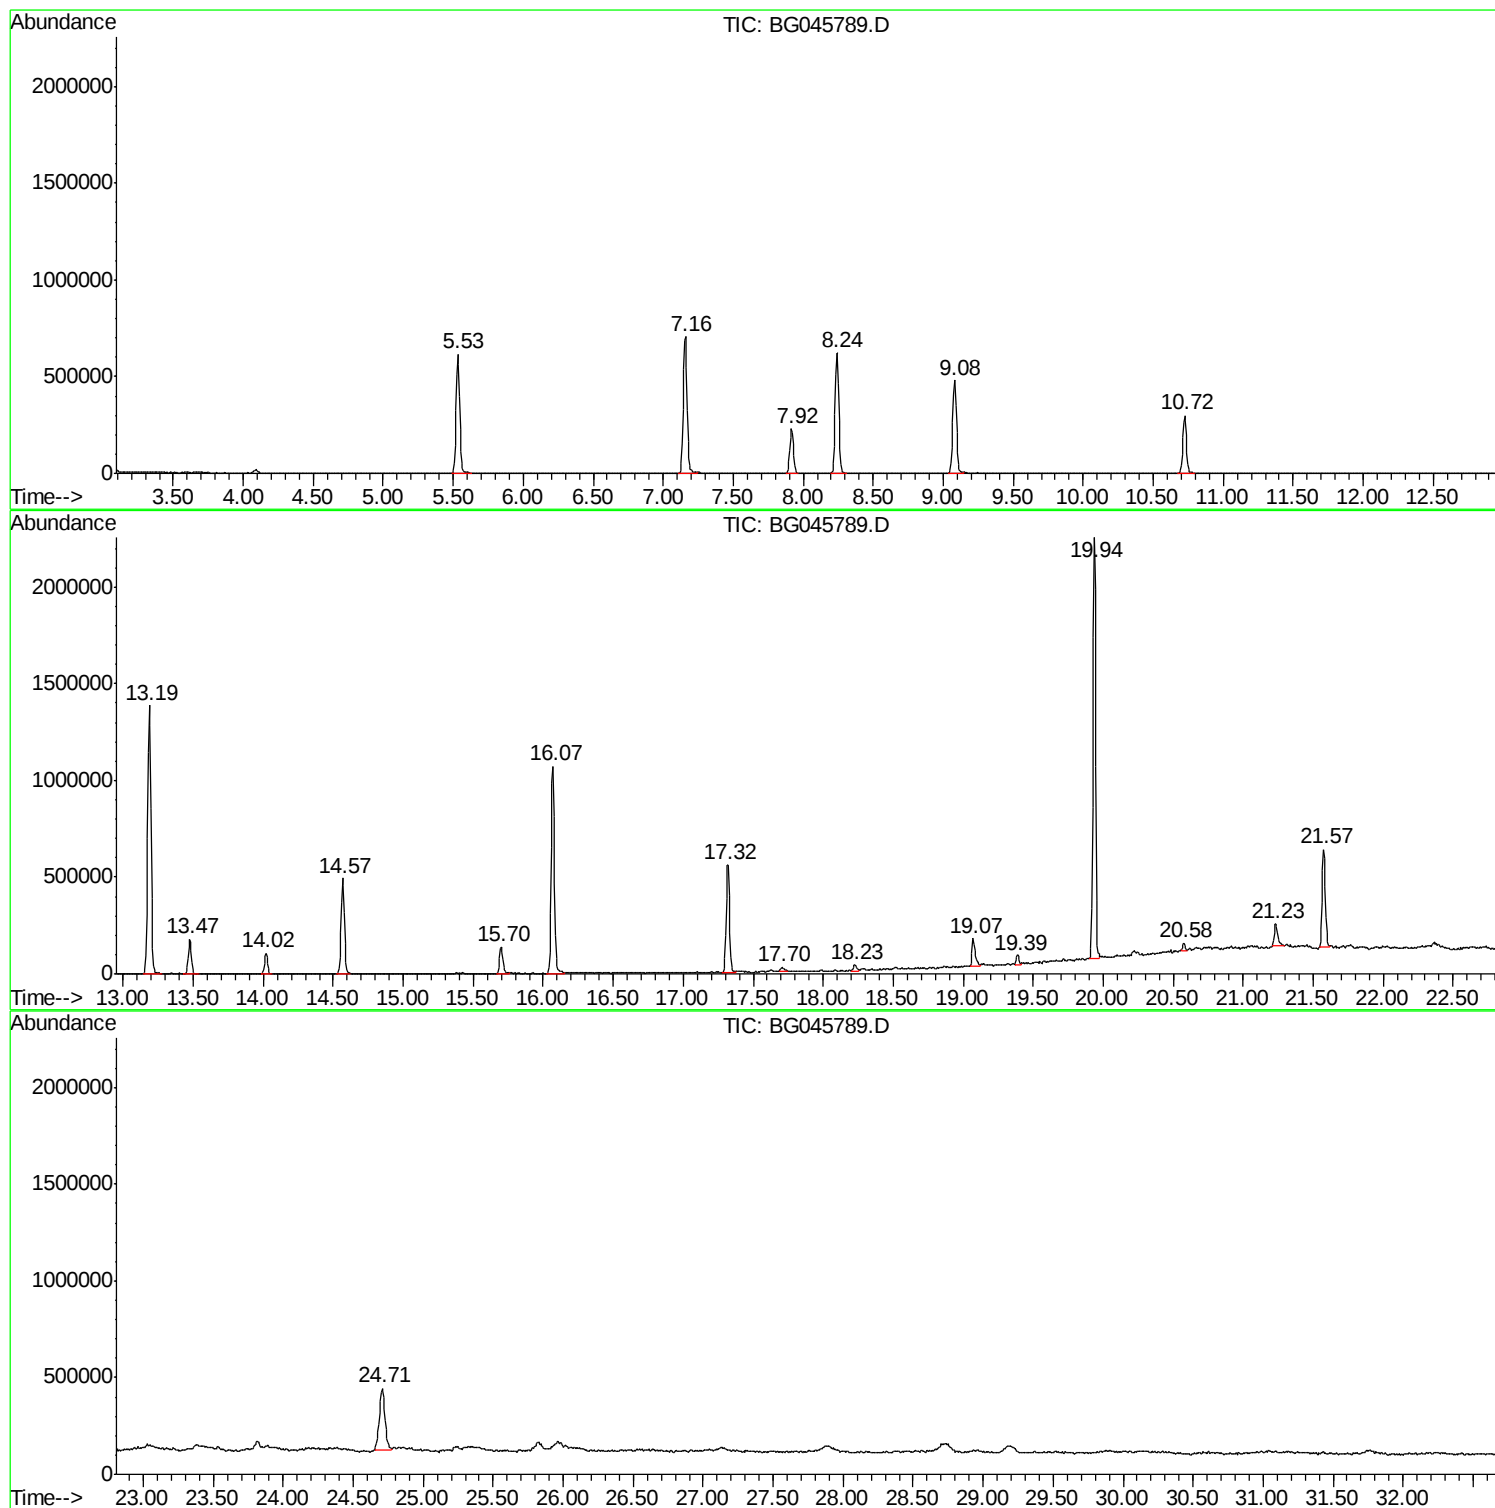

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061720\
Data File : BG045789.D
Acq On : 17 Jun 2020 14:03
Operator : CG/JU
Sample : L3017-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SG1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061720\
Data File : BG045789.D
Acq On : 17 Jun 2020 14:03
Operator : CG/JU
Sample : L3017-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SG1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc