


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061720\
 Data File : BG045783.D
 Acq On : 17 Jun 2020 9:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 15 18:34:19 2020

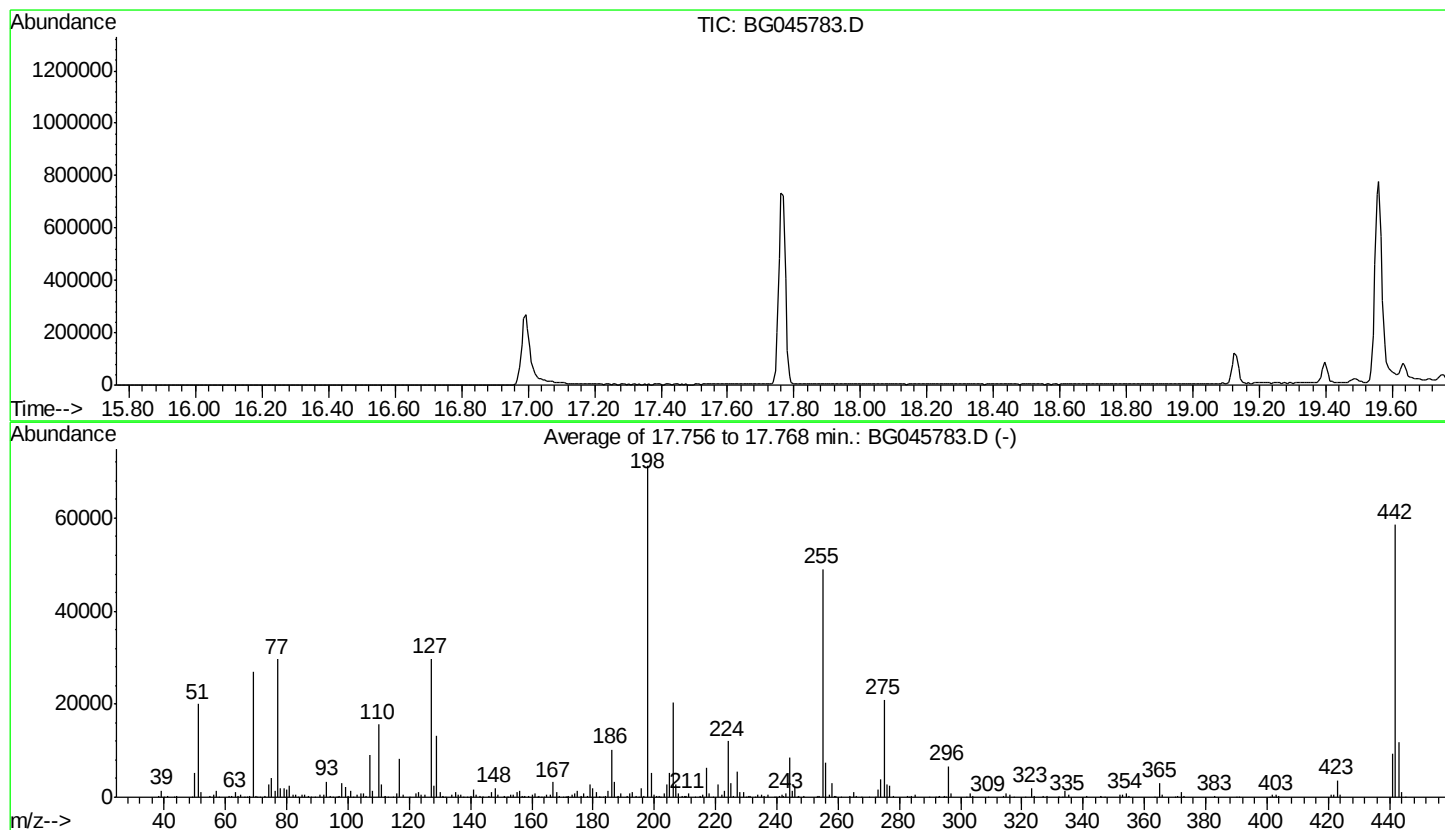

AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	20021	PASS
68	69	0.00	2	1.6	422	PASS
69	198	0.00	100	37.7	26844	PASS
70	69	0.00	2	0.9	231	PASS
127	198	10	80	41.7	29736	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71272	PASS
199	198	5	9	7.2	5132	PASS
275	198	10	60	29.4	20984	PASS
365	198	1	100	4.3	3073	PASS
441	198	0.01	100	13.3	9462	PASS
442	198	50	100	82.1	58530	PASS
443	442	15	24	20.4	11937	PASS