
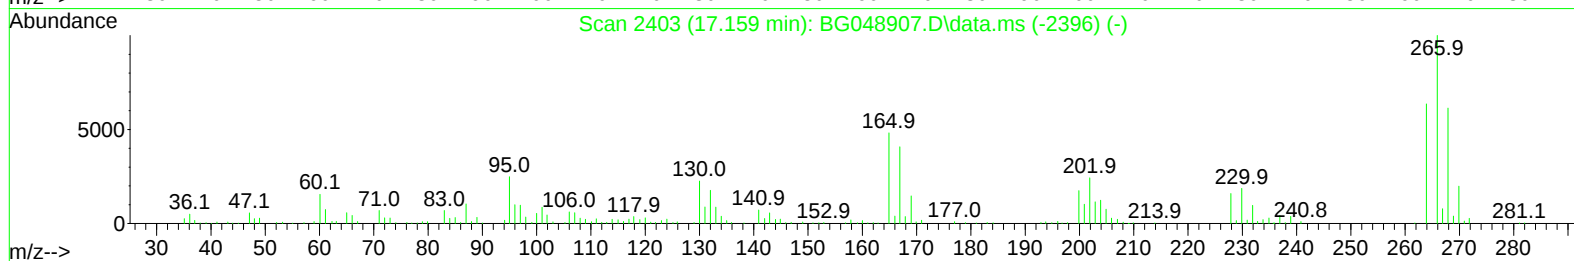
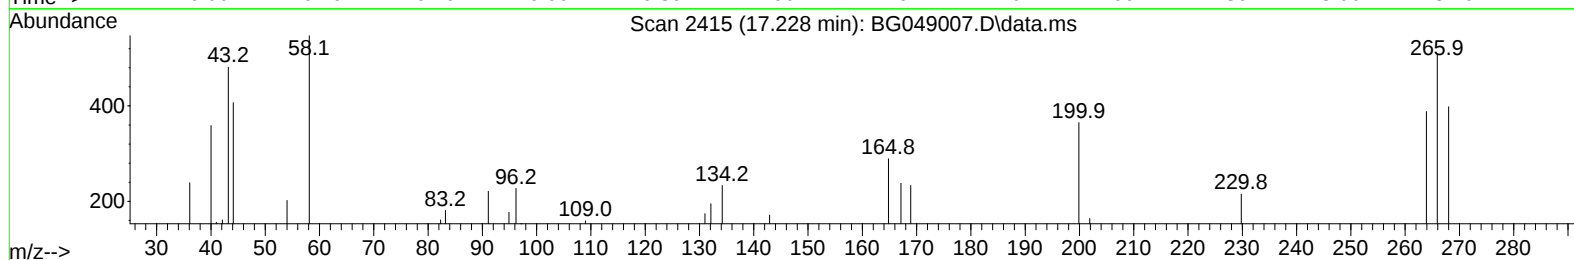


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061721\
Data File : BG049007.D
Acq On : 17 Jun 2021 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 12:30:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

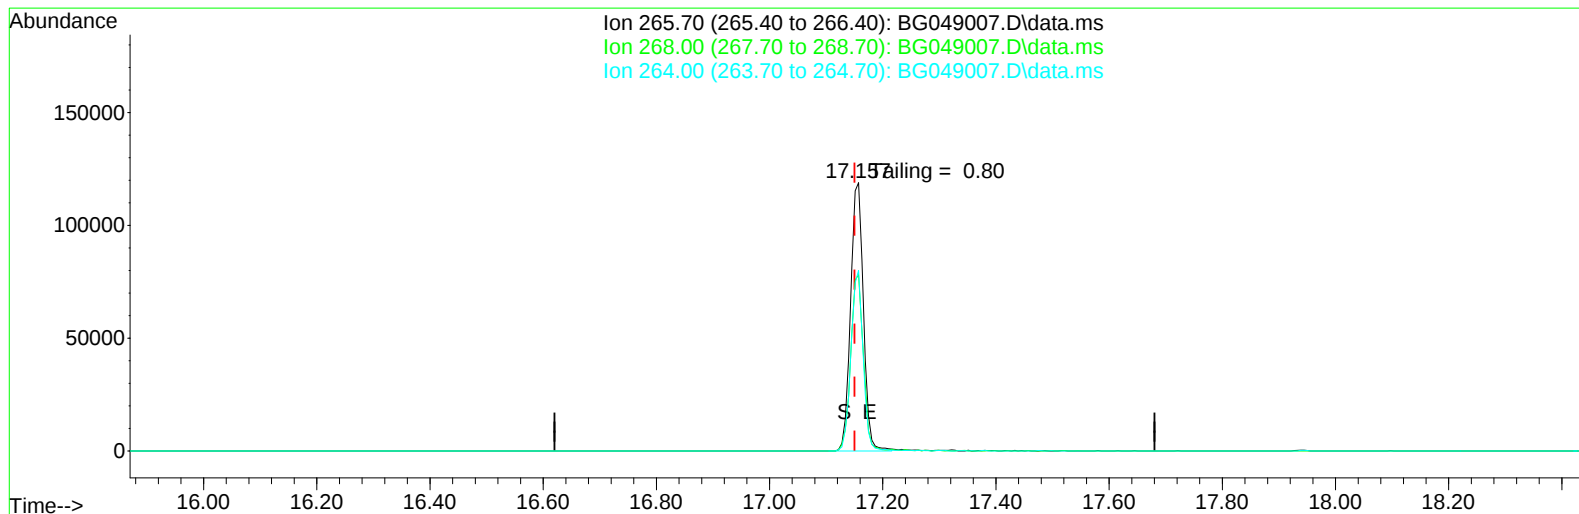

TIC: BG049007.D\data.ms

(70) Pentachlorophenol (C)




17.157min (+ 0.007) 204901.82 ng

response 188314

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.68
264.00	61.30	67.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061721\
 Data File : BG049007.D
 Acq On : 17 Jun 2021 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 17 12:30:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 12:04:50 2021
 Response via : Initial Calibration

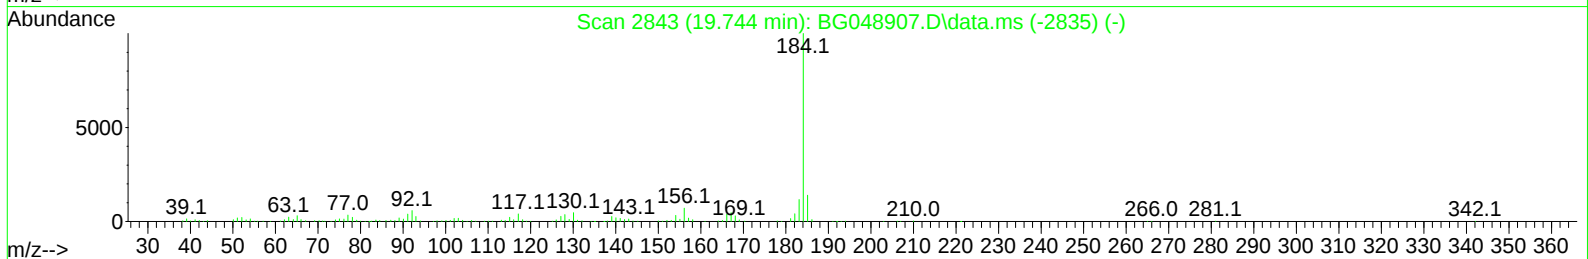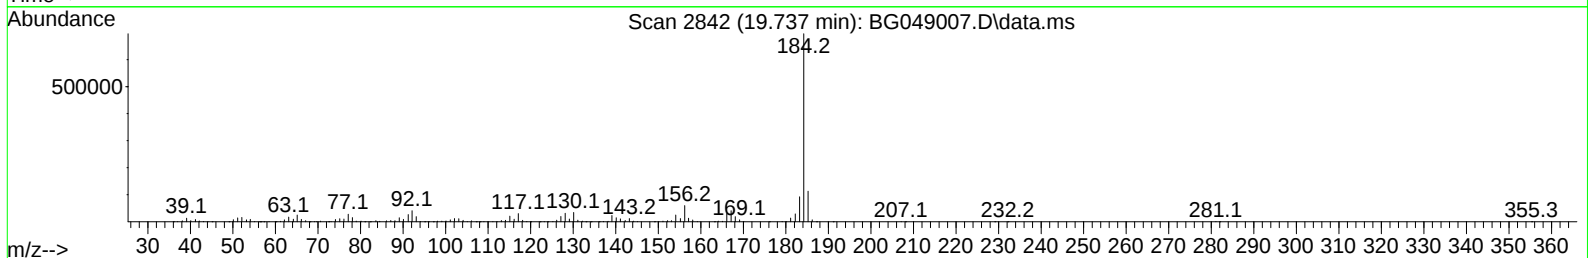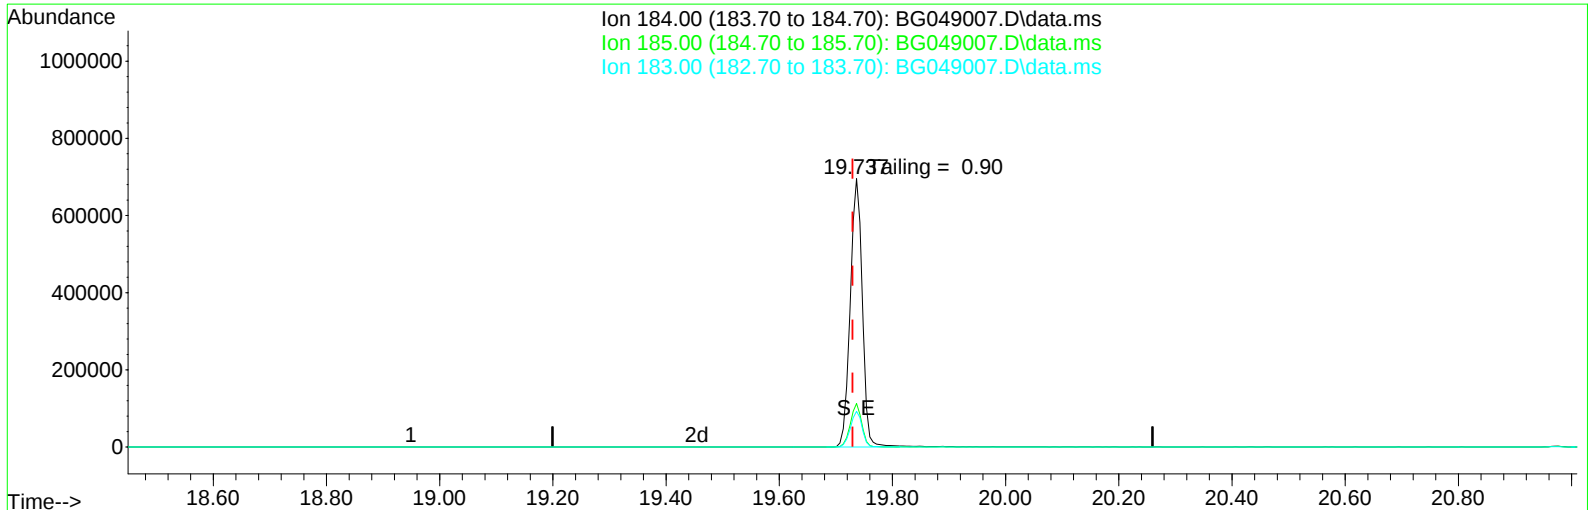

TIC: BG049007.D\data.ms

(77) Benzidine

19.737min (+ 0.007) 6283.28 ng m

response 1029445

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	16.26#
183.00	11.70	13.31
0.00	0.00	0.00