
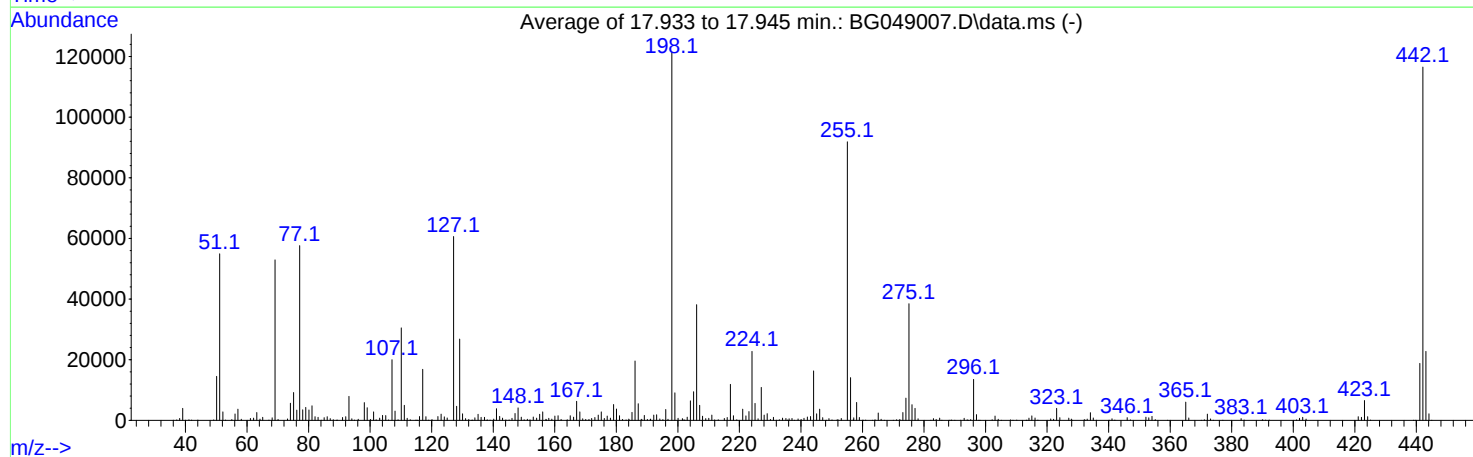


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061721\
 Data File : BG049007.D
 Acq On : 17 Jun 2021 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 16 12:04:50 2021

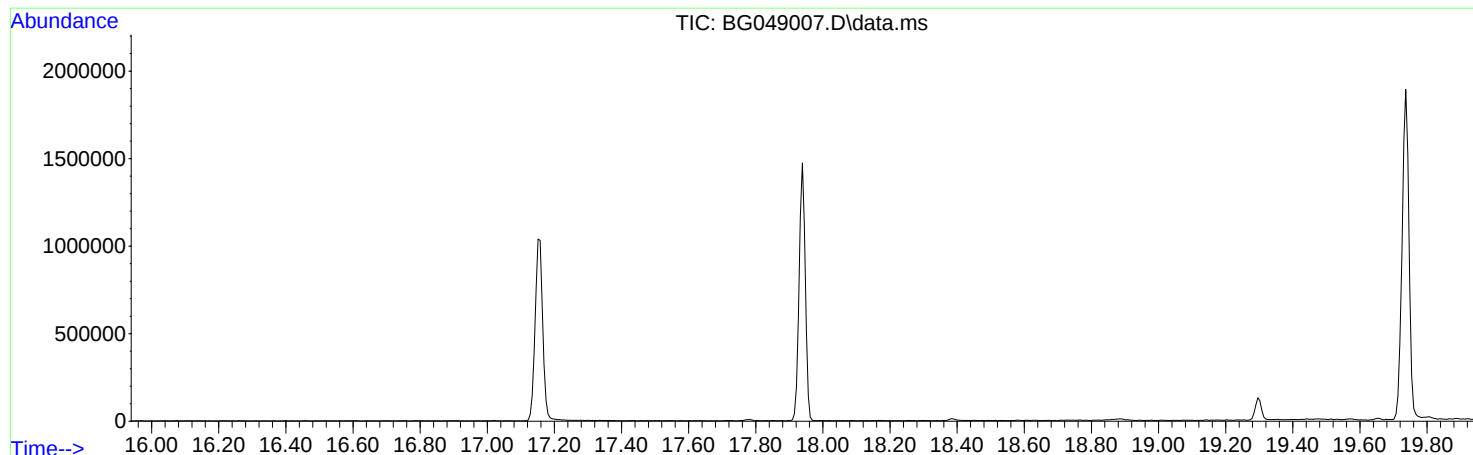


AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	54941	PASS
68	69	0.00	2	1.6	865	PASS
69	198	0.00	100	43.6	52903	PASS
70	69	0.00	2	0.7	344	PASS
127	198	10	80	50.0	60619	PASS
197	198	0.00	2	0.3	363	PASS
198	198	100	100	100.0	121307	PASS
199	198	5	9	7.5	9063	PASS
275	198	10	60	31.7	38472	PASS
365	198	1	100	4.9	5999	PASS
441	198	0.01	100	15.5	18797	PASS
442	442	100	100	100.0	116501	PASS
443	442	15	24	19.5	22733	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061721\
Data File : BG049007.D
Acq On : 17 Jun 2021 9:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 17 12:30:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

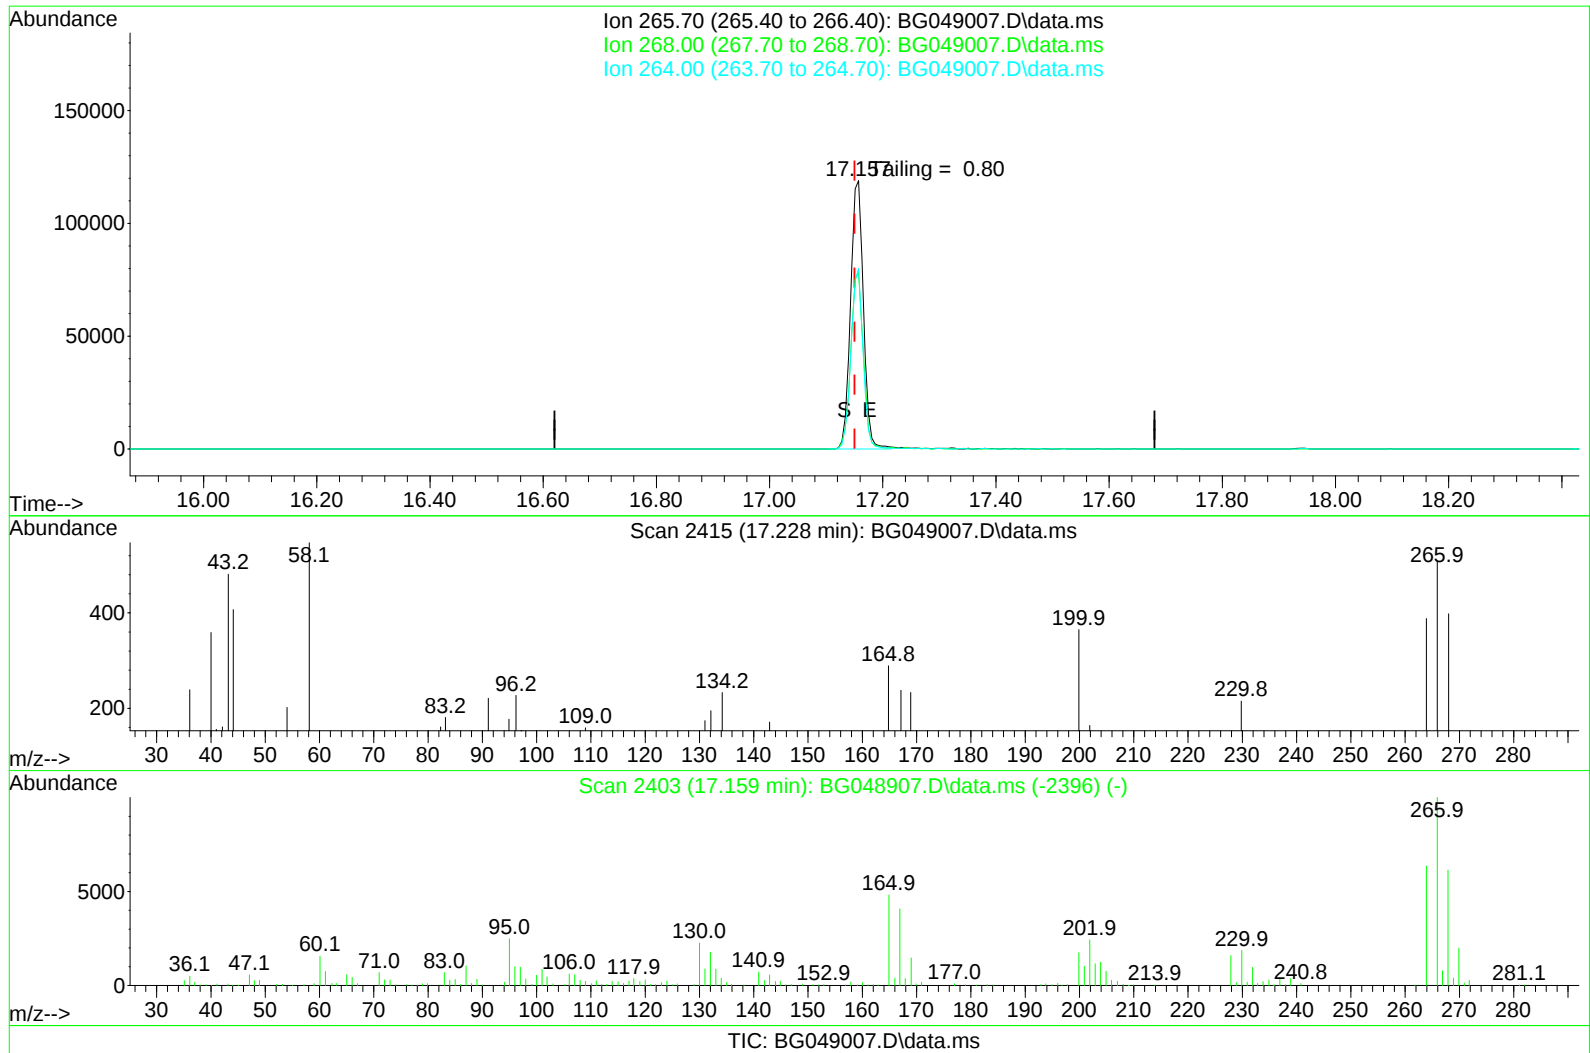

(70) Pentachlorophenol (C)

17.157min (+ 0.007) 204901.82 ng




response 188314

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	65.68
264.00	61.30	67.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061721\
 Data File : BG049007.D
 Acq On : 17 Jun 2021 9:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 17 12:30:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 16 12:04:50 2021
 Response via : Initial Calibration

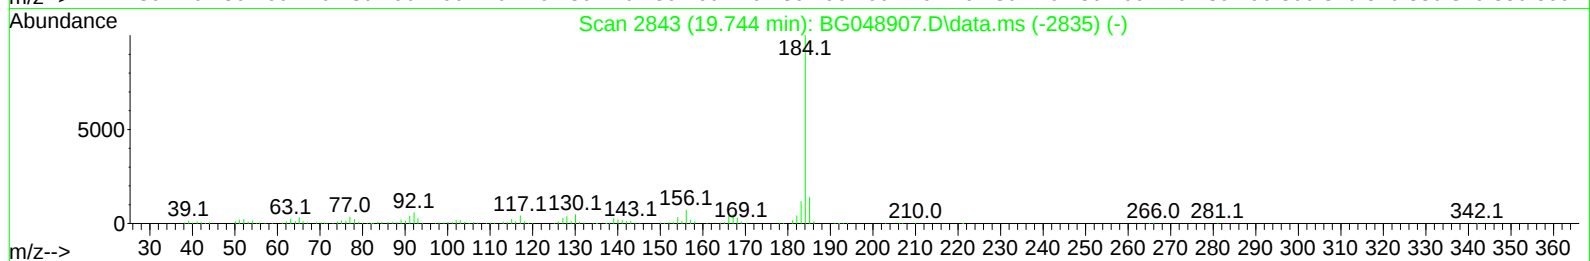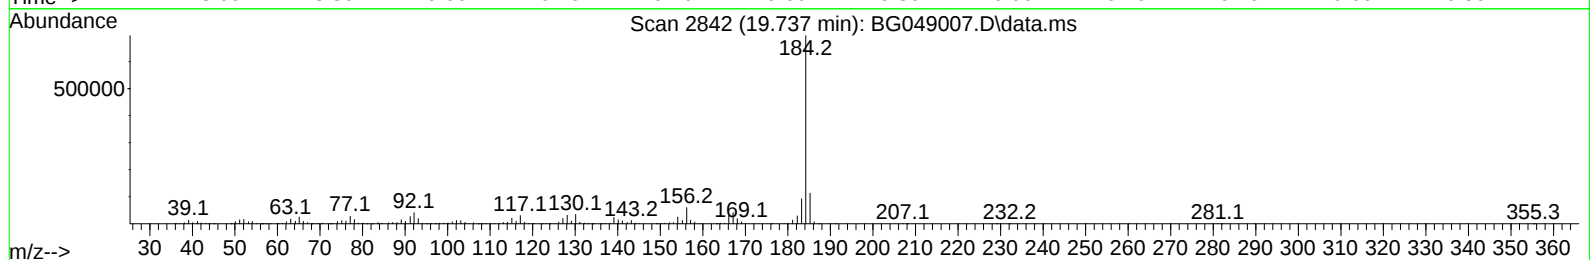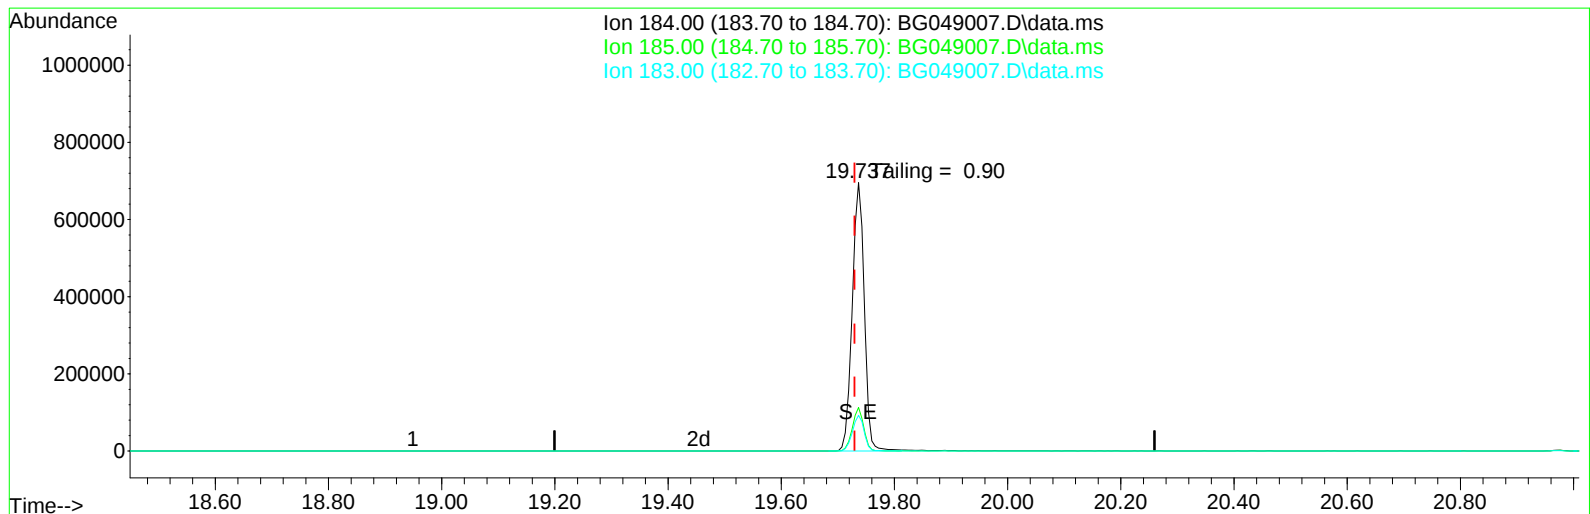

TIC: BG049007.D\data.ms

(77) Benzidine

19.737min (+ 0.007) 6283.28 ng m

response 1029445

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	16.26#
183.00	11.70	13.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/17/2021	BNA_G	BG049007.D
Compound Name	Response	Retention Time
DDT	547679	20.97
DDD	2705	20.52
DDE	860	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3565	551244	0.65