



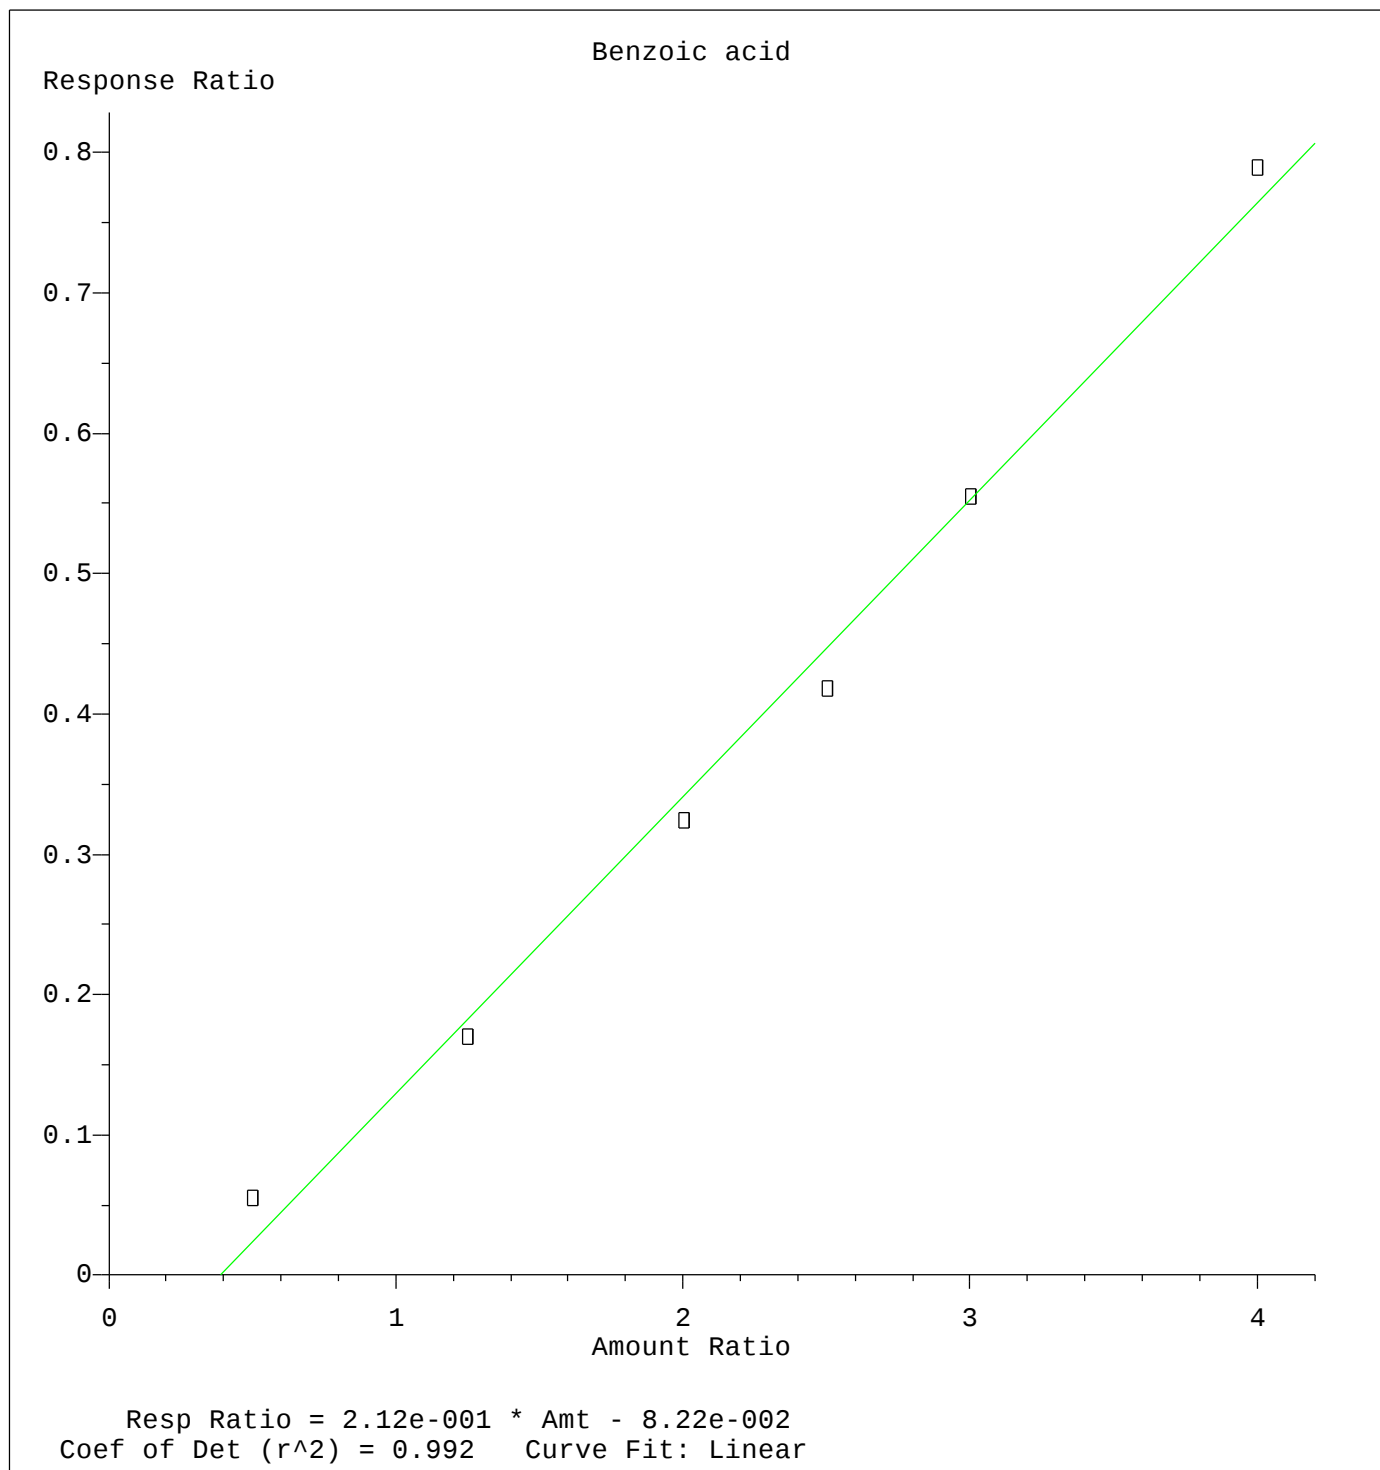


Method Name: Z:\HPCHEM1\BNA\_G\METHODS\8270-BG061815.M  
Calibration Table Last Updated: Fri Jun 19 06:05:07 2015

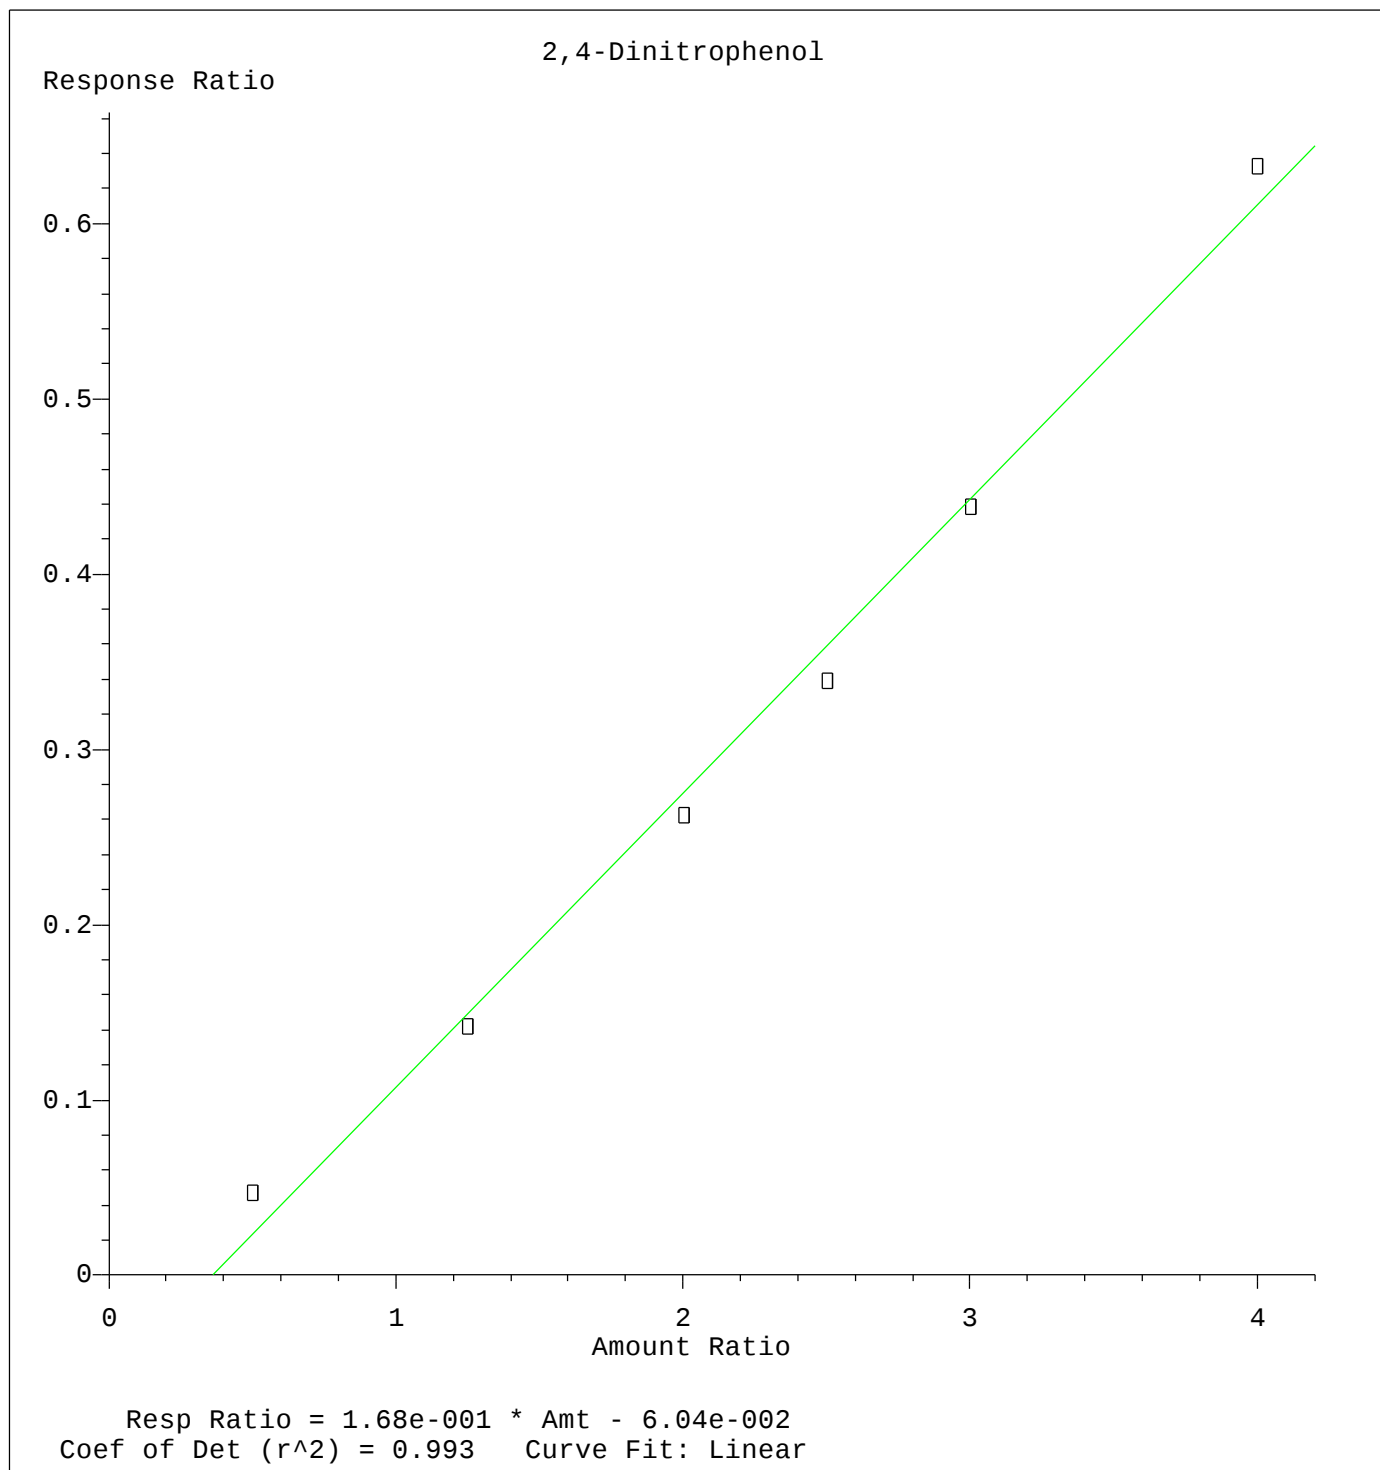

Method Name: Z:\HPCHEM1\BNA\_G\METHODS\8270-BG061815.M  
Calibration Table Last Updated: Fri Jun 19 06:05:07 2015

# 2,4-Dinitrotoluene


Response Ratio

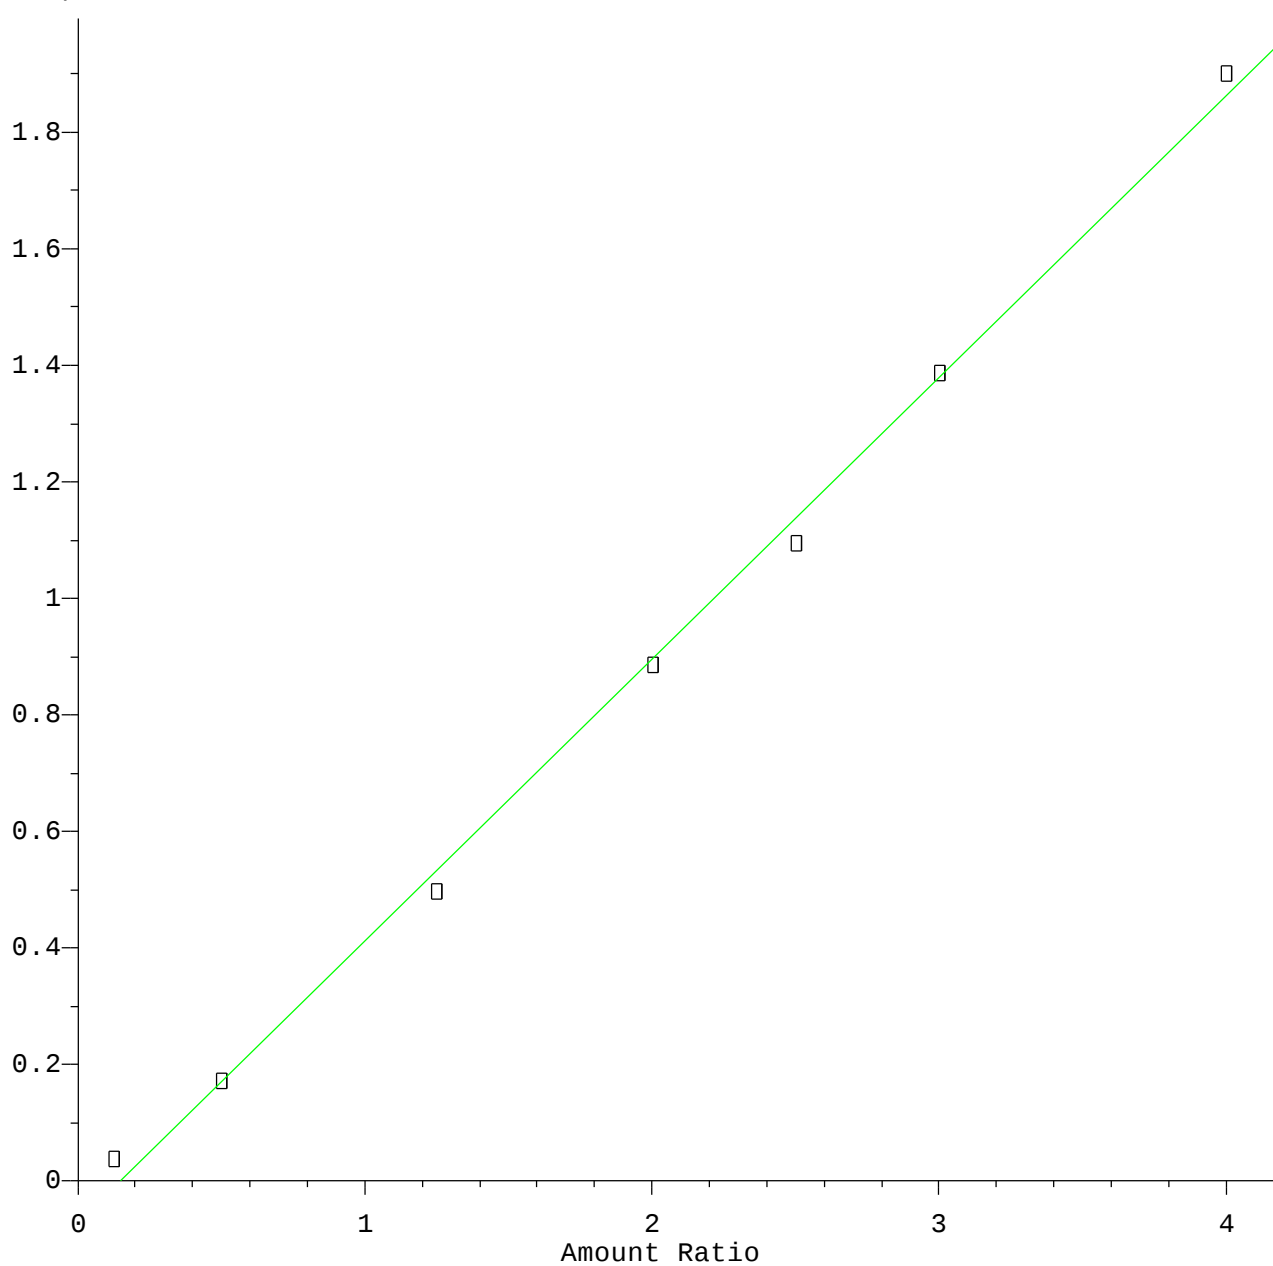

Resp Ratio =  $4.83 \times 10^{-1} \times \text{Amt} - 7.08 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.997    Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA\_G\METHODS\8270-BG061815.M  
Calibration Table Last Updated: Fri Jun 19 06:05:07 2015

4,6-Dinitro-2-methylphenol

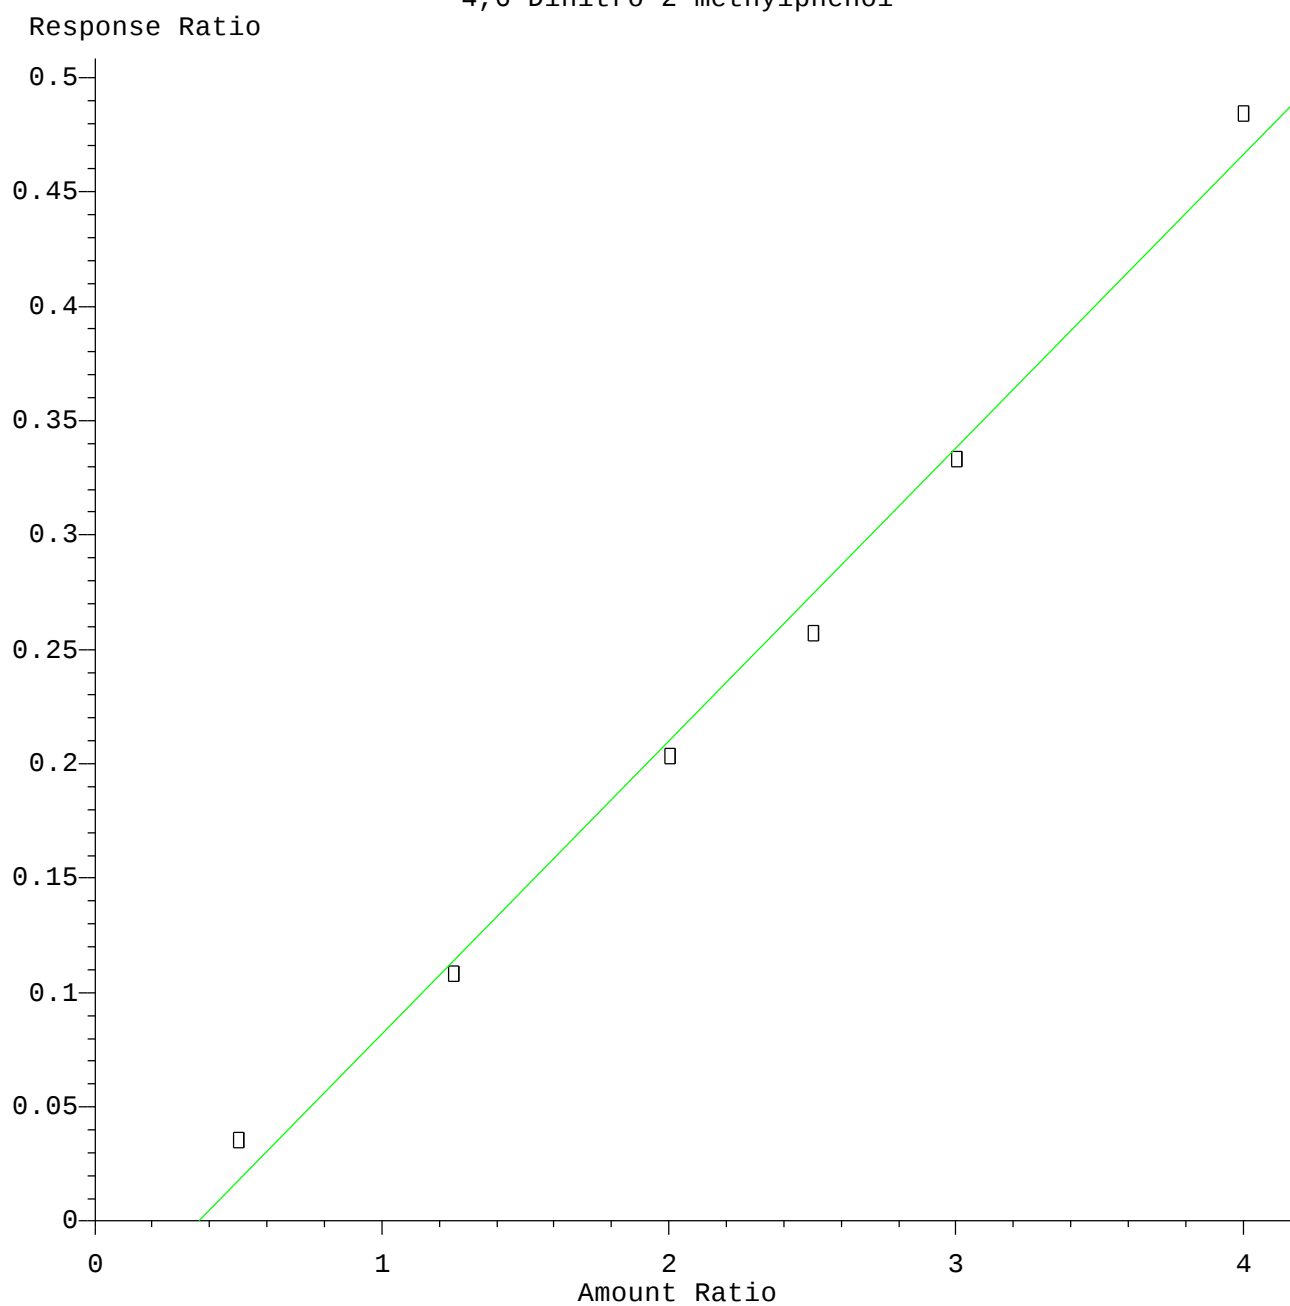

Resp Ratio =  $1.28 \times 10^{-1} \times \text{Amt} - 4.60 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.992    Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA\_G\METHODS\8270-BG061815.M  
Calibration Table Last Updated: Fri Jun 19 06:05:07 2015