
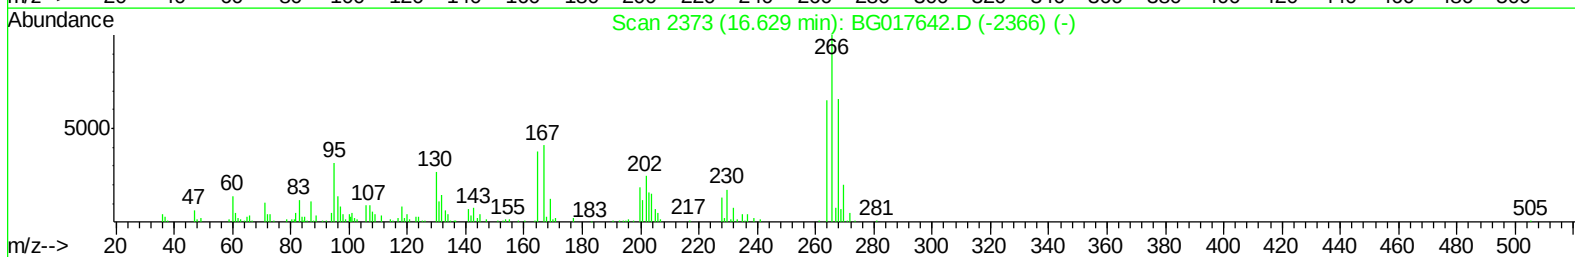
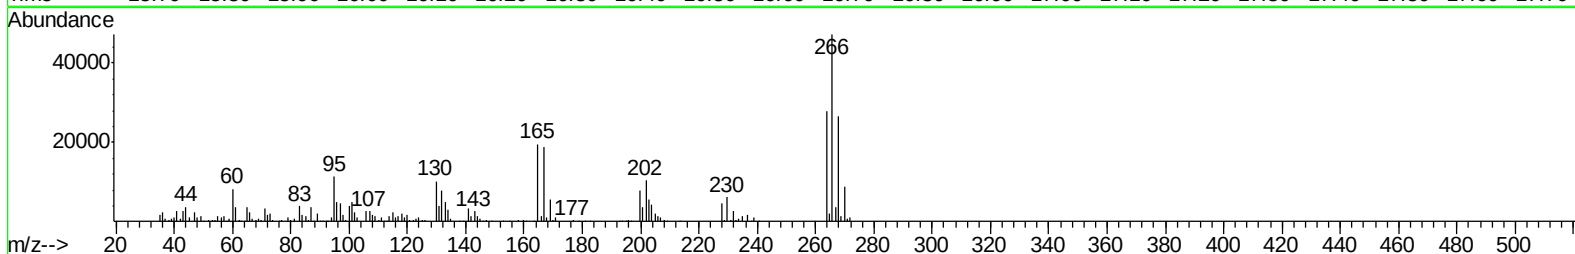


Data Path : Z:\HPCHEM1\BNA_G\Data\BG061815\
Data File : BG017716.D
Acq On : 18 Jun 2015 9:58
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 09:48:32 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 13 02:22:44 2015
Response via : Initial Calibration

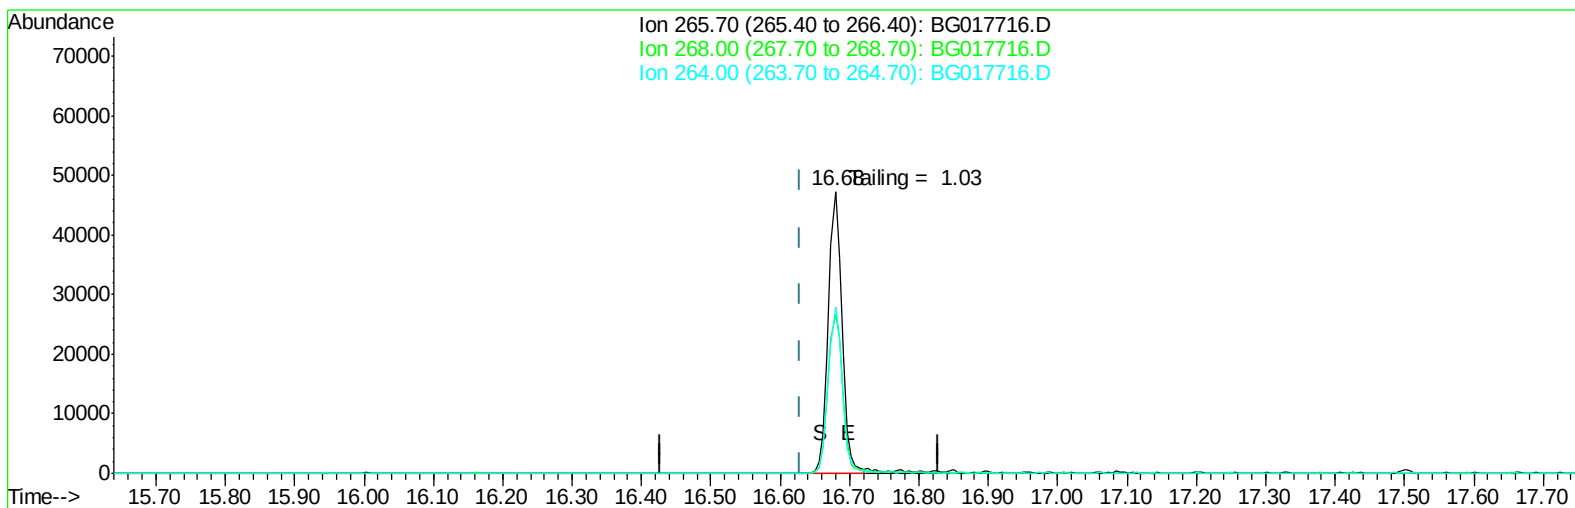

TIC: BG017716.D

(69) Pentachlorophenol (C)




16.679min (+0.050) 0.00ng

response 65337

Ion	Exp%	Act%
265.70	100	100
268.00	65.90	56.23
264.00	65.30	59.18
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG061815\
Data File : BG017716.D
Acq On : 18 Jun 2015 9:58
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 19 09:48:32 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 13 02:22:44 2015
Response via : Initial Calibration

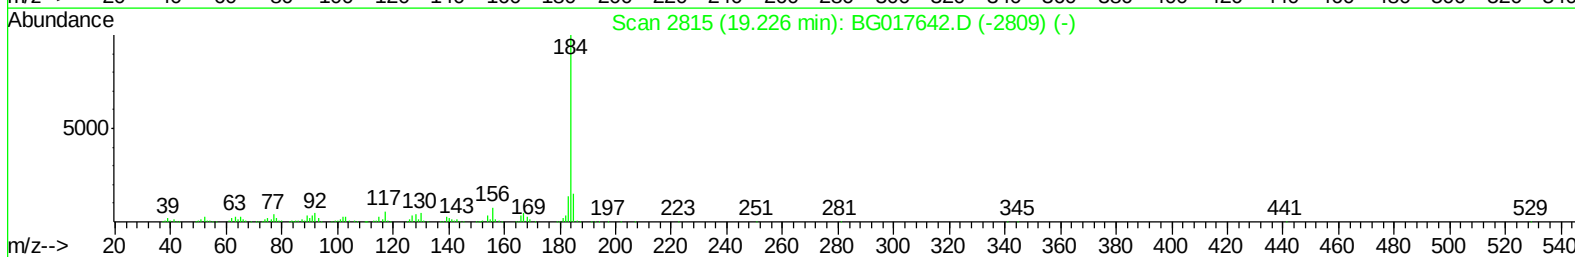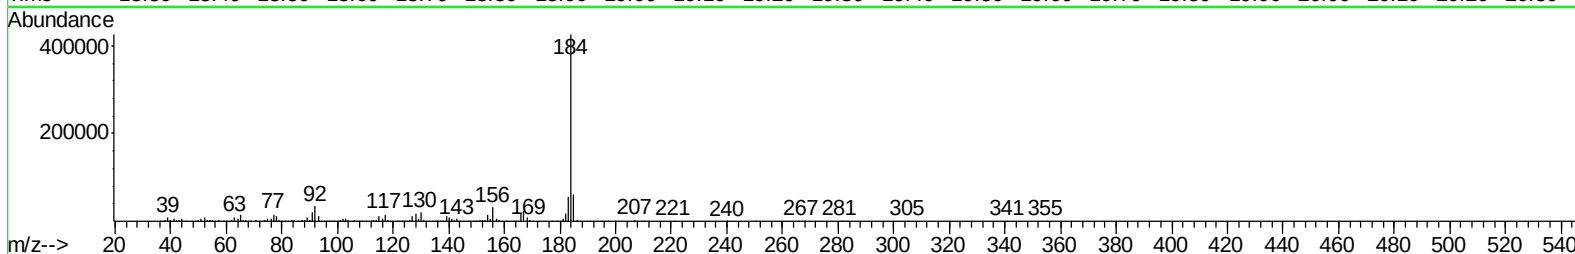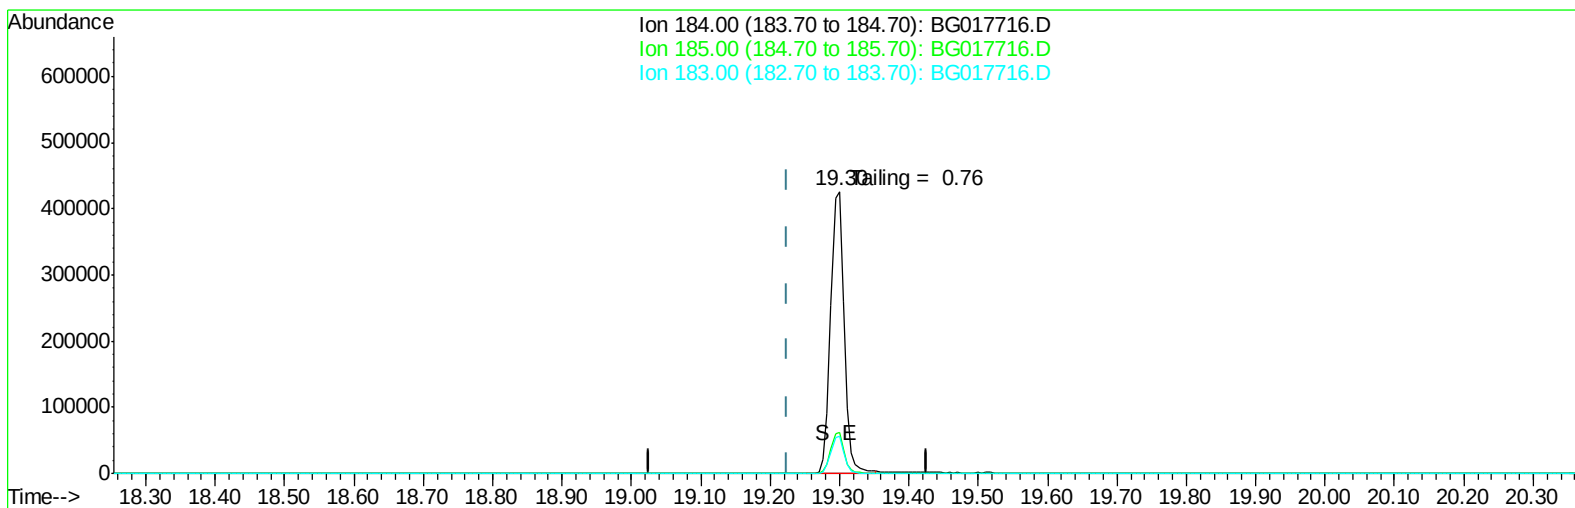

TIC: BG017716.D

(76) Benzidine

19.300min (+0.073) 61432.27ng

response 578563

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.60
183.00	14.00	13.00
0.00	0.00	0.00