


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG061815\
Data File : BG017716.D
Acq On : 18 Jun 2015 9:58
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG061815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 19 06:05:07 2015

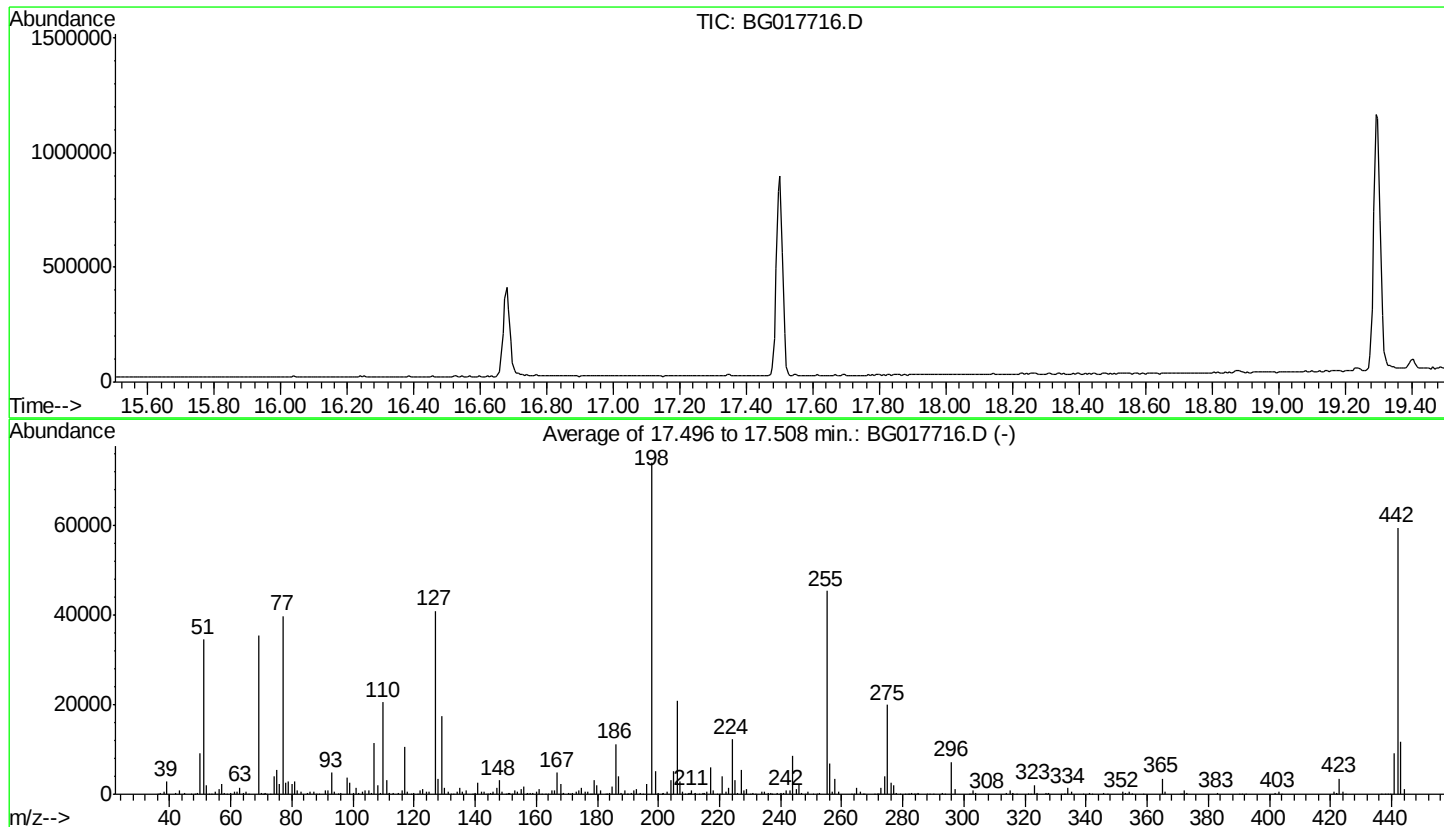

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	34537	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.7	35299	PASS
70	69	0.00	2	1.1	383	PASS
127	198	10	80	55.3	40882	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73960	PASS
199	198	5	9	7.0	5210	PASS
275	198	10	60	26.9	19903	PASS
365	198	1	100	4.7	3456	PASS
441	442	0.01	24	15.5	9239	PASS
442	198	50	100	80.5	59528	PASS
443	442	15	24	19.5	11600	PASS