
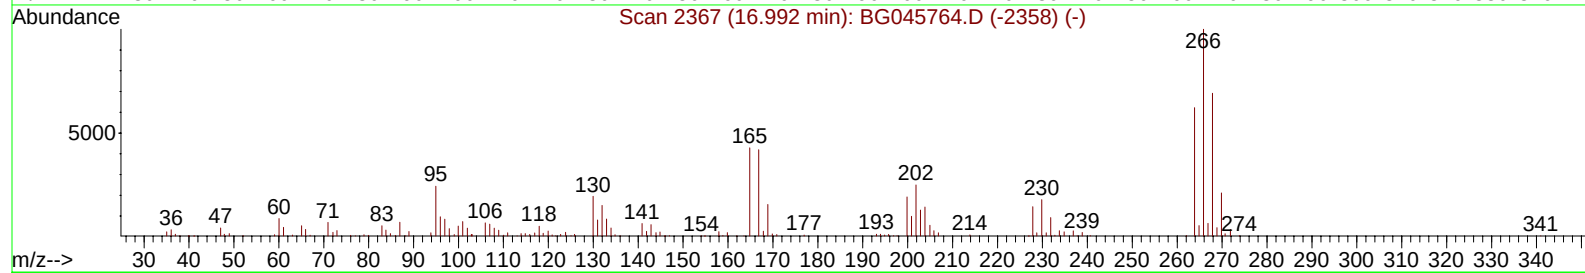
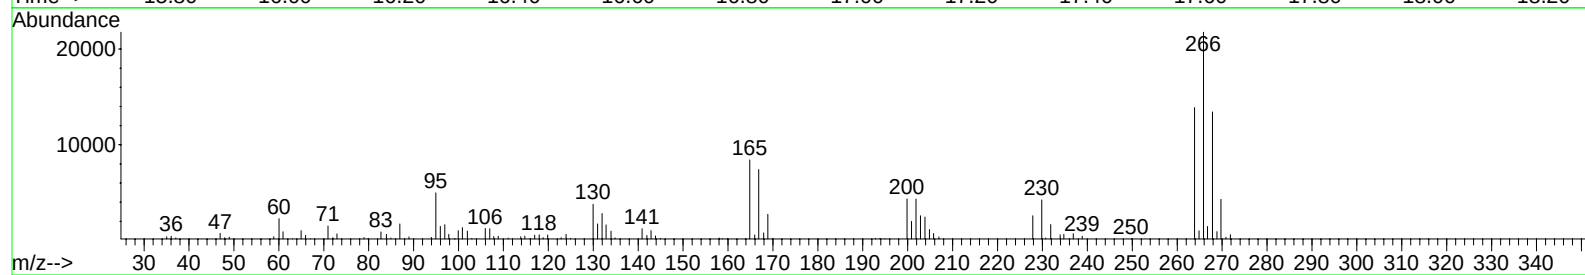


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061820\
 Data File : BG045794.D
 Acq On : 18 Jun 2020 15:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 18:17:45 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 15 18:34:19 2020
 Response via : Initial Calibration

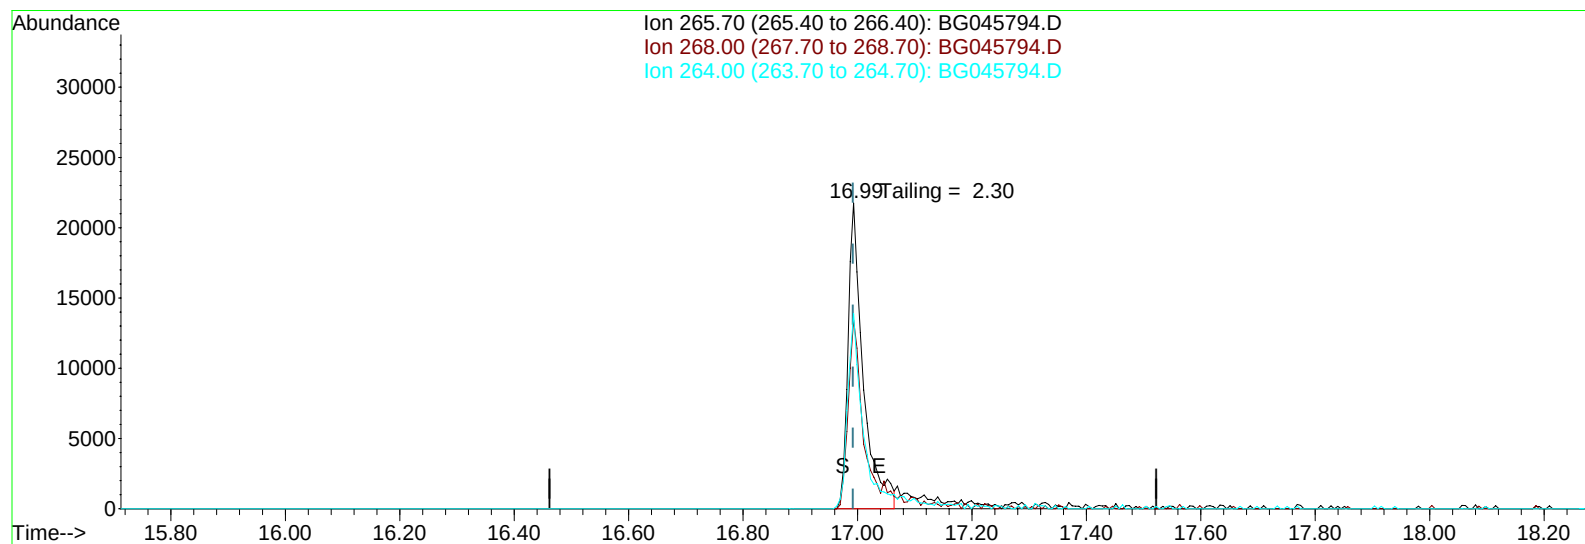

TIC: BG045794.D

(70) Pentachlorophenol (C)




16.993min (+0.001) 24717.96ng

response 38300

Ion	Exp%	Act%
265.70	100	100
268.00	69.20	61.73
264.00	62.20	63.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG061820\
Data File : BG045794.D
Acq On : 18 Jun 2020 15:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 18:17:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG061520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 15 18:34:19 2020
Response via : Initial Calibration

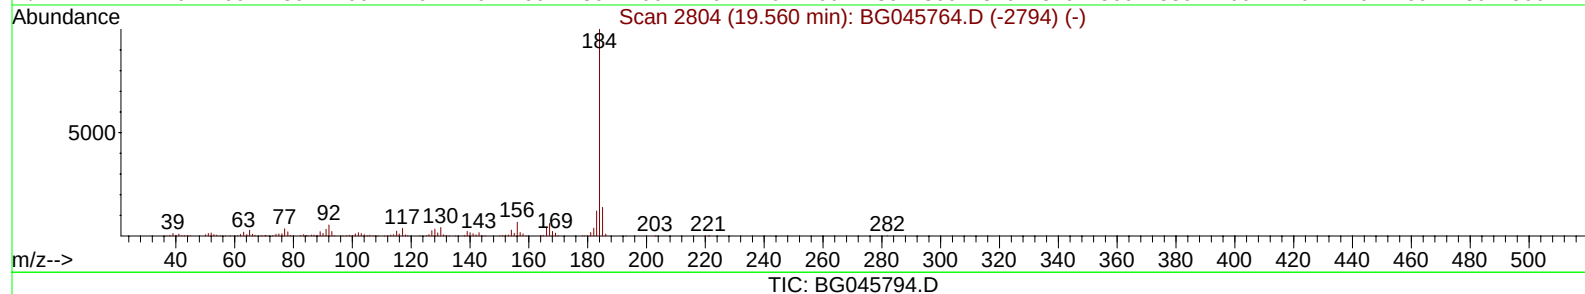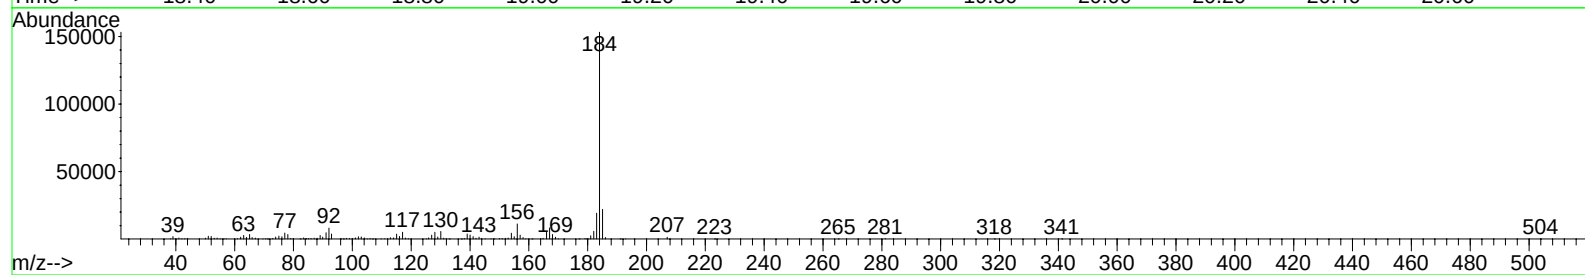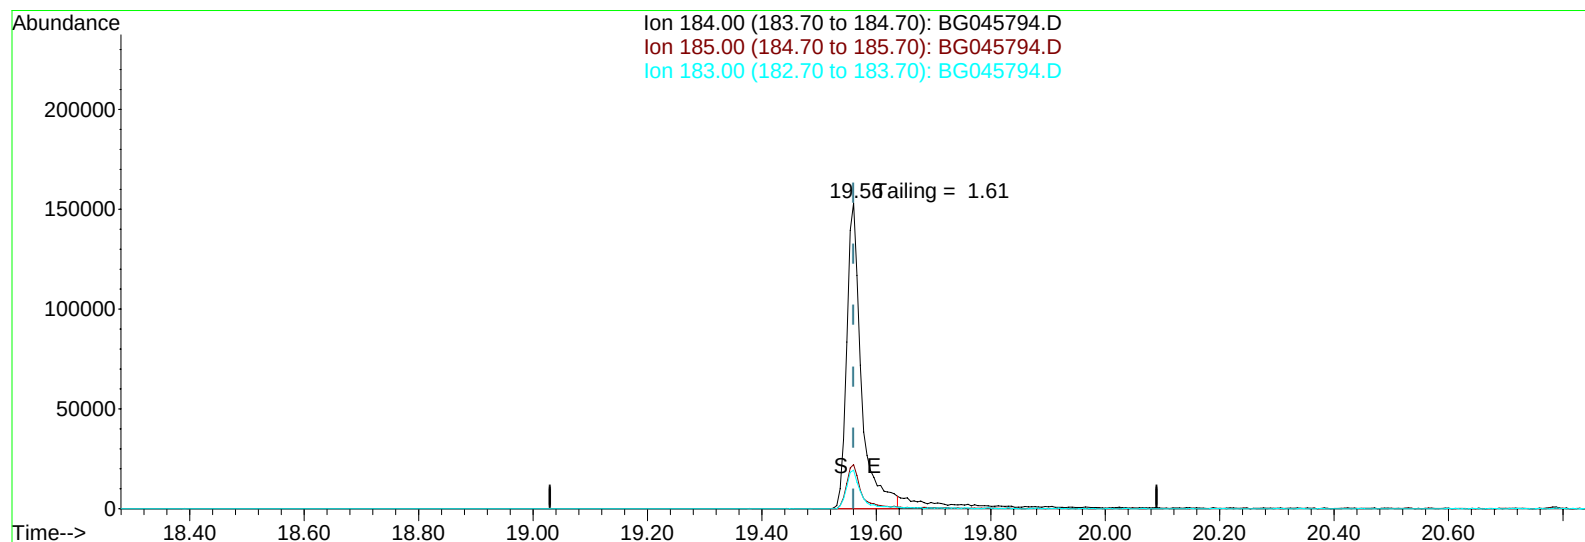

(77) Benzidine

19.560min (+0.001) 154744.76ng

response 285626

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.44
183.00	12.10	12.59
0.00	0.00	0.00