
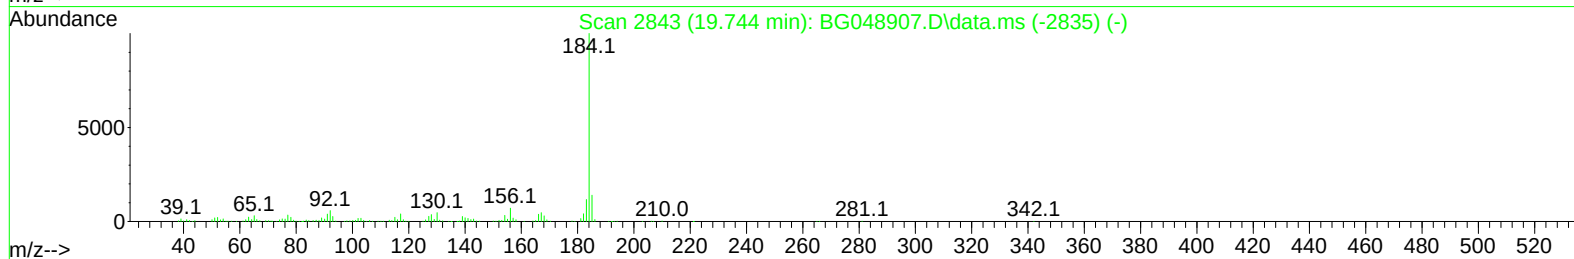
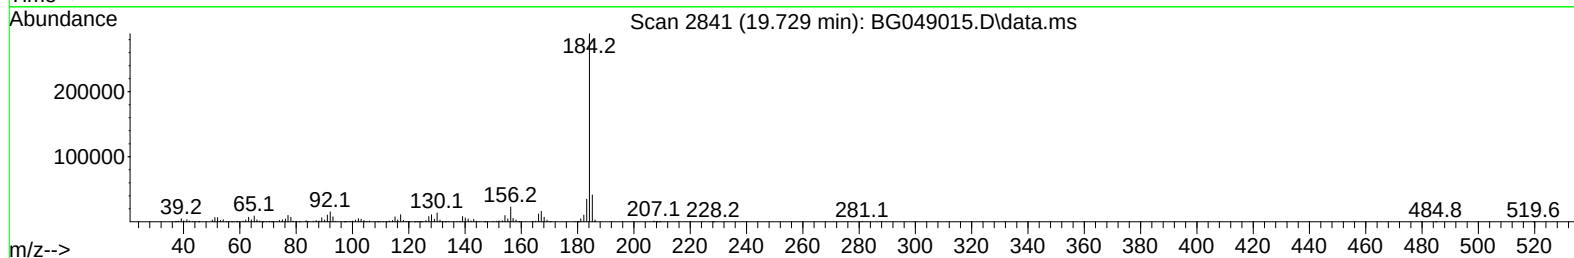


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061821\
Data File : BG049015.D
Acq On : 18 Jun 2021 11:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 12:28:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

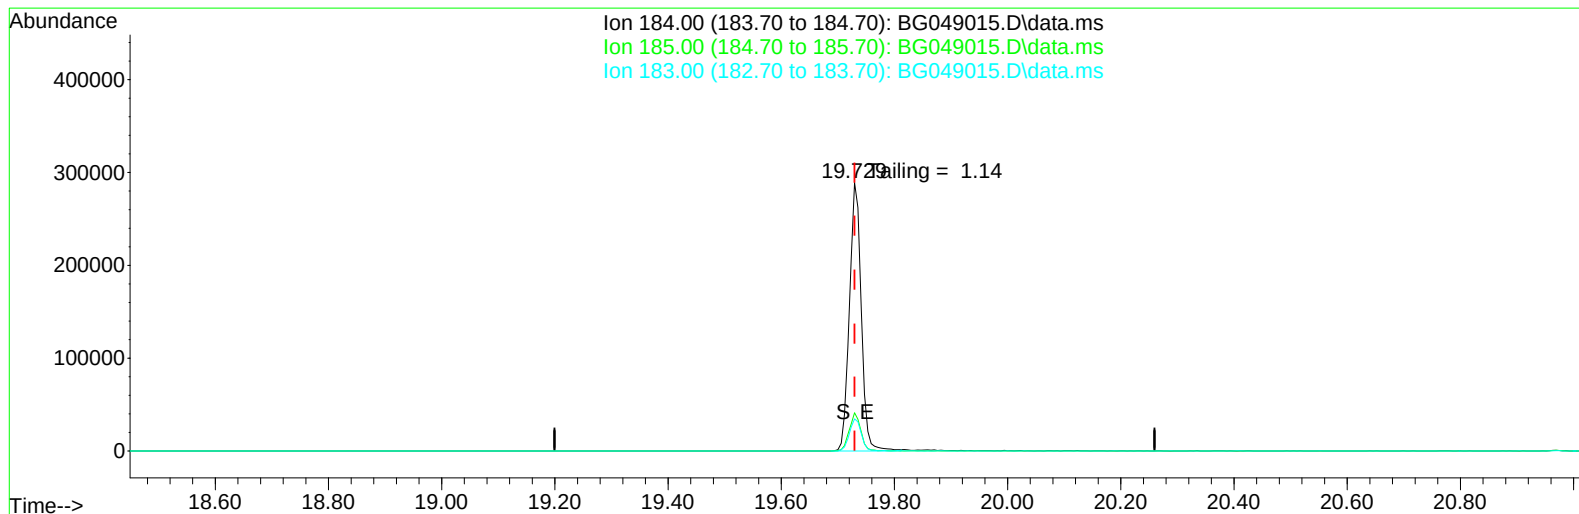




TIC: BG049015.D\data.ms

(77) Benzidine**19.729min (+ 0.000) 247899.75 ng****response 419490**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.28
183.00	11.70	12.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061821\
Data File : BG049015.D
Acq On : 18 Jun 2021 11:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 12:28:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

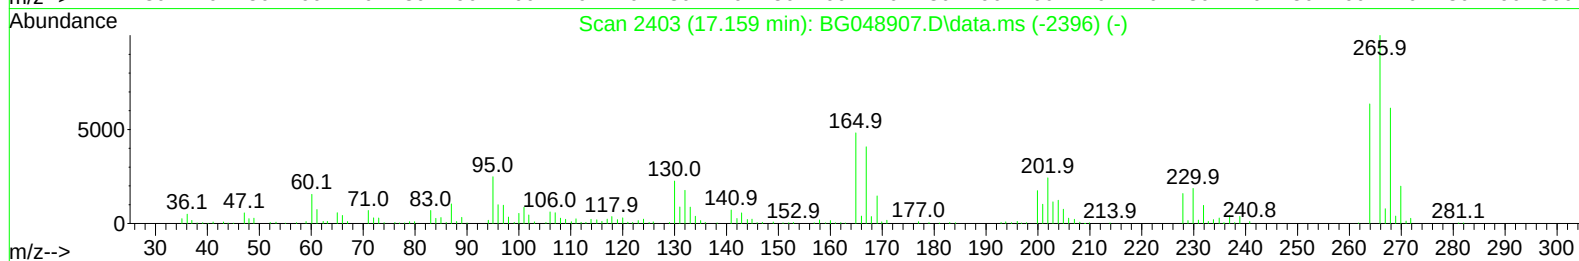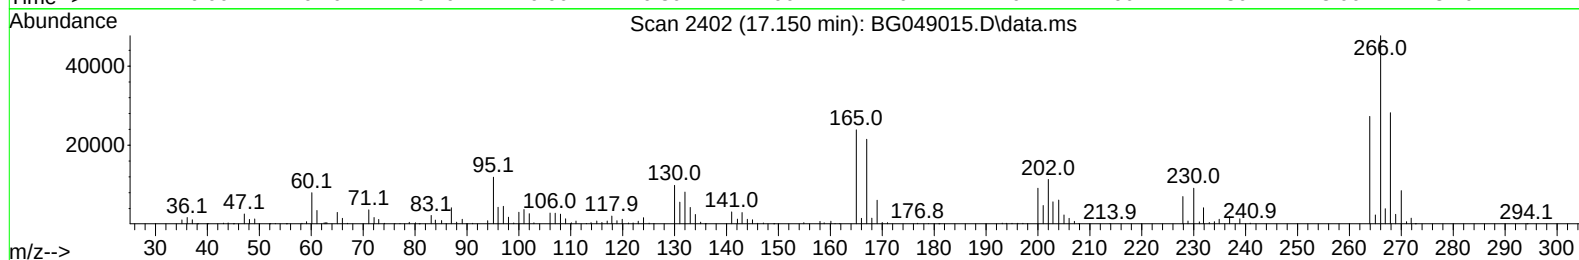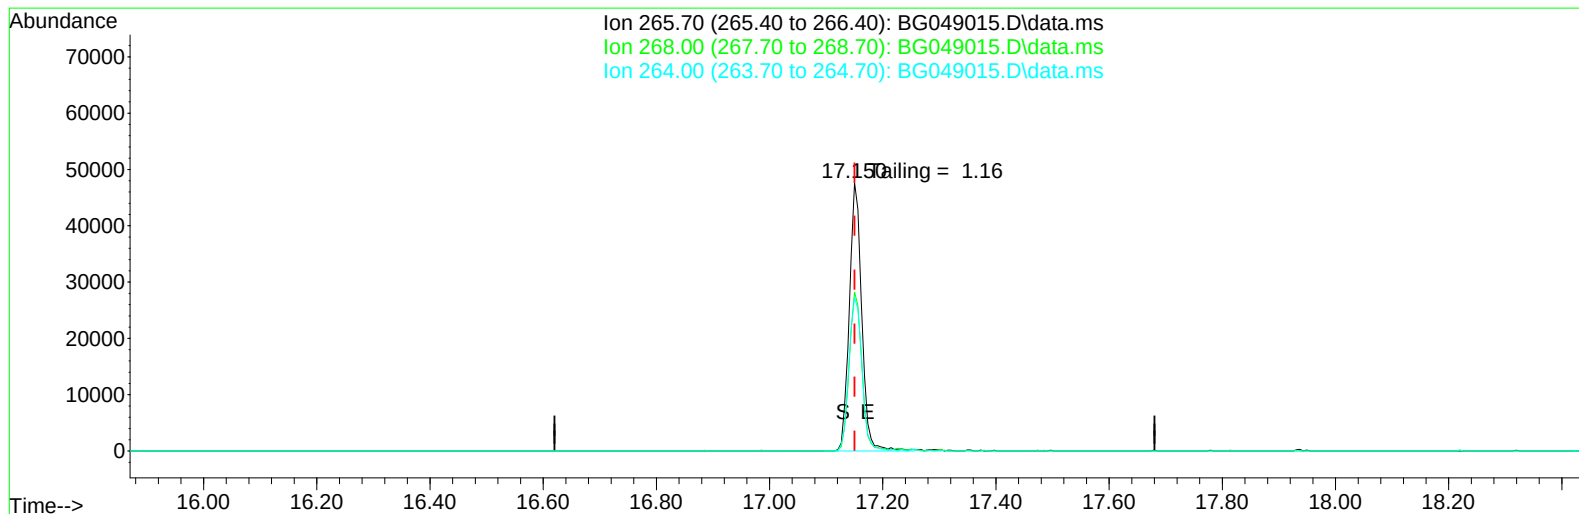

TIC: BG049015.D\data.ms

(70) Pentachlorophenol (C)

17.150min (+ 0.000) 121890.92 ng

response 72369

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	59.20
264.00	61.30	57.25
0.00	0.00	0.00