


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061821\
 Data File : BG049015.D
 Acq On : 18 Jun 2021 11:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 16 12:04:50 2021

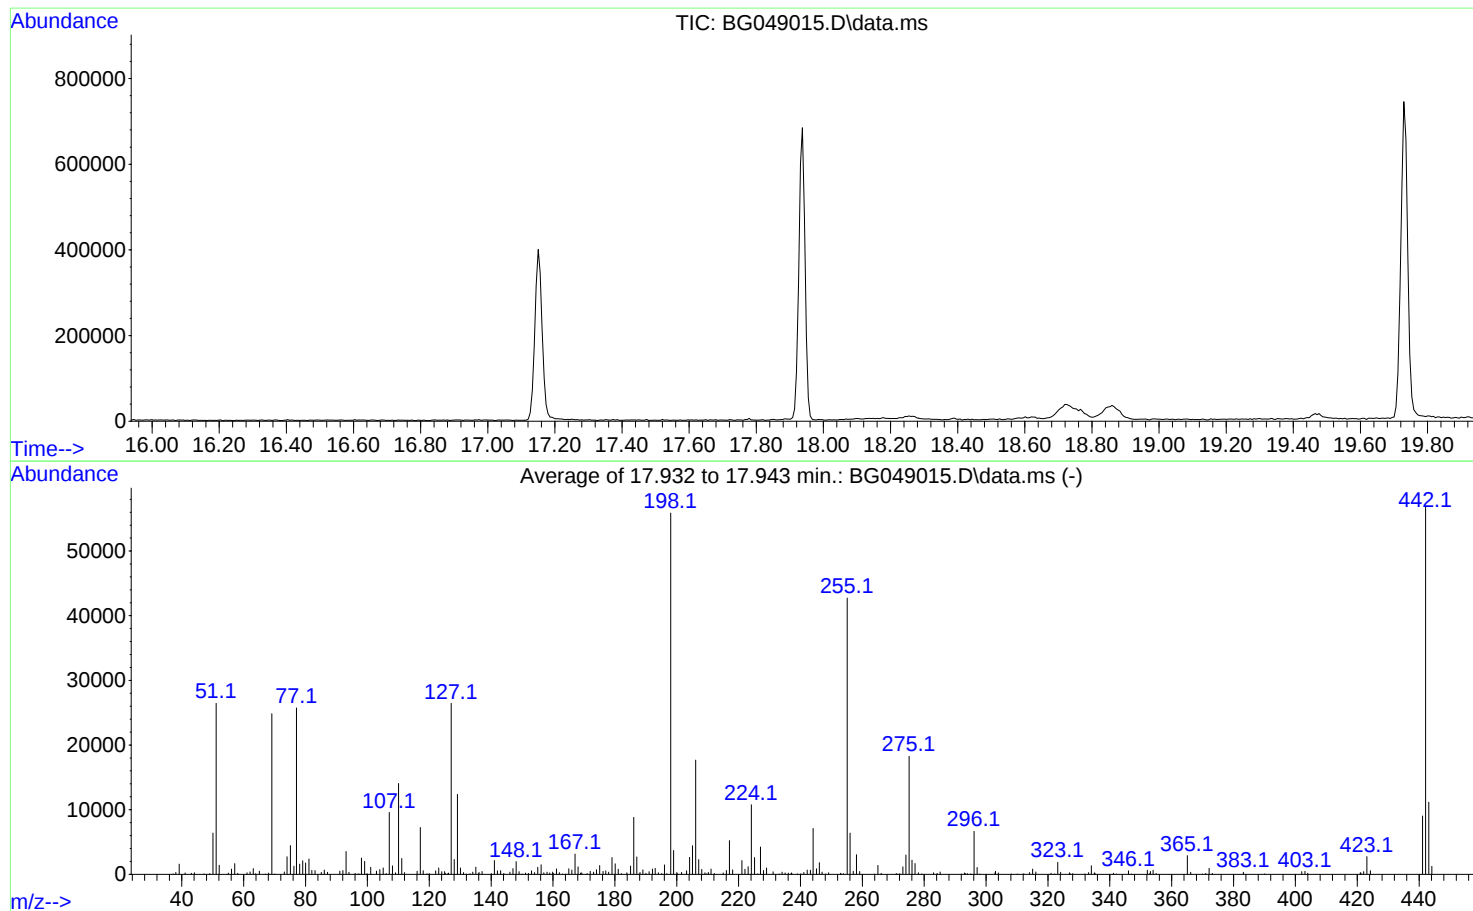




AutoFind: Scans 2535, 2536, 2537; Background Corrected with Scan 2528

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.3	26455	PASS
68	69	0.00	2	0.8	198	PASS
69	198	0.00	100	44.4	24837	PASS
70	69	0.00	2	0.2	51	PASS
127	198	10	80	47.3	26440	PASS
197	198	0.00	2	0.2	103	PASS
198	198	100	100	100.0	55880	PASS
199	198	5	9	6.6	3688	PASS
275	198	10	60	32.7	18264	PASS
365	198	1	100	5.2	2890	PASS
441	198	0.01	100	16.1	9021	PASS
442	442	100	100	100.0	56885	PASS
443	442	15	24	19.6	11168	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061821\
Data File : BG049015.D
Acq On : 18 Jun 2021 11:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 18 12:28:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

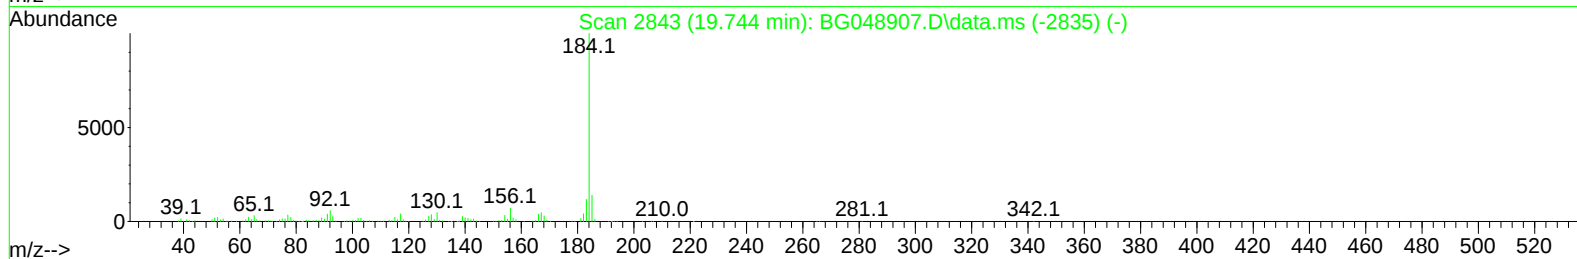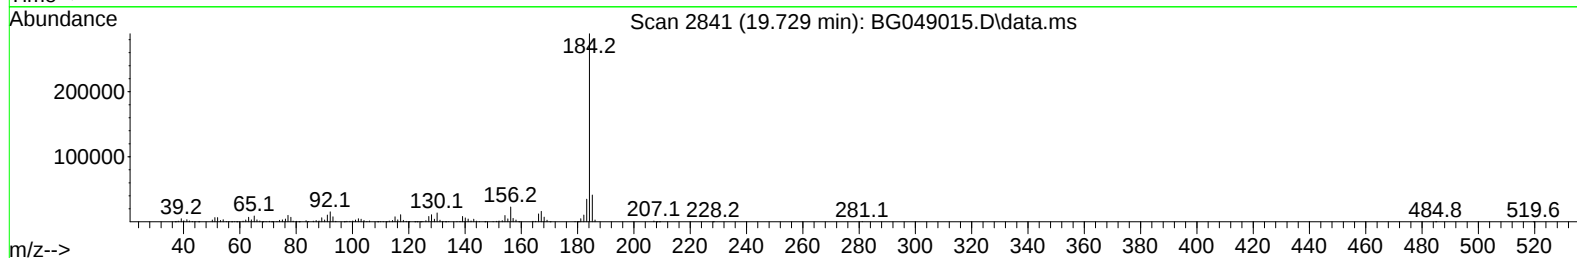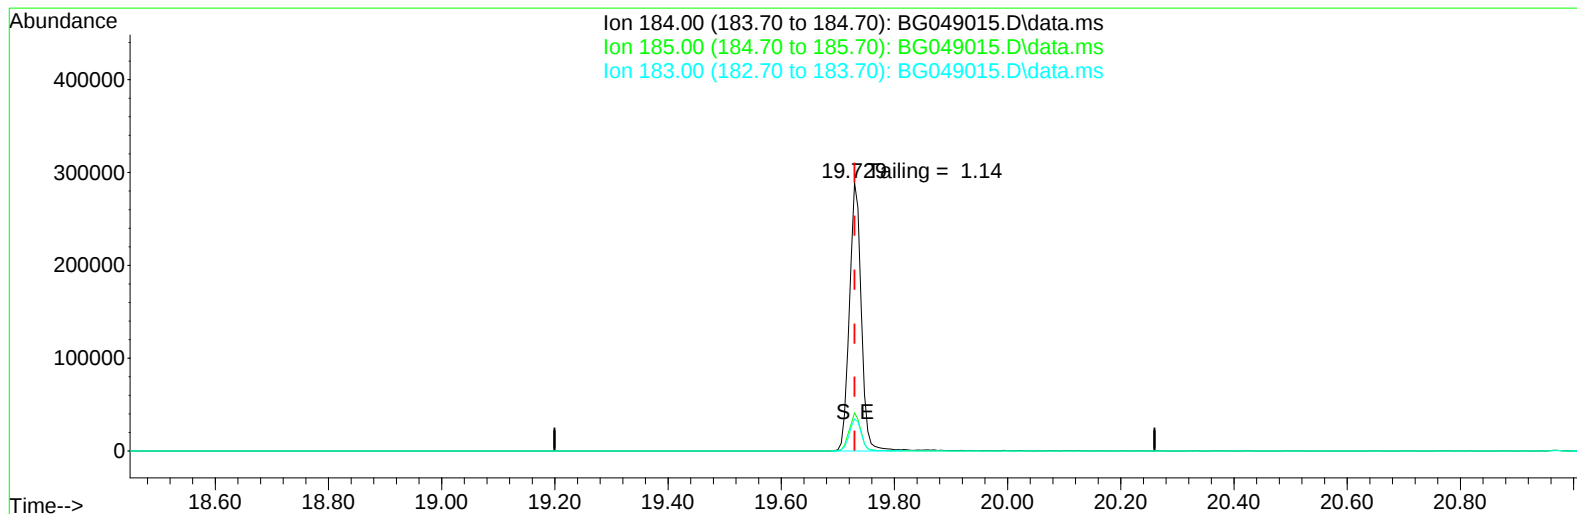

TIC: BG049015.D\data.ms

(77) Benzidine

19.729min (+ 0.000) 247899.75 ng




response 419490

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.28
183.00	11.70	12.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG061821\
Data File : BG049015.D
Acq On : 18 Jun 2021 11:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 18 12:28:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 16 12:04:50 2021
Response via : Initial Calibration

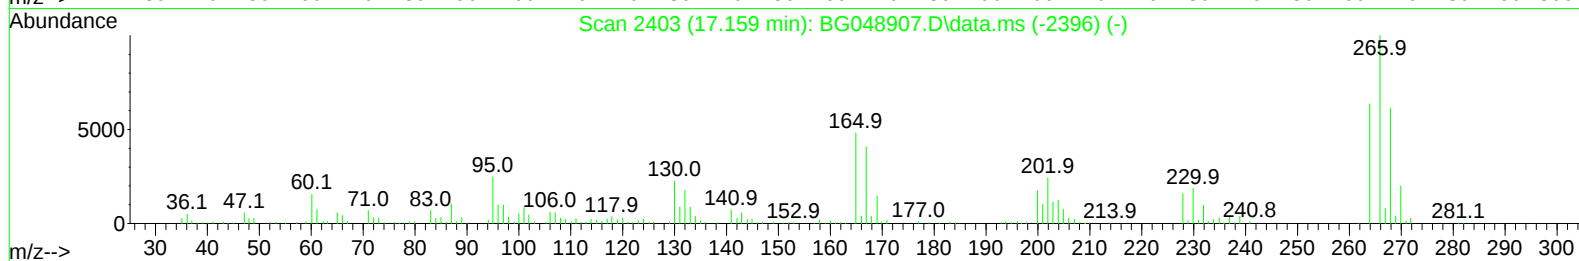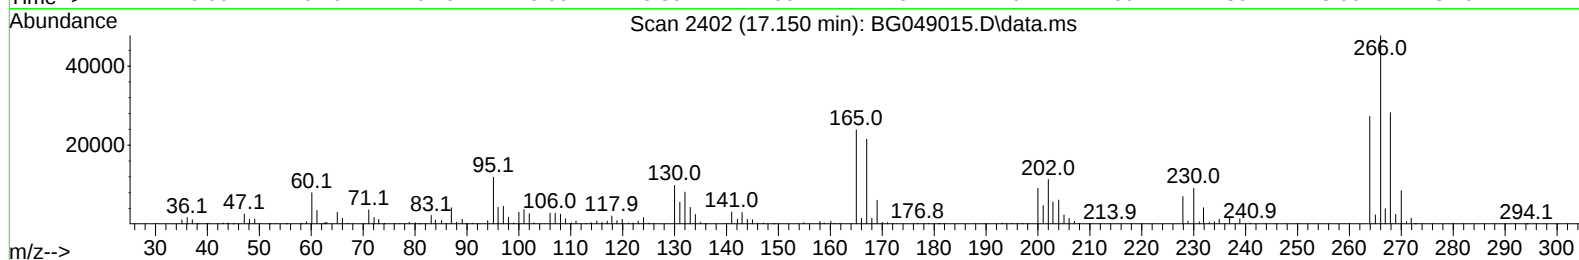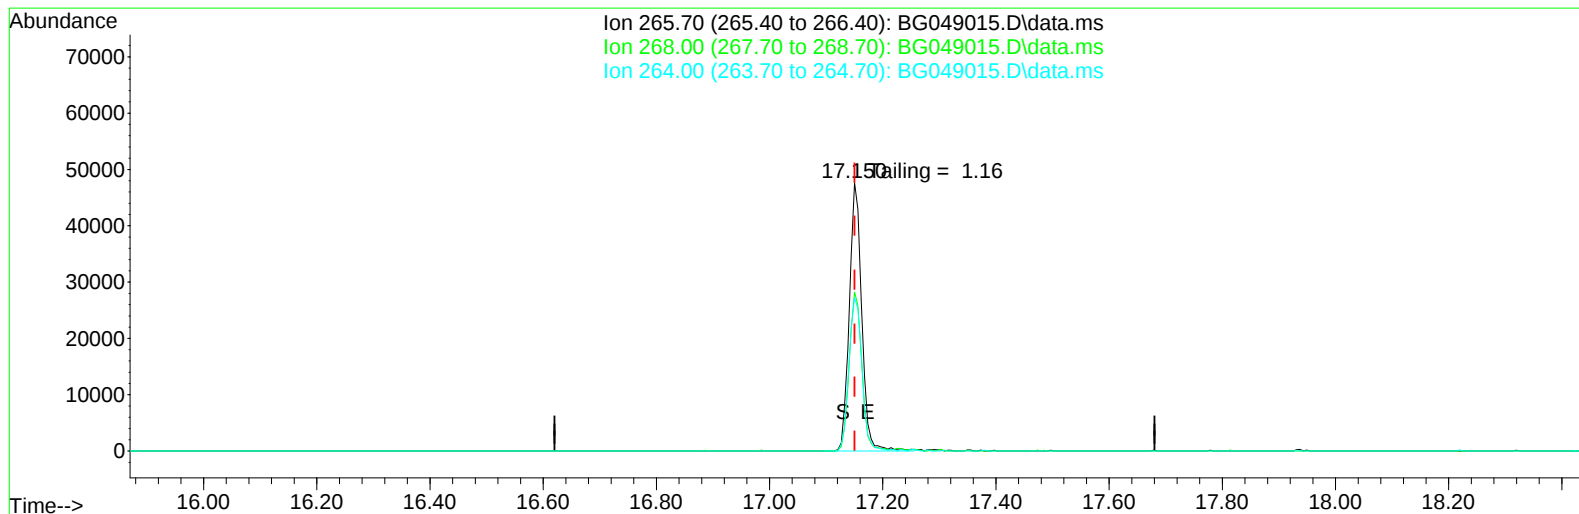

TIC: BG049015.D\data.ms

(70) Pentachlorophenol (C)

17.150min (+ 0.000) 121890.92 ng

response 72369

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	59.20
264.00	61.30	57.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/18/2021	BNA_G	BG049015.D
Compound Name	Response	Retention Time
DDT	209384	20.96
DDD	2436	20.52
DDE	524	20.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2960	212344	1.39